

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
 Data File : BP017461.D
 Acq On : 30 Sep 2023 00:07
 Operator : MA/JU
 Sample : 04497-21
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJ05

Quant Time: Sep 30 00:55:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 29 22:31:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	192099	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.787	136	761001	20.000	ng/ul	-0.02
38) Acenaphthene-d10	14.646	164	457016	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.428	188	1030780	20.000	ng/ul	-0.02
79) Chrysene-d12	21.557	240	1032356	20.000	ng/ul	-0.02
88) Perylene-d12	24.133	264	1168202	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	10320	2.207	ng/uL	0.00
4) Pyridine-d5	3.746	84	35512	2.716	ng/ul	0.01
7) Phenol-d5	7.105	99	117959	7.477	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.293	67	275825	28.969	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.469	132	303802	24.278	ng/ul	-0.01
15) 4-Methylphenol-d8	8.669	113	198612	16.192	ng/ul	-0.02
21) Nitrobenzene-d5	9.158	128	181875	33.059	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.875	143	191560	32.067	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.405	165	329326	29.180	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.957	131	386907	23.666	ng/ul	-0.01
46) Dimethylphthalate-d6	14.057	166	1063763	32.492	ng/ul	-0.01
49) Acenaphthylene-d8	14.340	160	1212717	32.207	ng/ul	-0.02
54) 4-Nitrophenol-d4	14.887	143	31217	5.473	ng/ul	0.00
60) Fluorene-d10	15.645	176	937828	33.273	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.787	200	136819	23.550	ng/ul	-0.02
73) Anthracene-d10	17.534	188	1577347	34.503	ng/ul	-0.01
81) Pyrene-d10	19.781	212	1917165	34.341	ng/ul	-0.02
92) Benzo(a)pyrene-d12	23.963	264	1915947	34.064	ng/ul	-0.02
Target Compounds						
34) Caprolactam	11.804	113	12447	3.871	ng/ul	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017461.D
Acq On : 30 Sep 2023 00:07
Operator : MA/JU
Sample : 04497-21
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ05

Quant Time: Sep 30 00:55:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 29 22:31:03 2023
Response via : Initial Calibration

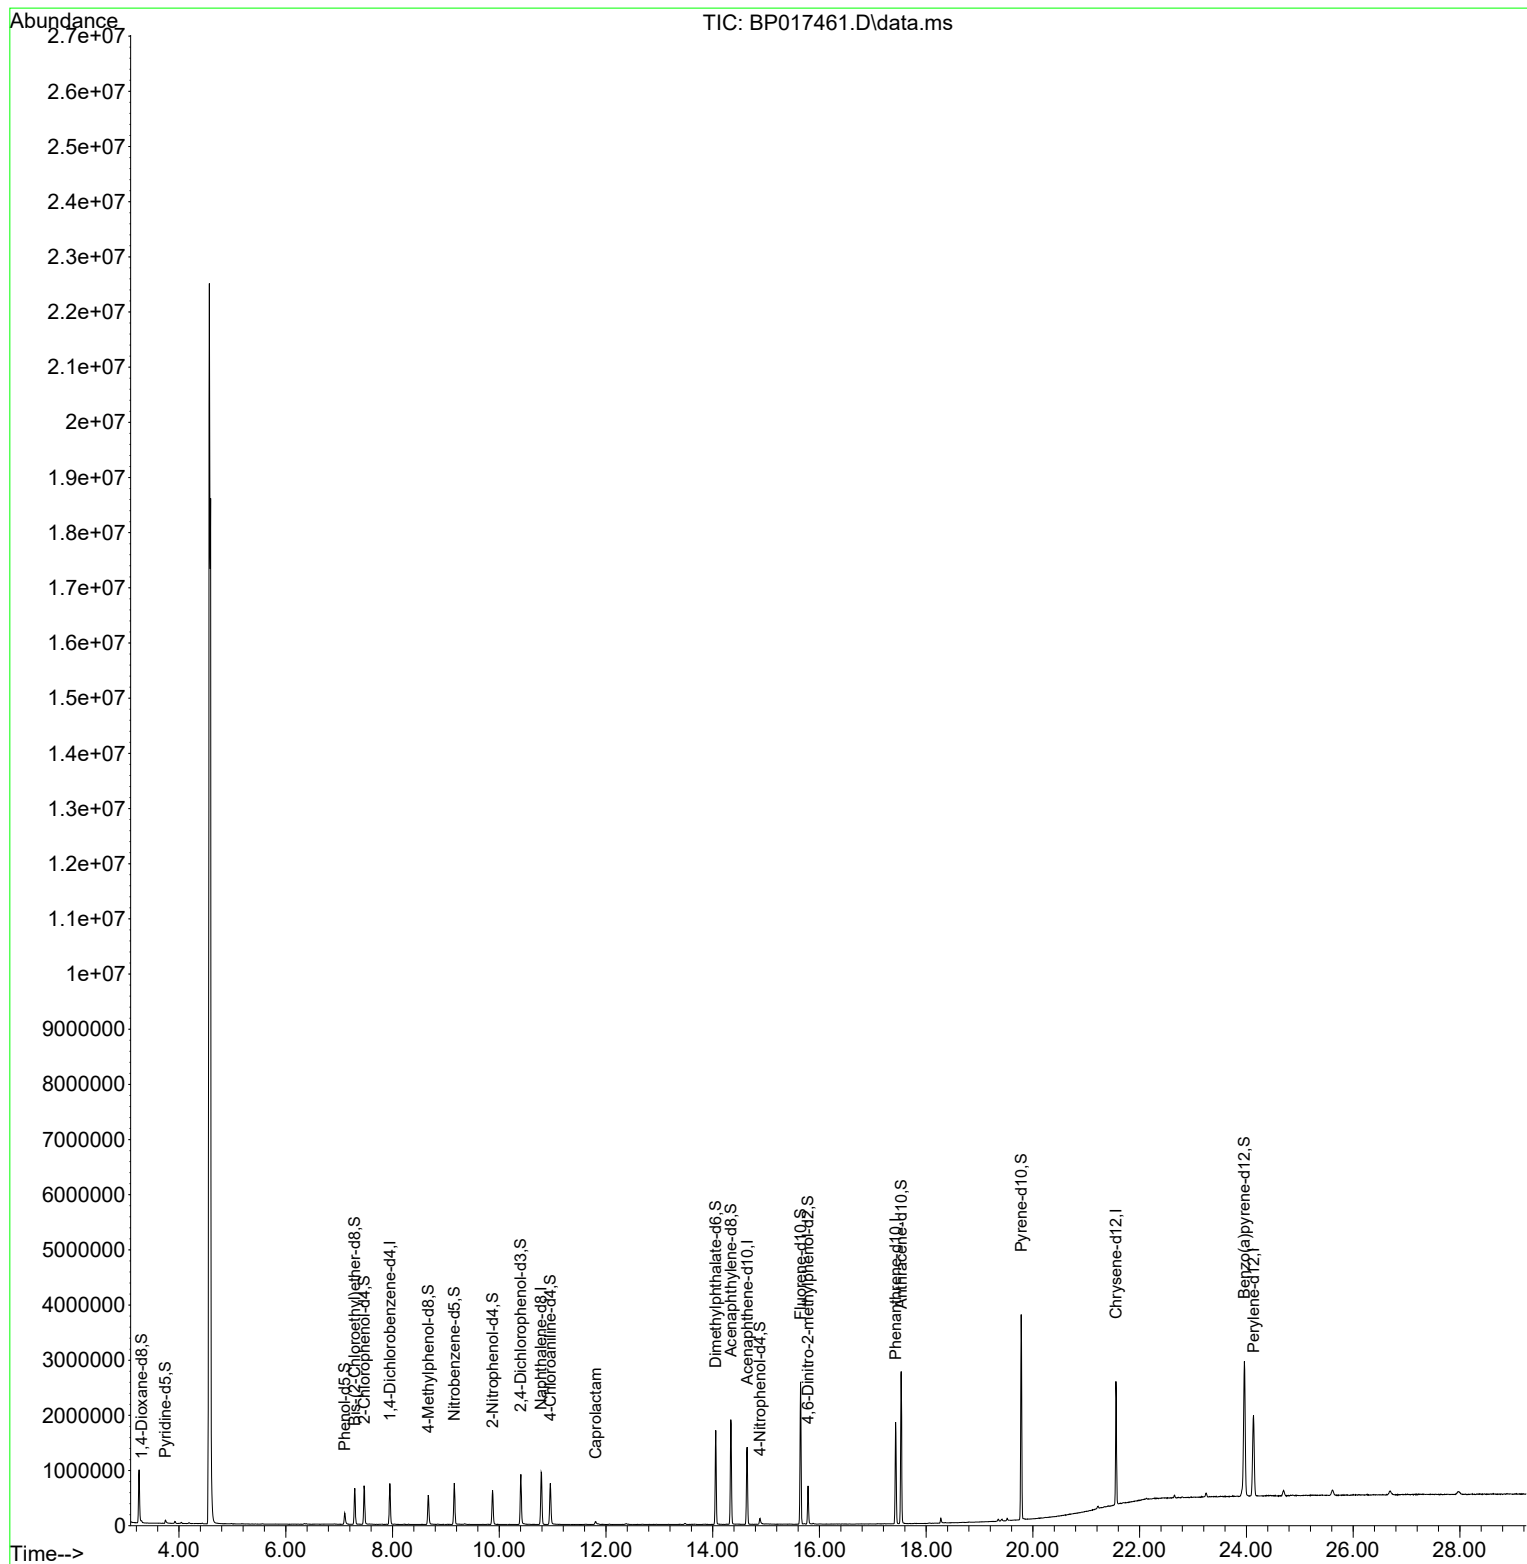

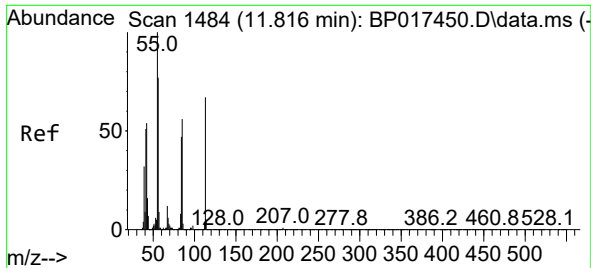

#34
Caprolactam
Concen: 3.871 ng/ul
RT: 11.804 min Scan# 14
Delta R.T. -0.018 min
Lab File: BP017461.D
Acq: 30 Sep 2023 00:07

Instrument :
BNA_P
ClientSampleId :
BBJ05

Tgt Ion	Ratio	Lower	Upper
113	100		
55	165.2	127.4	191.0
56	112.7	94.5	141.7

