

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
 Data File : BP017464.D
 Acq On : 30 Sep 2023 01:49
 Operator : MA/JU
 Sample : 04571-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBK64

Quant Time: Sep 30 02:56:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 29 22:31:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	237894	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.787	136	996040	20.000	ng/ul	-0.02
38) Acenaphthene-d10	14.646	164	645142	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.428	188	1476775	20.000	ng/ul	-0.02
79) Chrysene-d12	21.557	240	1432671	20.000	ng/ul	-0.02
88) Perylene-d12	24.133	264	1607168	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	10219	1.764	ng/uL	0.00
4) Pyridine-d5	3.734	84	138258	8.539	ng/ul	0.00
7) Phenol-d5	7.105	99	121111	6.199	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.293	67	295988	25.103	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.469	132	322753	20.828	ng/ul	-0.01
15) 4-Methylphenol-d8	8.669	113	225220	14.827	ng/ul	-0.02
21) Nitrobenzene-d5	9.158	128	201163	27.936	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.875	143	221562	28.337	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.405	165	381868	25.851	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.957	131	320508	14.978	ng/ul	-0.01
46) Dimethylphthalate-d6	14.057	166	1342221	29.042	ng/ul	-0.01
49) Acenaphthylene-d8	14.340	160	1498926	28.200	ng/ul	-0.02
54) 4-Nitrophenol-d4	14.881	143	38778	4.816	ng/ul	-0.01
60) Fluorene-d10	15.645	176	1170289	29.413	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.787	200	198750	23.878	ng/ul	-0.02
73) Anthracene-d10	17.534	188	1950158	29.775	ng/ul	-0.01
81) Pyrene-d10	19.781	212	2352573	30.366	ng/ul	-0.02
92) Benzo(a)pyrene-d12	23.963	264	2263087	29.246	ng/ul	-0.02
Target Compounds						
					Qvalue	
34) Caprolactam	11.810	113	7434	1.767	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017464.D
Acq On : 30 Sep 2023 01:49
Operator : MA/JU
Sample : 04571-03
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBK64

Quant Time: Sep 30 02:56:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 29 22:31:03 2023
Response via : Initial Calibration

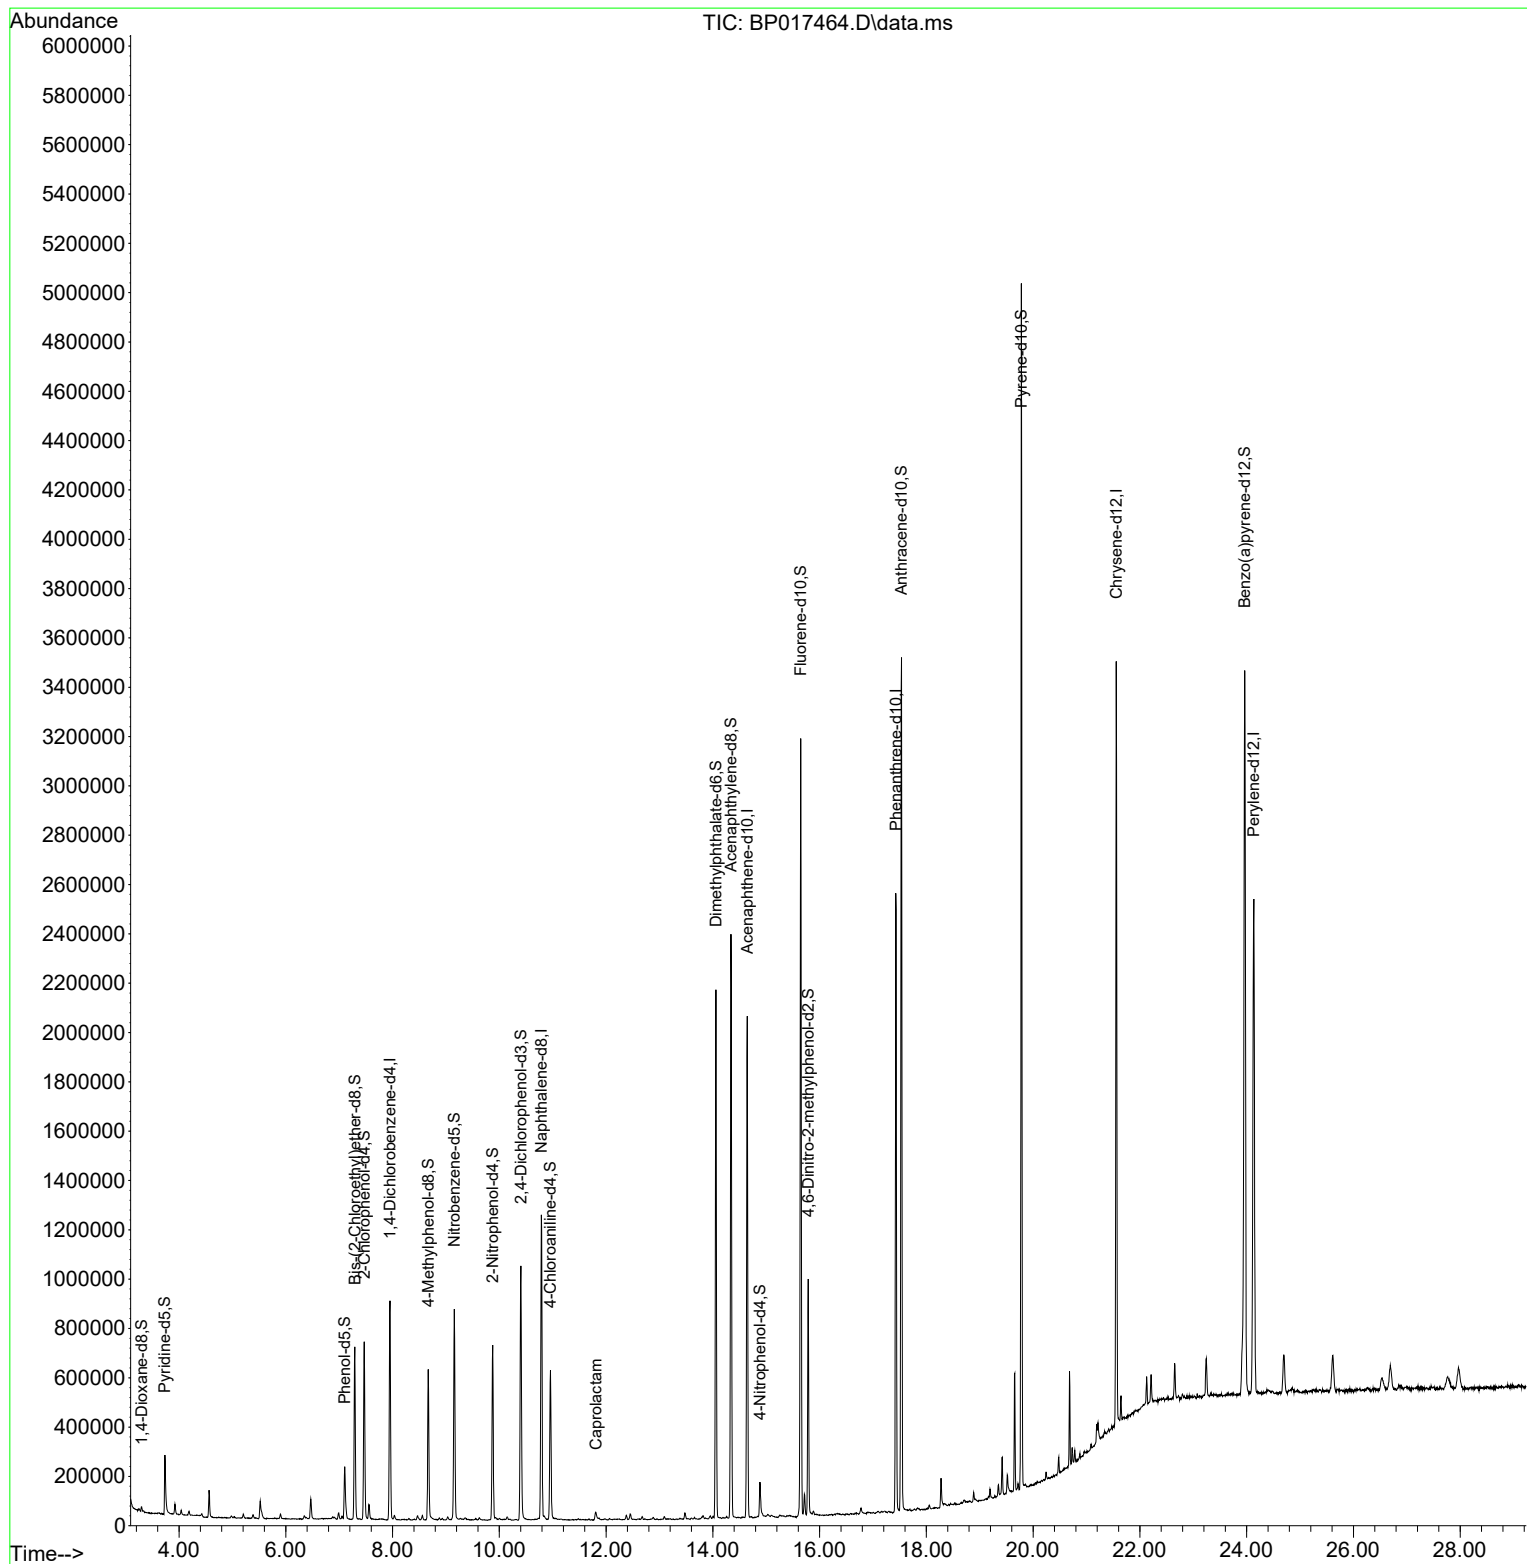

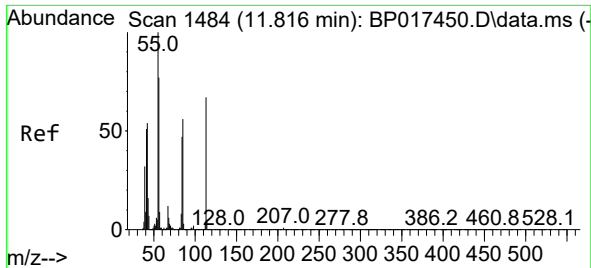

#34

Caprolactam

Concen: 1.767 ng/ul

RT: 11.810 min Scan# 14

Delta R.T. -0.012 min

Lab File: BP017464.D


Acq: 30 Sep 2023 01:49

Instrument :

BNA_P

ClientSampleId :

BBK64

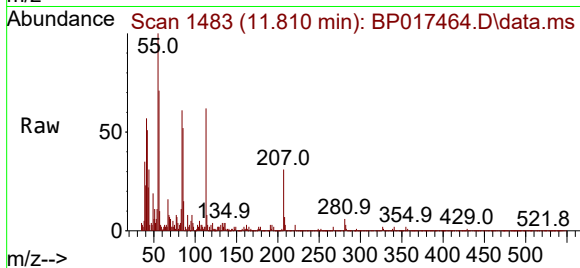

Tgt Ion:113 Resp: 7434

Ion Ratio Lower Upper

113 100

55 160.4 127.4 191.0

56 113.3 94.5 141.7

