

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
 Data File : BP017439.D
 Acq On : 29 Sep 2023 10:41
 Operator : MA/JU
 Sample : PB155862BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK862

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017439.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	33	36	42	rVB	42153	51978	1.35%	0.131%
2	3.740	107	111	129	rBV	485637	735174	19.07%	1.853%
3	4.051	160	164	170	rVB2	11755	18398	0.48%	0.046%
4	7.122	679	686	696	rBV	567082	925241	24.00%	2.333%
5	7.304	711	717	730	rVB	462358	712533	18.48%	1.796%
6	7.487	739	748	757	rBV	592225	961971	24.95%	2.425%
7	7.963	823	829	839	rBV	599427	976906	25.34%	2.463%
8	8.687	945	952	964	rBV	700086	1157325	30.02%	2.918%
9	9.175	1027	1035	1044	rBV	547563	894907	23.21%	2.256%
10	9.892	1148	1157	1169	rBV	457877	761394	19.75%	1.920%
11	10.422	1240	1247	1257	rBV	690191	1193958	30.97%	3.010%
12	10.804	1303	1312	1321	rBV	862988	1404563	36.43%	3.541%
13	10.975	1333	1341	1350	rBV	715897	1199313	31.10%	3.024%
14	12.398	1578	1583	1590	rVB2	11187	19148	0.50%	0.048%
15	13.492	1763	1769	1777	rBV6	13007	22890	0.59%	0.058%
16	14.075	1859	1868	1877	rBV	1214284	1707684	44.29%	4.305%
17	14.357	1909	1916	1930	rVV	1485670	2126782	55.16%	5.362%
18	14.657	1959	1967	1976	rBV	1293800	1920654	49.81%	4.842%
19	14.892	2001	2007	2023	rBV	417247	742959	19.27%	1.873%
20	15.663	2131	2138	2148	rBV	1955536	2669401	69.23%	6.730%
21	15.804	2155	2162	2172	rBV	448616	607523	15.76%	1.532%
22	15.898	2175	2178	2184	rVB6	9784	15467	0.40%	0.039%
23	16.245	2233	2237	2240	rBV6	2936	4338	0.11%	0.011%
24	16.451	2270	2272	2279	rVB8	2560	3987	0.10%	0.010%
25	16.557	2288	2290	2297	rVB8	2712	4830	0.13%	0.012%
26	17.239	2401	2406	2413	rBV8	5489	12063	0.31%	0.030%
27	17.445	2435	2441	2452	rBV	1715223	2433123	63.10%	6.134%
28	17.551	2452	2459	2471	rVV	2188049	3080141	79.89%	7.765%
29	17.921	2518	2522	2524	rBV5	2742	4019	0.10%	0.010%
30	17.980	2530	2532	2535	rBV4	3245	3960	0.10%	0.010%
31	18.086	2547	2550	2553	rBV5	5479	6695	0.17%	0.017%
32	19.362	2765	2767	2772	rVB3	29447	32655	0.85%	0.082%
33	19.439	2777	2780	2783	rVB	21347	26047	0.68%	0.066%
34	19.798	2836	2841	2848	rBV	2931026	3753319	97.34%	9.462%
35	21.580	3139	3144	3149	rBV	1976565	2664030	69.09%	6.716%
36	23.992	3547	3554	3566	rVB2	1898399	3855718	100.00%	9.721%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017439.D
Acq On : 29 Sep 2023 10:41
Operator : MA/JU
Sample : PB155862BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK862

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Title : SVOA CALIBRATION

37	24.162	3577	3583	3593	rVB	1416651	2954471	76.63%	7.448%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 39665565

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017439.D
Acq On : 29 Sep 2023 10:41
Operator : MA/JU
Sample : PB155862BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK862

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

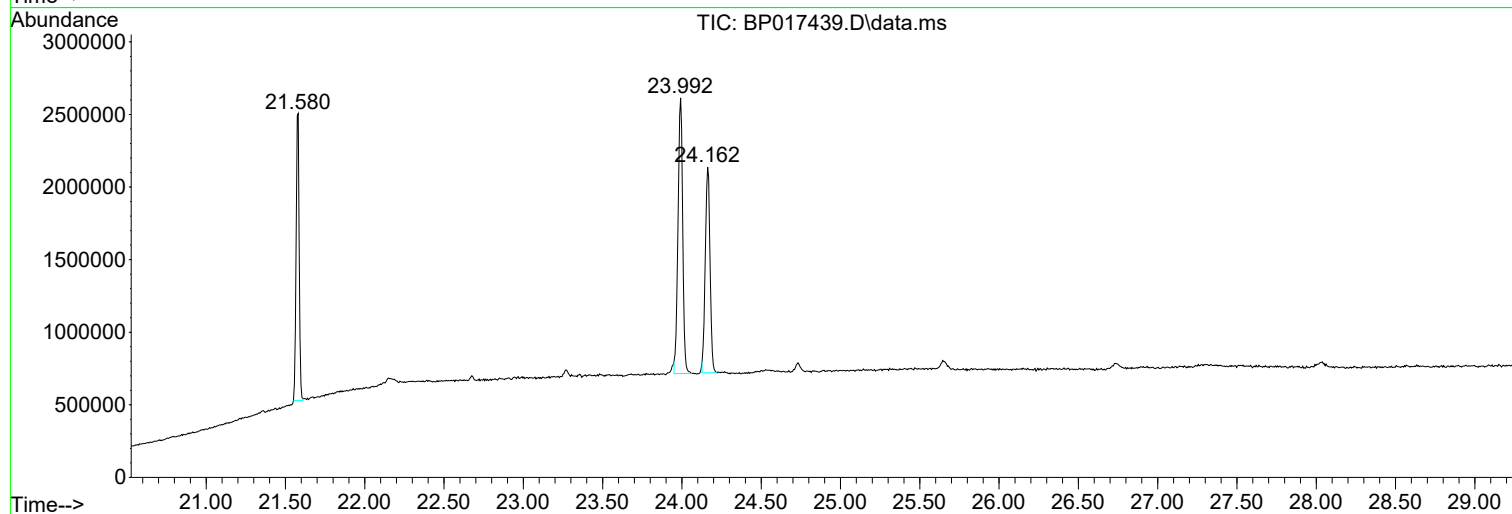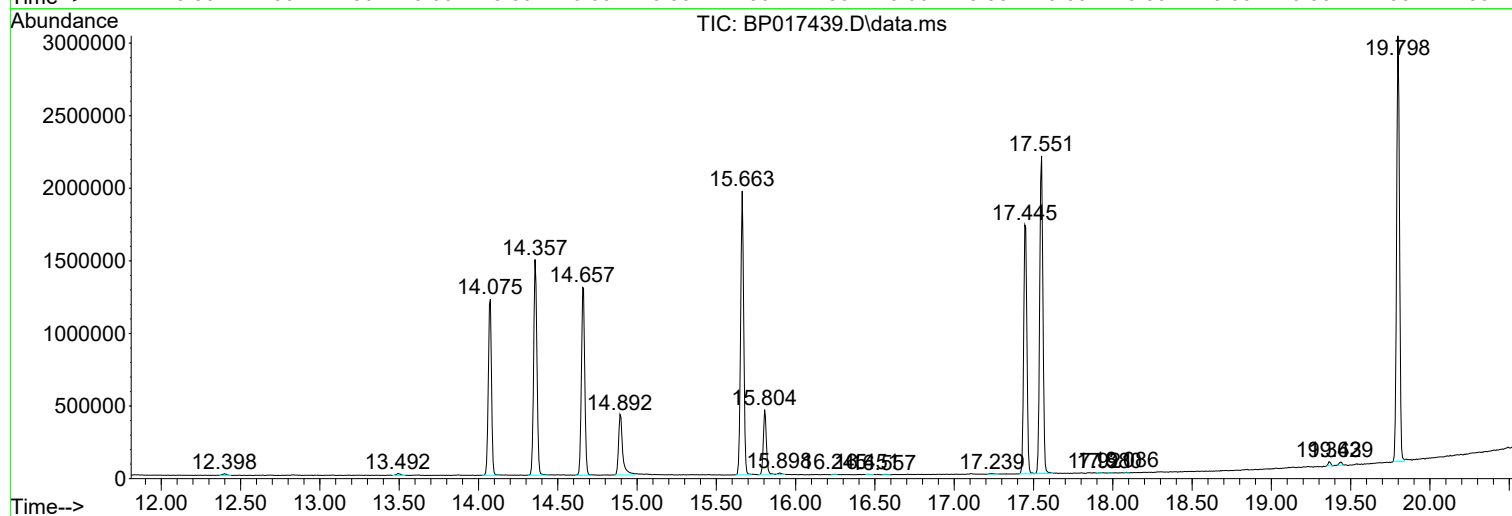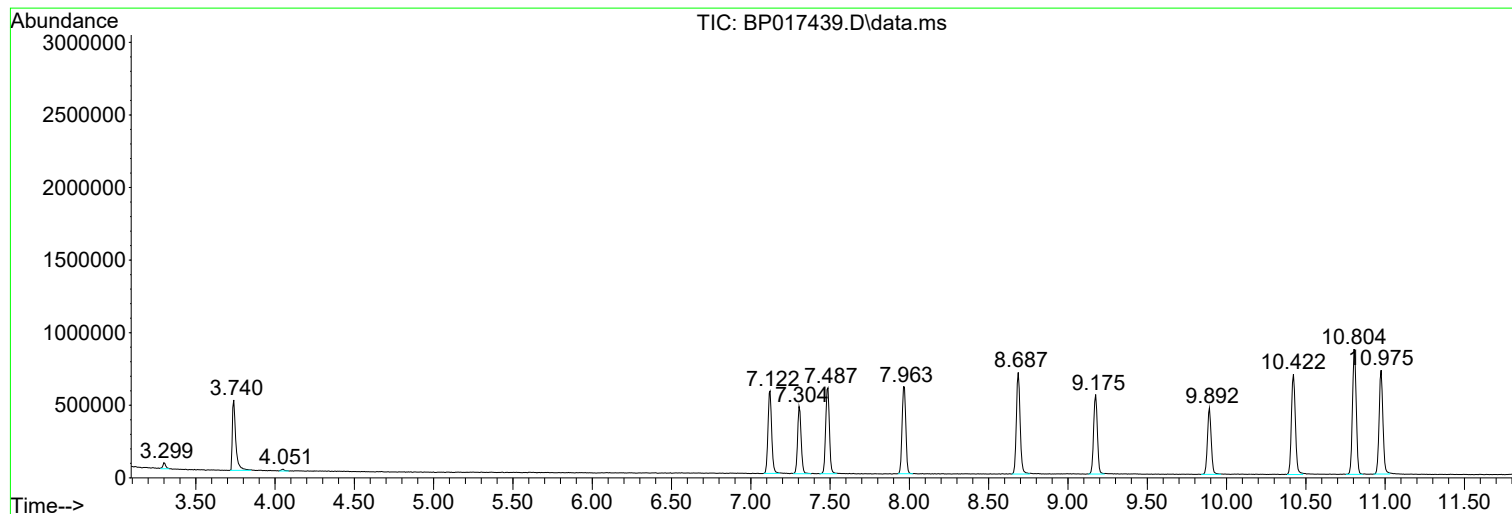

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017439.D
Acq On : 29 Sep 2023 10:41
Operator : MA/JU
Sample : PB155862BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK862

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017439.D
Acq On : 29 Sep 2023 10:41
Operator : MA/JU
Sample : PB155862BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK862

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------