

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
 Data File : BP017444.D
 Acq On : 29 Sep 2023 13:56
 Operator : MA/JU
 Sample : 04497-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017444.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	23	28	34	rBV	677347	881985	2.28%	1.058%
2	3.734	107	110	124	rBV	172896	269512	0.70%	0.323%
3	3.928	137	143	147	rBV	37091	53148	0.14%	0.064%
4	4.569	245	252	255	rBV	21961279	38719336	100.00%	46.437%
5	7.110	678	684	695	rVB	145621	249756	0.65%	0.300%
6	7.293	708	715	727	rBV	598719	947660	2.45%	1.137%
7	7.475	739	746	759	rBV	591535	941025	2.43%	1.129%
8	7.958	821	828	838	rBV	515143	829220	2.14%	0.994%
9	8.675	942	950	961	rBV	427426	708811	1.83%	0.850%
10	9.163	1025	1033	1041	rBV	733671	1188662	3.07%	1.426%
11	9.881	1148	1155	1162	rBV	575475	947509	2.45%	1.136%
12	10.410	1237	1245	1258	rBV	805054	1398638	3.61%	1.677%
13	10.793	1303	1310	1320	rBV	683609	1137841	2.94%	1.365%
14	10.963	1331	1339	1356	rBV	759332	1304949	3.37%	1.565%
15	11.804	1473	1482	1490	rBV	151551	301519	0.78%	0.362%
16	14.063	1859	1866	1875	rBV	1672236	2271795	5.87%	2.725%
17	14.345	1907	1914	1925	rBV	1925548	2792745	7.21%	3.349%
18	14.651	1958	1966	1973	rBV	1007032	1477632	3.82%	1.772%
19	14.887	2001	2006	2017	rBV	89412	185063	0.48%	0.222%
20	15.651	2129	2136	2143	rBV	2568296	3589658	9.27%	4.305%
21	15.722	2144	2148	2154	rVV4	25431	40806	0.11%	0.049%
22	15.792	2154	2160	2169	rVV	755440	976669	2.52%	1.171%
23	17.433	2433	2439	2447	rBV	1307124	1876832	4.85%	2.251%
24	17.539	2450	2457	2470	rVV	3040737	4295533	11.09%	5.152%
25	18.280	2579	2583	2591	rBV	103143	151195	0.39%	0.181%
26	19.357	2762	2766	2770	rBV2	41193	53122	0.14%	0.064%
27	19.427	2774	2778	2782	rVB	37225	52049	0.13%	0.062%
28	19.522	2791	2794	2800	rBV3	60650	84555	0.22%	0.101%
29	19.786	2834	2839	2847	rBV	4111868	5372864	13.88%	6.444%
30	21.569	3137	3142	3147	rBV	1640033	2205811	5.70%	2.645%
31	23.974	3544	3551	3563	rVB2	2683649	5642965	14.57%	6.768%
32	24.145	3574	3580	3590	rVB	1165190	2432049	6.28%	2.917%




Sum of corrected areas: 83380914

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017444.D
Acq On : 29 Sep 2023 13:56
Operator : MA/JU
Sample : 04497-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJC4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

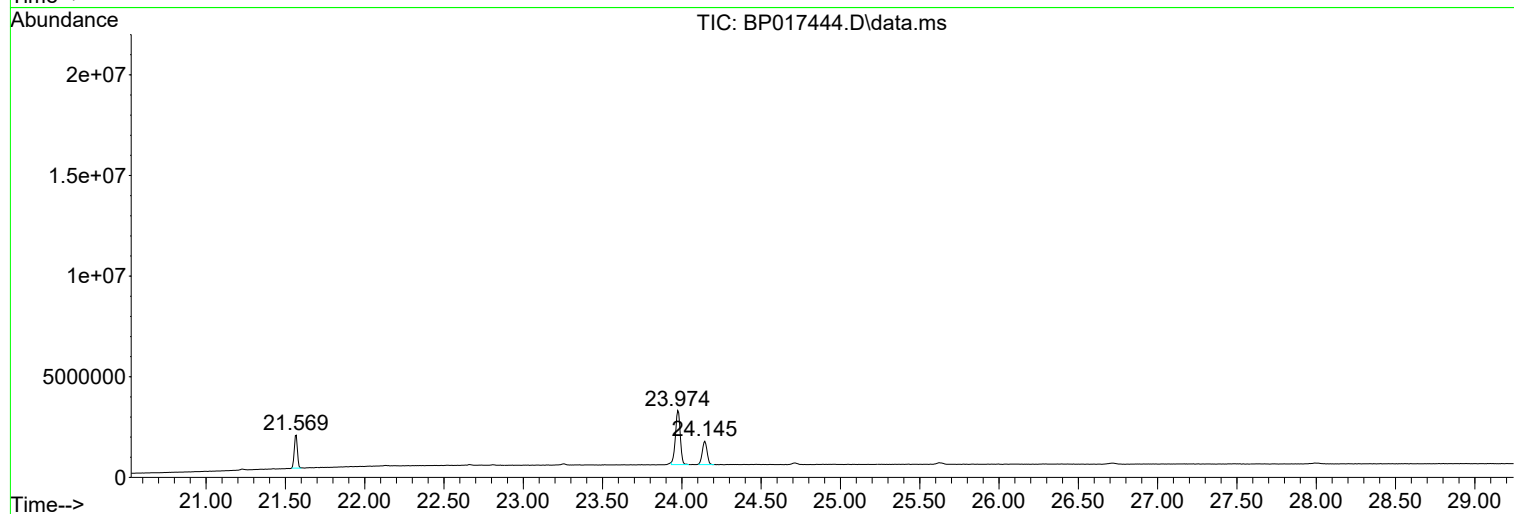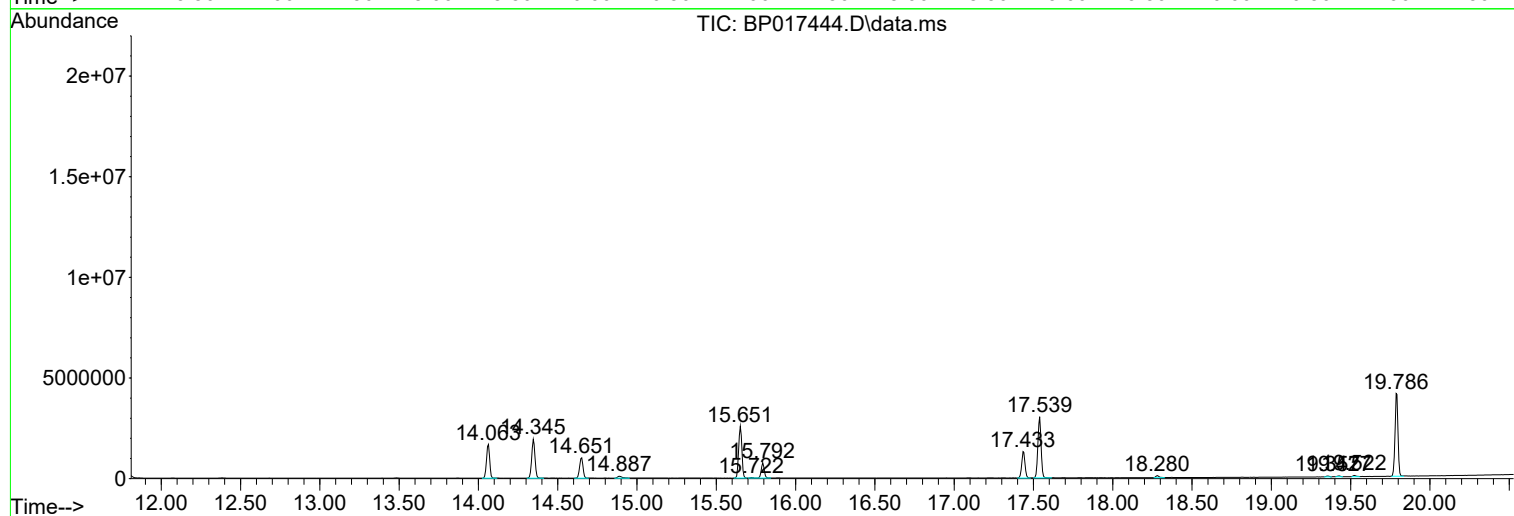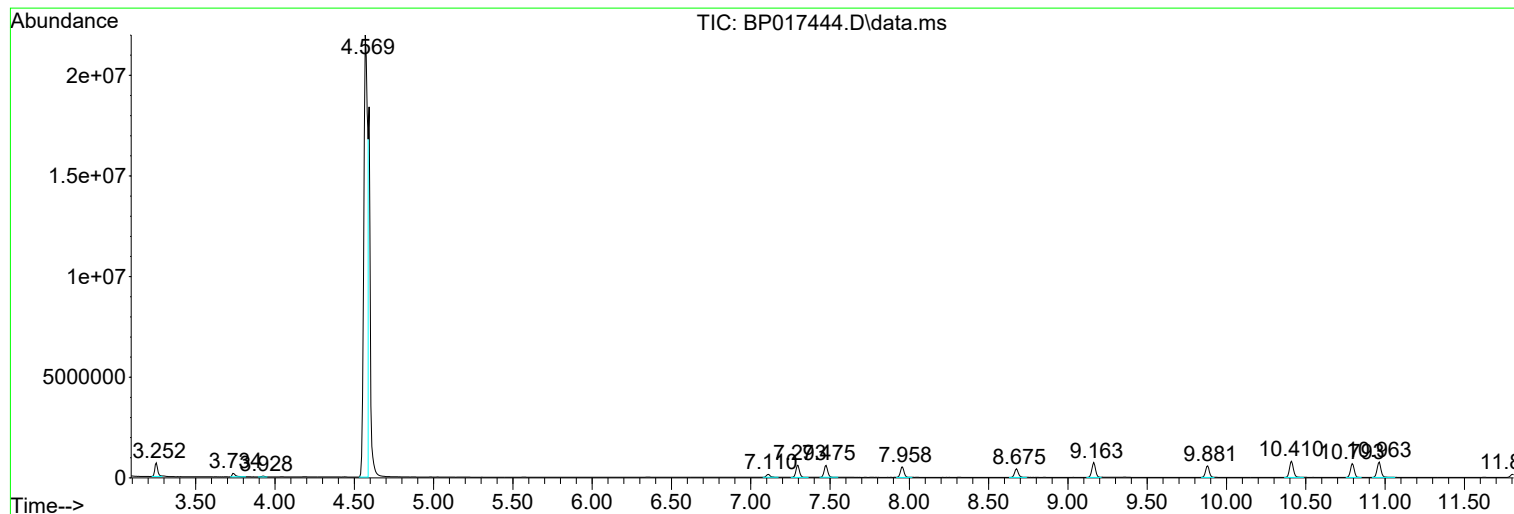

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017444.D
Acq On : 29 Sep 2023 13:56
Operator : MA/JU
Sample : 04497-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJC4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.569	933.87 ng/ul	38719300	1,4-Dichlorobenzene-d4	7.957

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

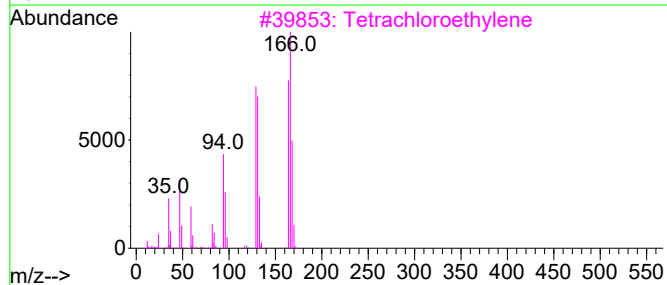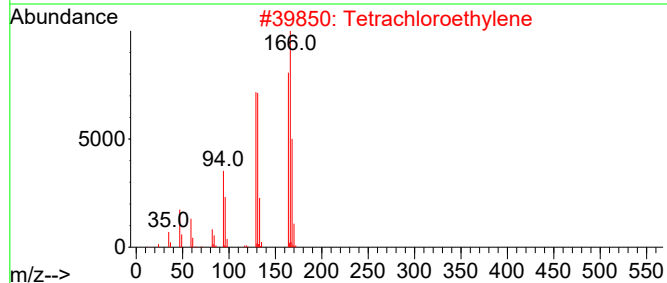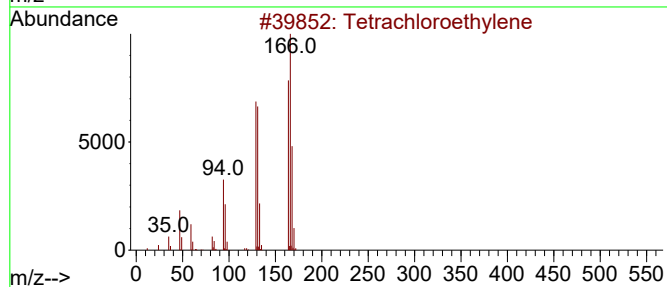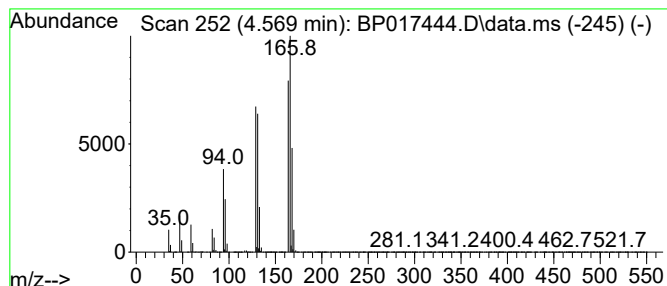

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017444.D
Acq On : 29 Sep 2023 13:56
Operator : MA/JU
Sample : 04497-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJC4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.569	933.9	ng/ul	38719300	1	7.957	829220	20.0