

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
 Data File : BP017452.D
 Acq On : 29 Sep 2023 19:01
 Operator : MA/JU
 Sample : PB155868BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK868

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017452.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	32	36	45	rVB	55752	72947	1.32%	0.140%
2	3.734	106	110	129	rBV	700679	1058824	19.18%	2.027%
3	4.040	159	162	166	rVB2	8742	13177	0.24%	0.025%
4	7.105	677	683	694	rBV	849955	1364552	24.72%	2.612%
5	7.293	709	715	726	rVB	684811	1034506	18.74%	1.980%
6	7.469	739	745	754	rBV	878989	1396409	25.29%	2.673%
7	7.952	821	827	835	rBV	602883	939199	17.01%	1.798%
8	8.675	942	950	962	rBV	1045205	1714785	31.06%	3.283%
9	9.163	1025	1033	1040	rBV	792405	1323330	23.97%	2.533%
10	9.875	1145	1154	1165	rBV	672346	1147077	20.78%	2.196%
11	10.404	1235	1244	1260	rBV	1054293	1811578	32.82%	3.468%
12	10.793	1301	1310	1323	rBV	823757	1369380	24.81%	2.622%
13	10.957	1330	1338	1357	rBV	1031388	1823227	33.03%	3.490%
14	11.840	1478	1488	1490	rBV	3334	9492	0.17%	0.018%
15	12.387	1575	1581	1588	rVB	17585	30062	0.54%	0.058%
16	13.481	1761	1767	1776	rVB8	12366	25568	0.46%	0.049%
17	14.057	1857	1865	1873	rBV	1844615	2557050	46.32%	4.895%
18	14.345	1907	1914	1925	rBV	2198102	3142455	56.92%	6.016%
19	14.645	1958	1965	1974	rBV	1292452	1843310	33.39%	3.529%
20	14.881	1997	2005	2023	rBV	688315	1202219	21.78%	2.302%
21	15.334	2078	2082	2086	rBV7	4197	6839	0.12%	0.013%
22	15.651	2129	2136	2145	rBV	2783052	3945560	71.47%	7.554%
23	15.786	2153	2159	2167	rBV	722576	989181	17.92%	1.894%
24	15.886	2172	2176	2182	rVV3	12044	18499	0.34%	0.035%
25	17.098	2378	2382	2386	rVB7	5269	9160	0.17%	0.018%
26	17.228	2400	2404	2406	rBV5	4160	6463	0.12%	0.012%
27	17.433	2432	2439	2448	rBV	1710889	2316684	41.96%	4.435%
28	17.533	2450	2456	2468	rVV	3238343	4517607	81.83%	8.649%
29	19.357	2762	2766	2770	rBV	42139	54761	0.99%	0.105%
30	19.422	2774	2777	2782	rVB	35960	45316	0.82%	0.087%
31	19.786	2833	2839	2845	rBV	4385897	5520536	100.00%	10.569%
32	21.563	3136	3141	3149	rBV	2130023	2639695	47.82%	5.054%
33	23.968	3543	3550	3560	rVB2	2648697	5512781	99.86%	10.554%
34	24.139	3573	3579	3589	rVB	1339221	2772538	50.22%	5.308%

Sum of corrected areas: 52234767




Instrument :
BNA_P
ClientSampleId :
SBLK868

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017452.D
Acq On : 29 Sep 2023 19:01
Operator : MA/JU
Sample : PB155868BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK868

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

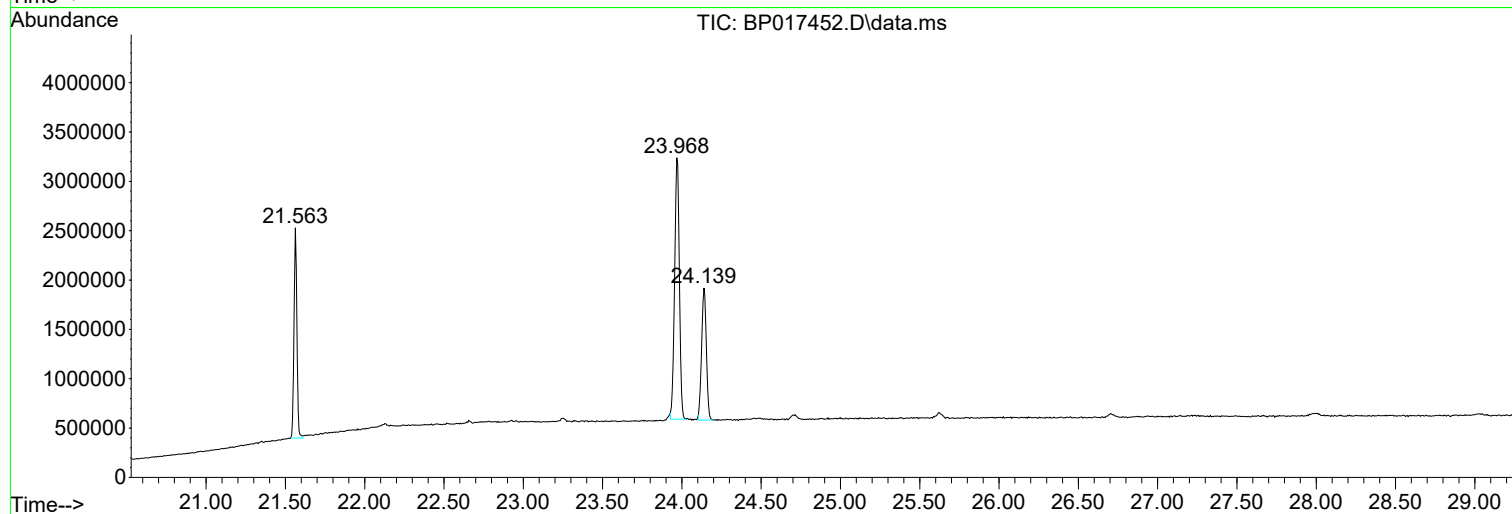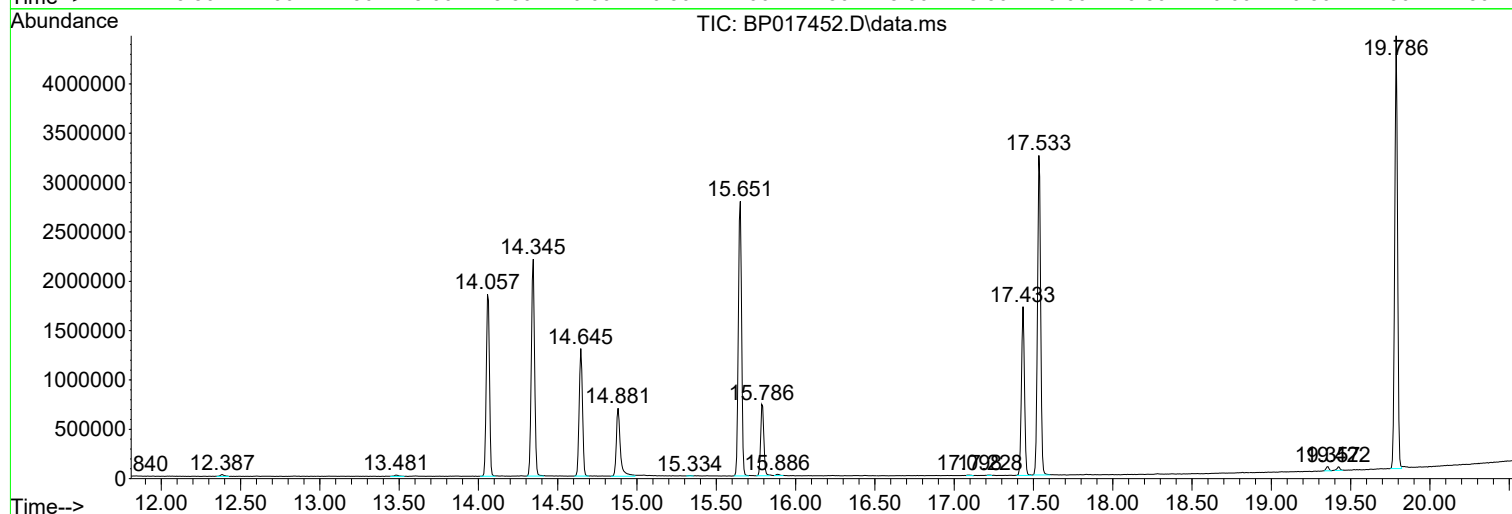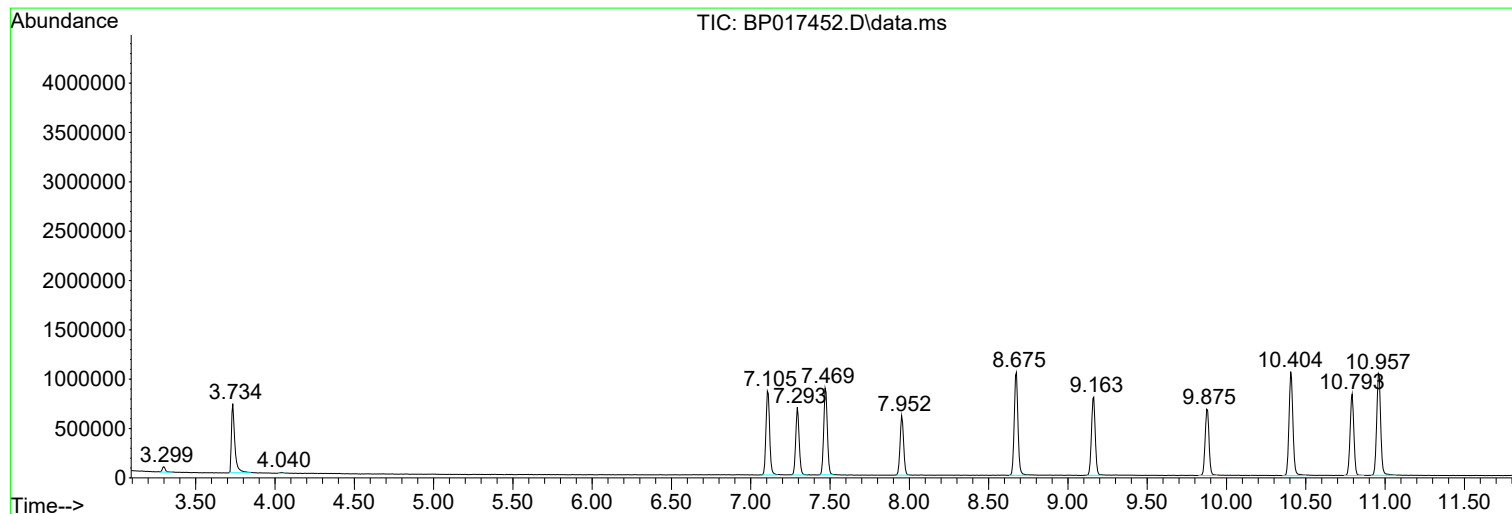

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017452.D
Acq On : 29 Sep 2023 19:01
Operator : MA/JU
Sample : PB155868BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK868

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017452.D
Acq On : 29 Sep 2023 19:01
Operator : MA/JU
Sample : PB155868BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK868

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc