

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
 Data File : BP017453.D
 Acq On : 29 Sep 2023 19:35
 Operator : MA/JU
 Sample : 04497-13
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBBP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017453.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	25	28	33	rVB5	17686	20142	0.19%	0.019%
2	3.299	33	36	40	rVB	32648	40154	0.37%	0.037%
3	3.734	106	110	126	rBV	329046	504176	4.70%	0.464%
4	3.923	137	142	150	rBV	71327	102707	0.96%	0.095%
5	4.040	158	162	167	rVB	32970	45281	0.42%	0.042%
6	4.187	183	187	195	rVB3	25425	39051	0.36%	0.036%
7	4.428	224	228	234	rVB2	20014	30819	0.29%	0.028%
8	4.570	248	252	257	rVB4	13665	19540	0.18%	0.018%
9	4.981	318	322	327	rBV	12191	17054	0.16%	0.016%
10	5.564	417	421	426	rBV	8636	13672	0.13%	0.013%
11	6.352	550	555	560	rBV	23014	35453	0.33%	0.033%
12	6.916	646	651	657	rVB5	11555	19957	0.19%	0.018%
13	7.105	677	683	694	rBV	287536	467274	4.36%	0.430%
14	7.293	707	715	728	rVB	1069125	1644719	15.33%	1.514%
15	7.469	738	745	759	rBV	1100558	1737734	16.20%	1.600%
16	7.952	820	827	839	rBV	2301345	3552990	33.13%	3.272%
17	8.675	940	950	966	rBV	805406	1352578	12.61%	1.245%
18	9.163	1025	1033	1039	rBV	1293290	2154139	20.08%	1.984%
19	9.228	1039	1044	1050	rVB	130788	215453	2.01%	0.198%
20	9.358	1061	1066	1071	rVB	10160	13036	0.12%	0.012%
21	9.875	1147	1154	1165	rBV	1101477	1805600	16.83%	1.663%
22	10.405	1234	1244	1258	rBV	1578764	2625991	24.48%	2.418%
23	10.793	1302	1310	1323	rBV	3162410	5145211	47.97%	4.738%
24	10.957	1328	1338	1359	rBV	1490814	2580701	24.06%	2.376%
25	11.857	1486	1491	1499	rVB3	13755	27498	0.26%	0.025%
26	12.381	1575	1580	1586	rBV2	27278	45384	0.42%	0.042%
27	12.516	1598	1603	1609	rBV2	5940	10843	0.10%	0.010%
28	13.481	1761	1767	1775	rBV	205425	325921	3.04%	0.300%
29	13.863	1821	1832	1837	rBV10	9469	22804	0.21%	0.021%
30	14.063	1859	1866	1873	rBV	3216907	4342793	40.49%	3.999%
31	14.257	1894	1899	1906	rBV	5800	13685	0.13%	0.013%
32	14.346	1906	1914	1925	rBV	3729891	5309157	49.50%	4.889%
33	14.645	1958	1965	1974	rVB	4735045	7081584	66.03%	6.521%
34	14.881	1999	2005	2018	rBV	224070	415699	3.88%	0.383%
35	15.028	2026	2030	2038	rBV8	9646	23857	0.22%	0.022%
36	15.093	2038	2041	2047	rVB8	8505	11726	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
 Data File : BP017453.D
 Acq On : 29 Sep 2023 19:35
 Operator : MA/JU
 Sample : 04497-13
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBBP6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

37	15.287	2070	2074	2078	rBV5	18304	26280	0.25%	0.024%
38	15.651	2126	2136	2144	rBV	4867381	6844772	63.82%	6.303%
39	15.792	2154	2160	2172	rBV	1527932	2039229	19.01%	1.878%
40	15.887	2172	2176	2181	rVB2	27132	38554	0.36%	0.036%
41	16.234	2228	2235	2241	rBV2	5376	11087	0.10%	0.010%
42	16.363	2254	2257	2262	rBV3	6248	11739	0.11%	0.011%
43	16.781	2324	2328	2334	rBV8	7611	12318	0.11%	0.011%
44	17.092	2378	2381	2390	rVB8	9045	12367	0.12%	0.011%
45	17.216	2398	2402	2409	rBV2	15211	24893	0.23%	0.023%
46	17.434	2432	2439	2450	rBV	6137917	8810917	82.15%	8.113%
47	17.539	2450	2457	2468	rVV	5525837	7942973	74.06%	7.314%
48	17.687	2480	2482	2488	rVB3	7597	10911	0.10%	0.010%
49	18.063	2542	2546	2552	rVB6	24149	32453	0.30%	0.030%
50	18.281	2578	2583	2593	rBV	276974	427186	3.98%	0.393%
51	19.192	2736	2738	2744	rVB7	14847	19232	0.18%	0.018%
52	19.351	2761	2765	2769	rBV3	72877	88765	0.83%	0.082%
53	19.422	2773	2777	2781	rVB	70149	90012	0.84%	0.083%
54	19.522	2789	2794	2806	rBV	238060	391782	3.65%	0.361%
55	19.786	2833	2839	2845	rBV	7347967	9557087	89.11%	8.800%
56	21.563	3135	3141	3152	rBV	7372530	9997097	93.21%	9.205%
57	23.974	3543	3551	3559	rVB2	4586968	9672868	90.19%	8.907%
58	24.145	3572	3580	3592	rVB2	4844376	10725455	100.00%	9.876%




Sum of corrected areas: 108602360

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017453.D
Acq On : 29 Sep 2023 19:35
Operator : MA/JU
Sample : 04497-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBBP6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

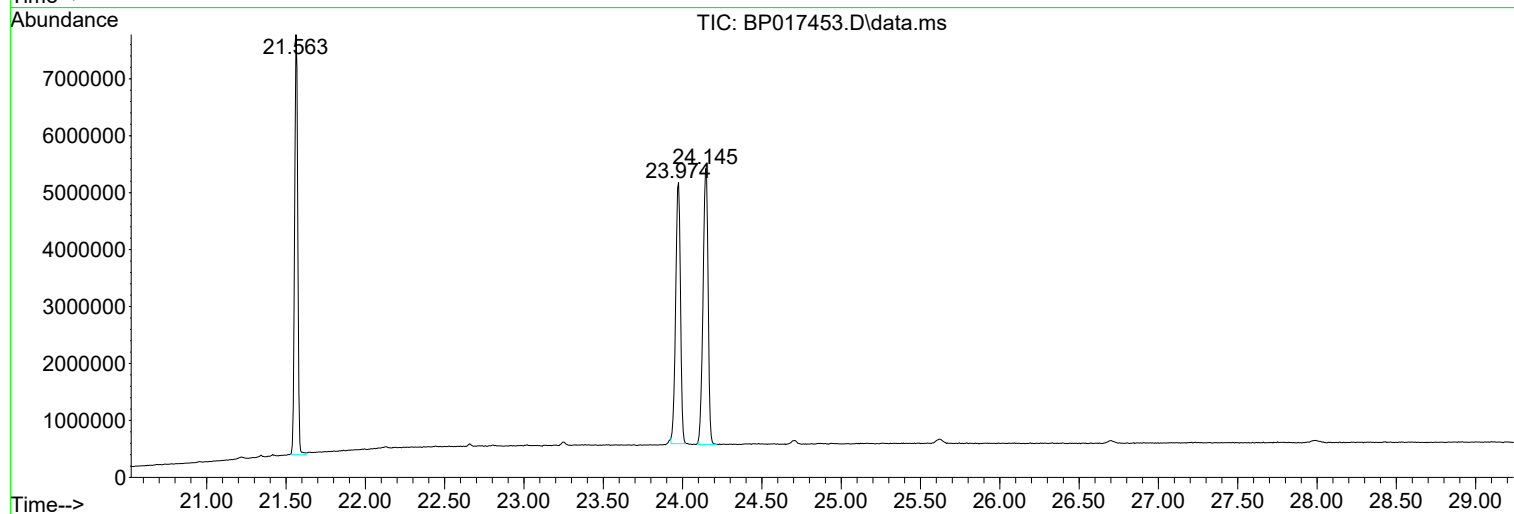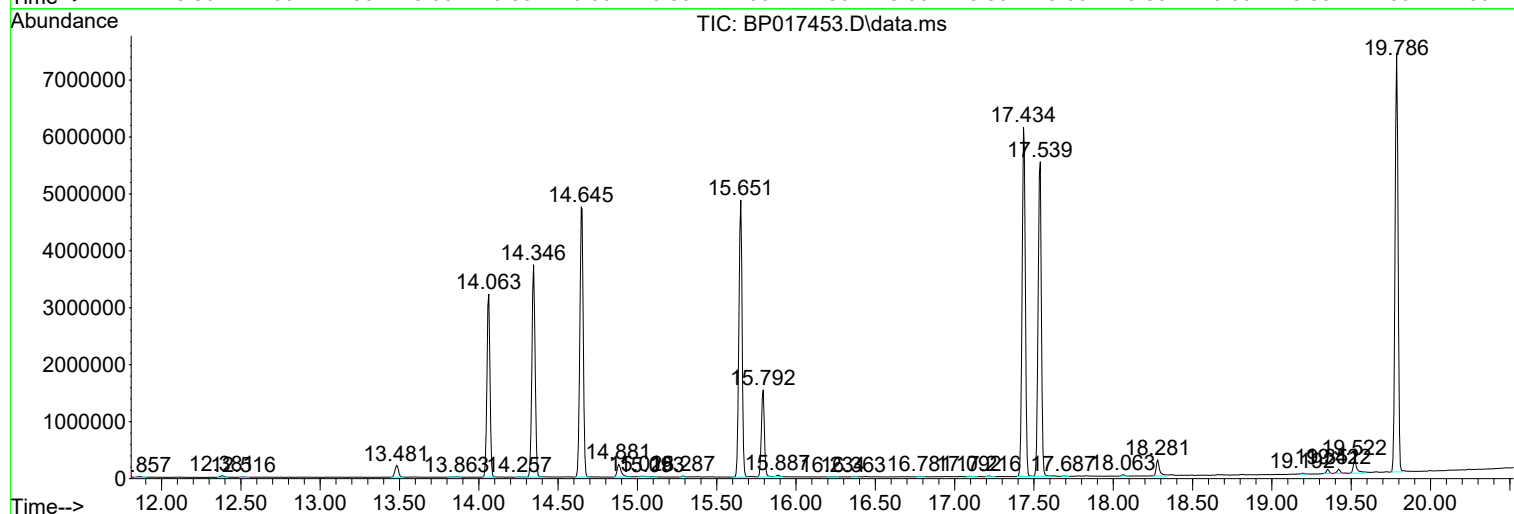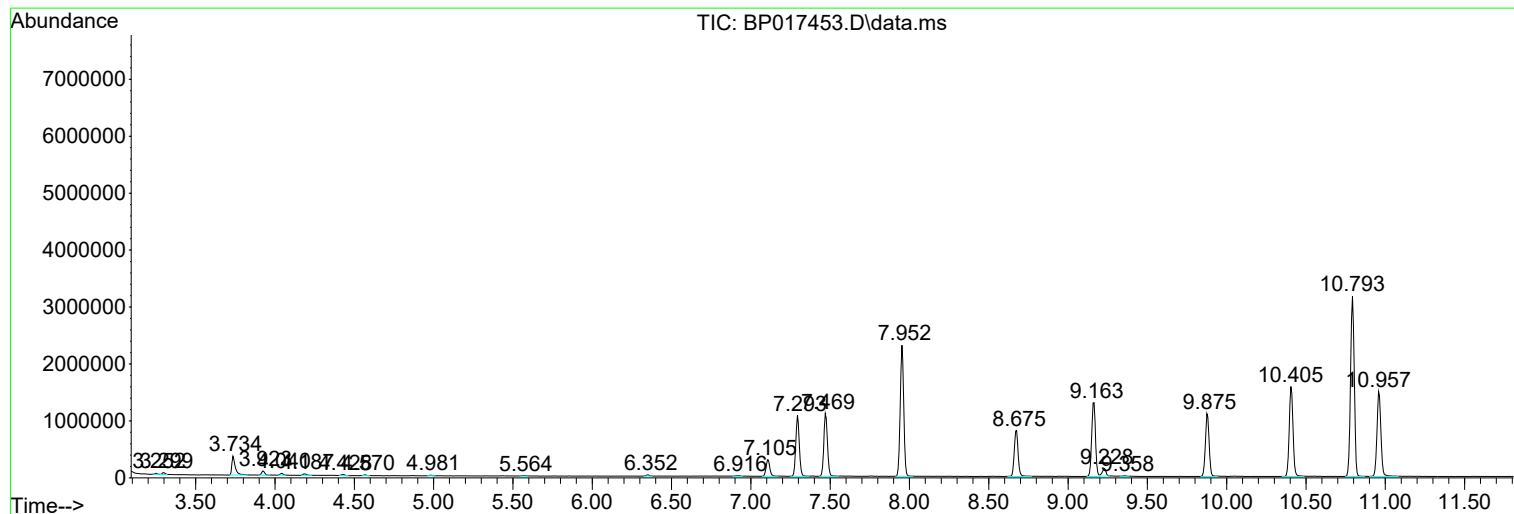

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017453.D
Acq On : 29 Sep 2023 19:35
Operator : MA/JU
Sample : 04497-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBBP6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017453.D
Acq On : 29 Sep 2023 19:35
Operator : MA/JU
Sample : 04497-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBBP6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------