

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
 Data File : BP017457.D
 Acq On : 29 Sep 2023 21:51
 Operator : MA/JU
 Sample : 04497-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJ60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017457.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	22	28	52	rVB	9553461	14871055	34.87%	13.225%
2	3.740	107	111	120	rBV	168429	247905	0.58%	0.220%
3	3.928	138	143	149	rVB	54286	77549	0.18%	0.069%
4	4.046	158	163	169	rVB	64310	92175	0.22%	0.082%
5	4.570	245	252	255	rBV	22204998	42643533	100.00%	37.925%
6	5.022	325	329	341	rVB	78848	119832	0.28%	0.107%
7	7.105	677	683	692	rBV	244324	399124	0.94%	0.355%
8	7.293	709	715	725	rBV	771471	1162212	2.73%	1.034%
9	7.469	739	745	754	rBV	803617	1263124	2.96%	1.123%
10	7.546	754	758	770	rVB	33375	67577	0.16%	0.060%
11	7.952	820	827	836	rBV	969984	1504414	3.53%	1.338%
12	8.669	942	949	965	rBV	639743	1027635	2.41%	0.914%
13	9.158	1024	1032	1044	rBV	907300	1466476	3.44%	1.304%
14	9.875	1147	1154	1164	rBV	730381	1168129	2.74%	1.039%
15	10.405	1237	1244	1264	rBV	1055116	1754679	4.11%	1.561%
16	10.793	1302	1310	1321	rBV	1250698	2120501	4.97%	1.886%
17	10.957	1331	1338	1350	rBV	866402	1460019	3.42%	1.298%
18	12.375	1569	1579	1588	rVB5	18989	47448	0.11%	0.042%
19	13.481	1762	1767	1773	rVB	46910	75217	0.18%	0.067%
20	14.057	1858	1865	1875	rBV	2035795	2679199	6.28%	2.383%
21	14.340	1905	1913	1927	rBV	2220780	3244068	7.61%	2.885%
22	14.645	1957	1965	1973	rVB	1850007	2711773	6.36%	2.412%
23	14.881	1999	2005	2021	rBV	140676	277729	0.65%	0.247%
24	15.645	2128	2135	2144	rBV	2892398	4069961	9.54%	3.620%
25	15.787	2153	2159	2170	rBV	802014	1056529	2.48%	0.940%
26	17.434	2432	2439	2447	rBV	2170044	3139442	7.36%	2.792%
27	17.534	2449	2456	2468	rVV	3299124	4507255	10.57%	4.008%
28	18.275	2578	2582	2590	rBV	147256	221225	0.52%	0.197%
29	19.351	2761	2765	2769	rBV2	44153	56598	0.13%	0.050%
30	19.422	2774	2777	2780	rVB	37520	47315	0.11%	0.042%
31	19.516	2790	2793	2798	rBV3	68196	93164	0.22%	0.083%
32	19.781	2832	2838	2846	rBV	4036515	5437037	12.75%	4.835%
33	21.563	3135	3141	3147	rBV	2666444	3591142	8.42%	3.194%
34	23.963	3542	3549	3561	rVB2	2849591	5787484	13.57%	5.147%
35	24.133	3571	3578	3591	rVB	1837382	3954178	9.27%	3.517%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017457.D
Acq On : 29 Sep 2023 21:51
Operator : MA/JU
Sample : 04497-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ60

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 112442703

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017457.D
Acq On : 29 Sep 2023 21:51
Operator : MA/JU
Sample : 04497-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ60

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

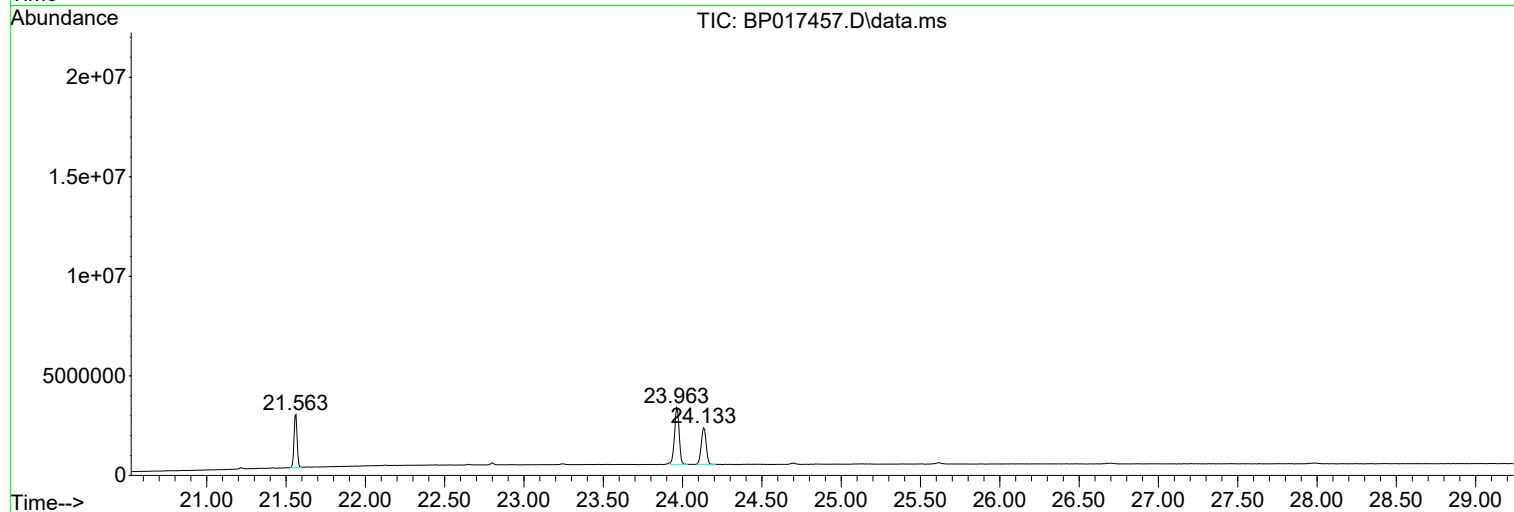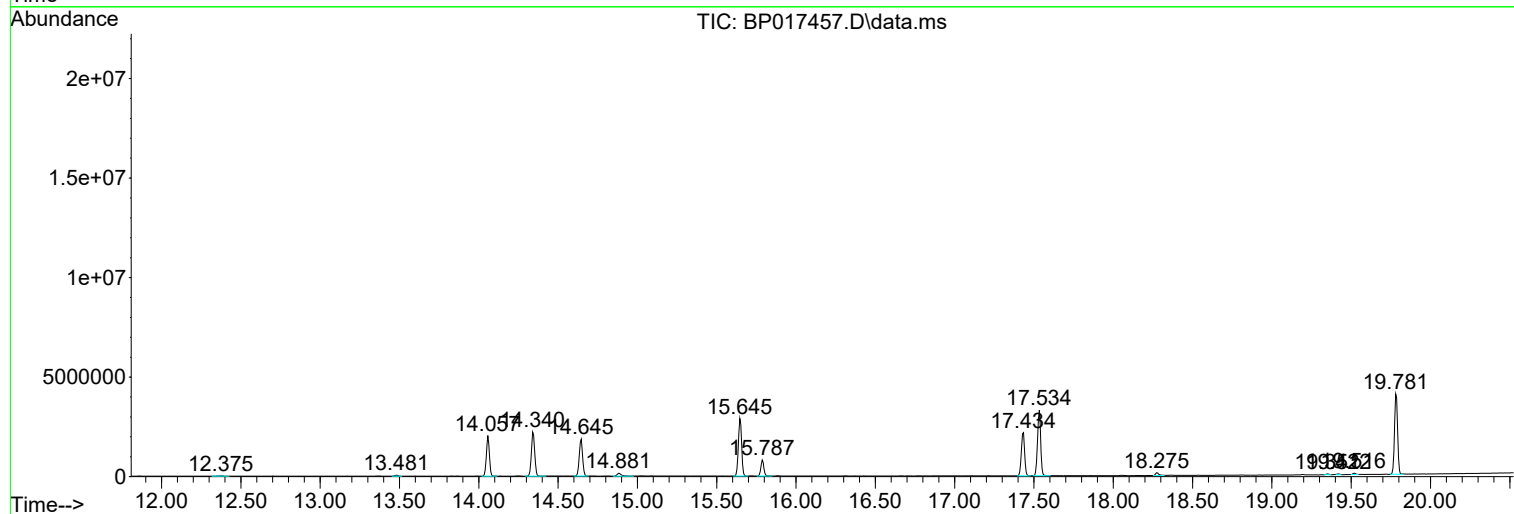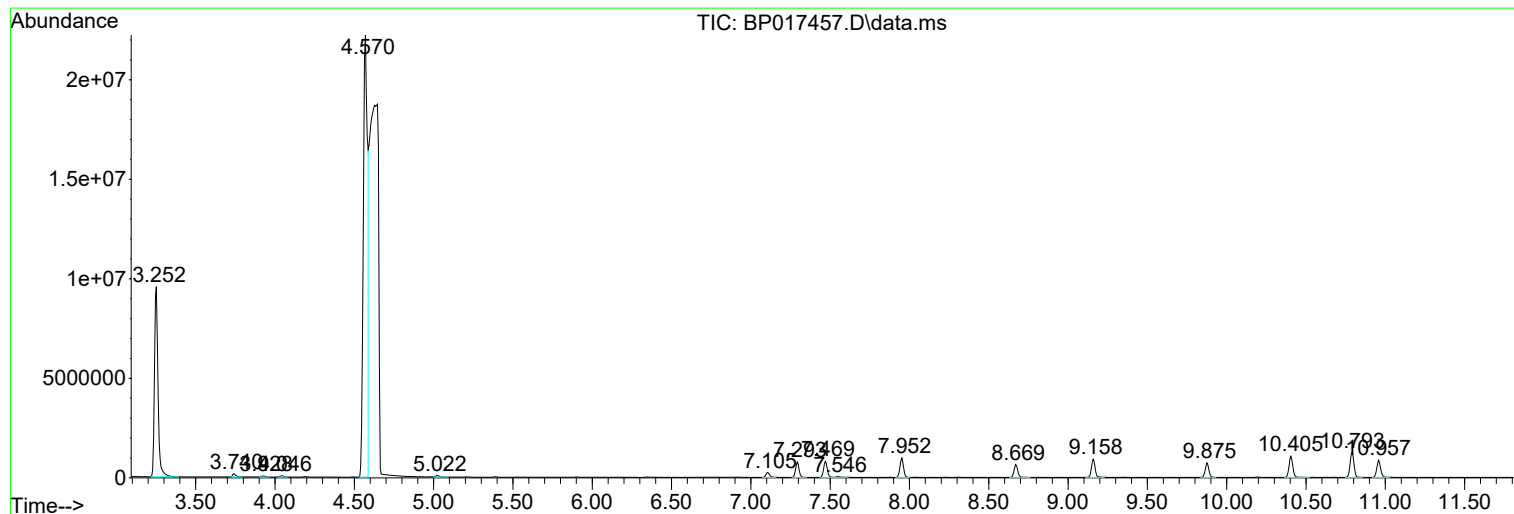

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017457.D
Acq On : 29 Sep 2023 21:51
Operator : MA/JU
Sample : 04497-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ60










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.570	566.91 ng/ul	42643500	1,4-Dichlorobenzene-d4	7.952

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			2,4-Dichloro-6-fluoropyrimidine	166	C4HC12FN2	003833-57-6	38

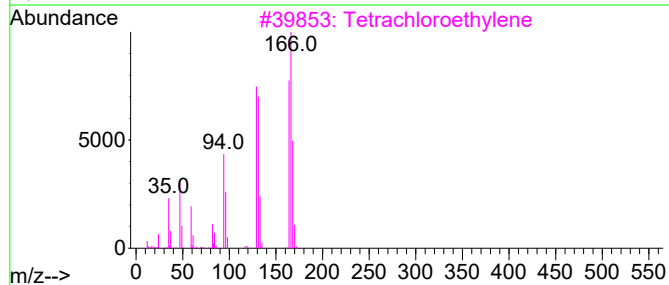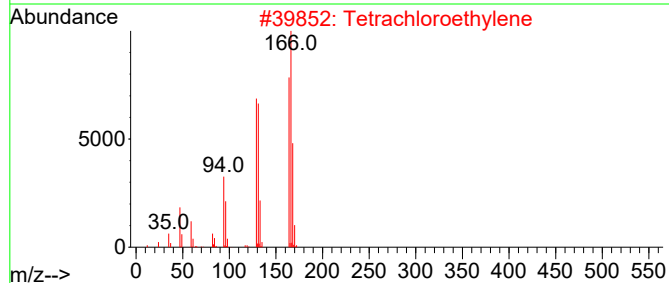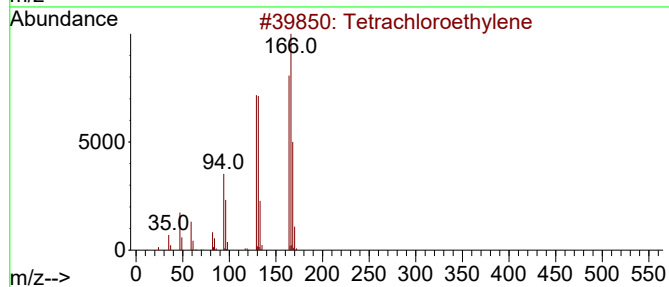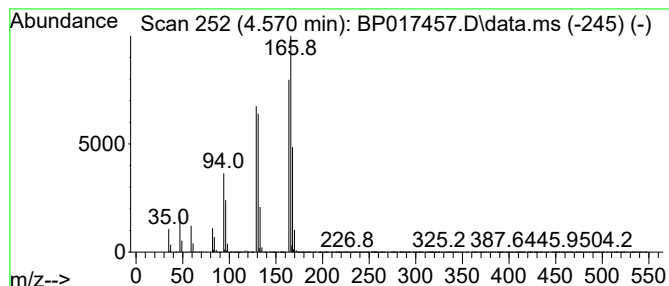

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017457.D
Acq On : 29 Sep 2023 21:51
Operator : MA/JU
Sample : 04497-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ60

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.570	566.9	ng/ul	42643500	1	7.952	1504410	20.0