

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
 Data File : BP017458.D
 Acq On : 29 Sep 2023 22:25
 Operator : MA/JU
 Sample : 04497-16
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJ22

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017458.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	22	28	54	rVB	8719194	12999058	30.65%	12.240%
2	3.734	107	110	125	rBV	287631	437449	1.03%	0.412%
3	3.928	138	143	151	rVB	54113	79853	0.19%	0.075%
4	4.046	157	163	170	rBV	62375	93677	0.22%	0.088%
5	4.569	244	252	255	rBV	22347781	42407516	100.00%	39.930%
6	5.022	325	329	335	rVB	73656	101388	0.24%	0.095%
7	7.105	676	683	696	rBV	224967	376369	0.89%	0.354%
8	7.293	706	715	728	rBV	760002	1151441	2.72%	1.084%
9	7.469	738	745	755	rBV	785547	1229231	2.90%	1.157%
10	7.952	820	827	836	rBV	890435	1366063	3.22%	1.286%
11	8.669	942	949	967	rBV	591470	977833	2.31%	0.921%
12	9.157	1024	1032	1046	rBV	865538	1426462	3.36%	1.343%
13	9.875	1147	1154	1166	rBV	706157	1132610	2.67%	1.066%
14	10.404	1237	1244	1255	rBV	991480	1665424	3.93%	1.568%
15	10.793	1301	1310	1322	rBV	1118001	1891384	4.46%	1.781%
16	10.957	1330	1338	1354	rBV	875770	1505694	3.55%	1.418%
17	12.381	1572	1580	1588	rVB3	19057	43938	0.10%	0.041%
18	13.481	1761	1767	1775	rBV	36862	63948	0.15%	0.060%
19	14.057	1858	1865	1877	rBV	1781318	2336734	5.51%	2.200%
20	14.340	1906	1913	1920	rBV	1974866	2955158	6.97%	2.783%
21	14.645	1955	1965	1974	rBV	1666423	2395122	5.65%	2.255%
22	14.881	1998	2005	2019	rBV2	109740	234040	0.55%	0.220%
23	15.645	2128	2135	2144	rBV	2545773	3633130	8.57%	3.421%
24	15.787	2153	2159	2172	rVV	701274	924485	2.18%	0.870%
25	17.433	2432	2439	2449	rBV	2043078	2898115	6.83%	2.729%
26	17.533	2449	2456	2469	rVV	3024750	4063322	9.58%	3.826%
27	18.275	2578	2582	2590	rBV	104106	152261	0.36%	0.143%
28	19.422	2774	2777	2783	rVB2	30682	42575	0.10%	0.040%
29	19.516	2790	2793	2799	rBV3	55962	80742	0.19%	0.076%
30	19.780	2833	2838	2844	rBV	3832613	5000098	11.79%	4.708%
31	21.563	3136	3141	3146	rBV	2575293	3318701	7.83%	3.125%
32	23.968	3542	3550	3560	rVB2	2608243	5541405	13.07%	5.218%
33	24.133	3571	3578	3587	rVB	1725782	3679255	8.68%	3.464%




Sum of corrected areas: 106204481

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017458.D
Acq On : 29 Sep 2023 22:25
Operator : MA/JU
Sample : 04497-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ22

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

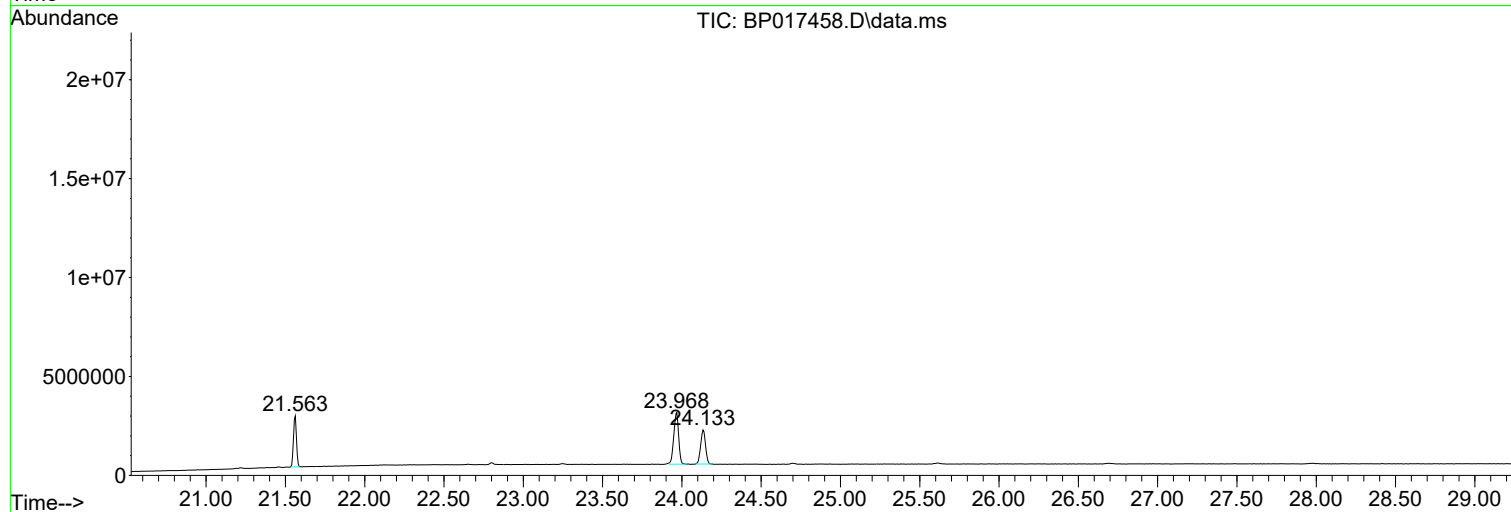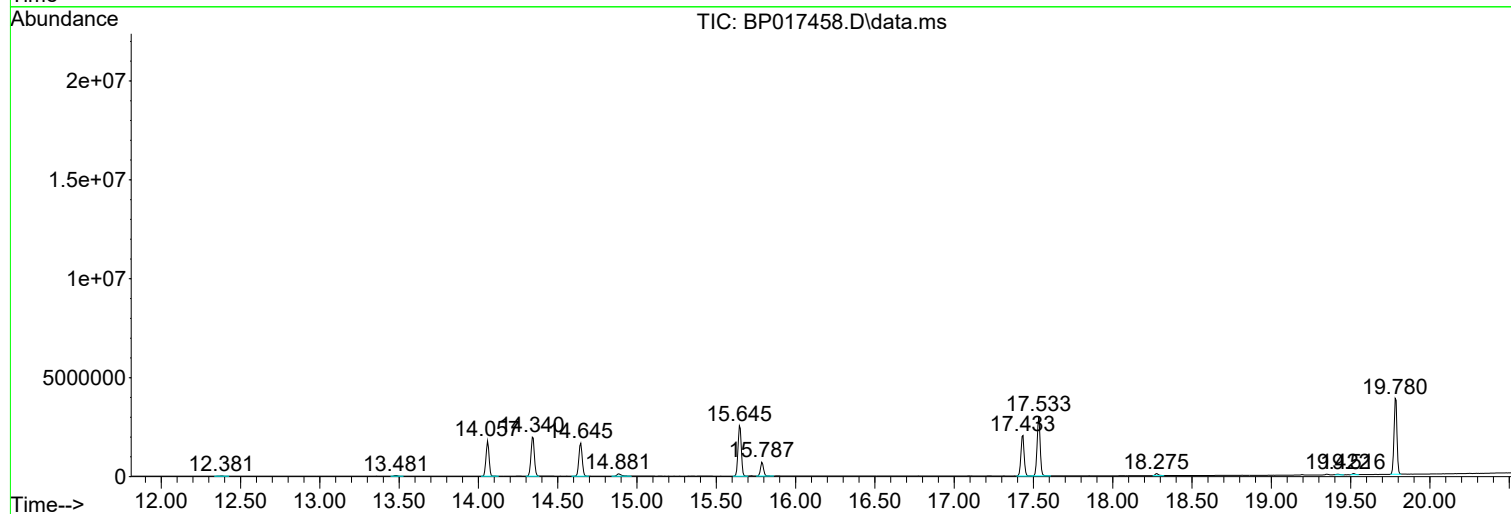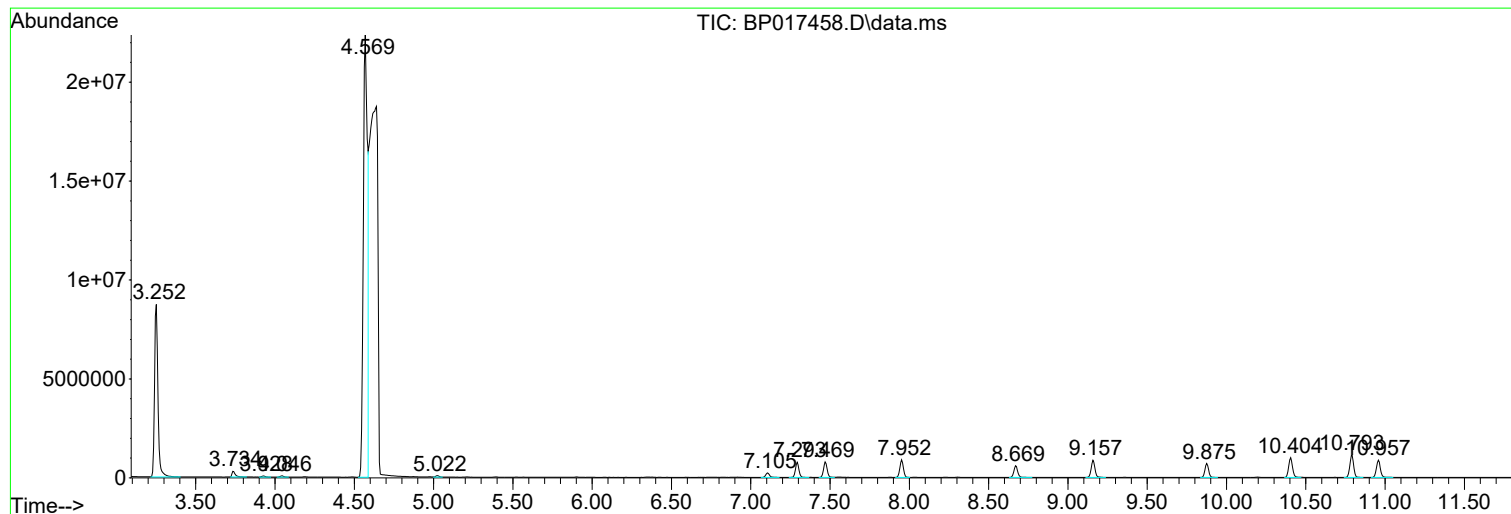

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017458.D
Acq On : 29 Sep 2023 22:25
Operator : MA/JU
Sample : 04497-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ22










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.569	620.87 ng/ul	42407500	1,4-Dichlorobenzene-d4	7.952

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			2,4-Dichloro-6-fluoropyrimidine	166	C4HC12FN2	003833-57-6	38

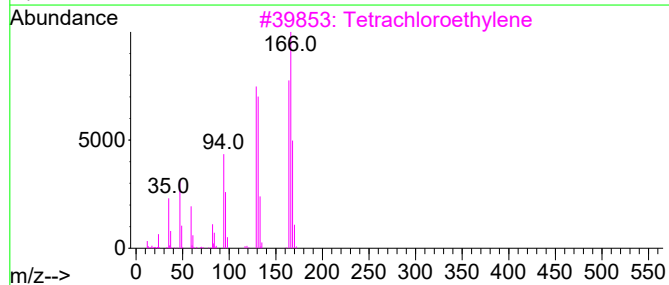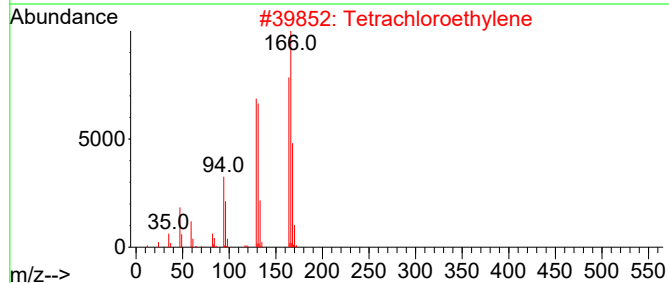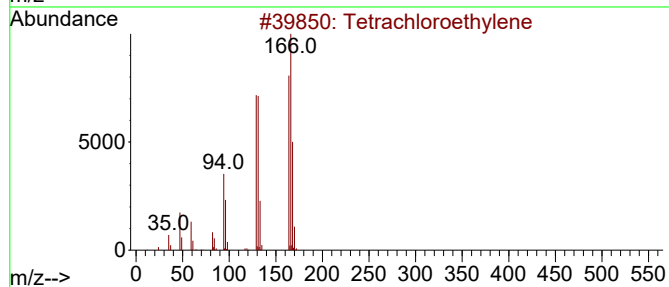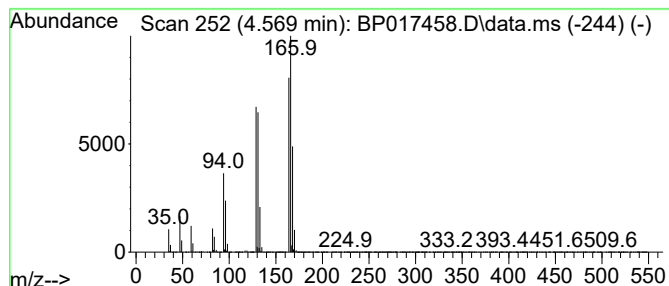

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017458.D
Acq On : 29 Sep 2023 22:25
Operator : MA/JU
Sample : 04497-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ22

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.569	620.9	ng/ul	42407500	1	7.952	1366060	20.0