

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
 Data File : BP017468.D
 Acq On : 30 Sep 2023 04:40
 Operator : MA/JU
 Sample : PB155898BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK898

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017468.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	32	35	42	rVB	46104	57488	1.53%	0.138%
2	3.728	106	109	122	rBV	533176	796796	21.17%	1.917%
3	4.040	159	162	166	rVB2	11599	13959	0.37%	0.034%
4	4.558	248	250	257	rBV7	3172	4157	0.11%	0.010%
5	7.105	676	683	695	rBV	637704	1022335	27.16%	2.460%
6	7.293	708	715	723	rVB	519446	798448	21.21%	1.921%
7	7.469	738	745	757	rBV	673333	1061499	28.20%	2.554%
8	7.952	818	827	839	rBV	764282	1219651	32.40%	2.935%
9	8.669	941	949	960	rBV	792785	1260633	33.49%	3.033%
10	9.157	1025	1032	1045	rBV	614811	996073	26.46%	2.397%
11	9.463	1082	1084	1089	rVB6	2781	4222	0.11%	0.010%
12	9.875	1147	1154	1163	rBV	507977	824345	21.90%	1.984%
13	10.404	1235	1244	1259	rBV	740291	1302315	34.60%	3.134%
14	10.575	1269	1273	1277	rVB7	2290	4408	0.12%	0.011%
15	10.787	1301	1309	1320	rVB	1039165	1685201	44.77%	4.055%
16	10.957	1327	1338	1353	rBV	759320	1316378	34.97%	3.168%
17	12.387	1574	1581	1586	rBV4	10641	17504	0.47%	0.042%
18	12.510	1598	1602	1604	rBV4	3054	3978	0.11%	0.010%
19	13.475	1762	1766	1772	rVB3	12901	21007	0.56%	0.051%
20	14.057	1857	1865	1872	rBV	1336547	1778800	47.26%	4.280%
21	14.339	1906	1913	1921	rBV2	1505701	2161910	57.43%	5.202%
22	14.639	1958	1964	1974	rBV	1451924	2142491	56.92%	5.155%
23	14.875	1998	2004	2022	rBV	383865	732370	19.46%	1.762%
24	15.039	2031	2032	2036	rVB4	4187	4657	0.12%	0.011%
25	15.645	2128	2135	2144	rBV	1976490	2674534	71.05%	6.436%
26	15.786	2153	2159	2173	rBV	459173	627171	16.66%	1.509%
27	15.886	2173	2176	2183	rVB8	9323	14145	0.38%	0.034%
28	17.092	2378	2381	2387	rVB8	4701	6876	0.18%	0.017%
29	17.210	2397	2401	2405	rBV7	5173	8296	0.22%	0.020%
30	17.428	2430	2438	2448	rBV	1827827	2541821	67.53%	6.116%
31	17.528	2448	2455	2465	rBV2	2100650	2935058	77.97%	7.063%
32	17.757	2491	2494	2497	rBV4	3438	5378	0.14%	0.013%
33	17.827	2504	2506	2510	rBV5	4254	7139	0.19%	0.017%
34	18.275	2580	2582	2585	rBV4	4018	4090	0.11%	0.010%
35	19.345	2761	2764	2769	rBV4	25143	33395	0.89%	0.080%
36	19.416	2773	2776	2780	rVV	21661	27928	0.74%	0.067%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017468.D
Acq On : 30 Sep 2023 04:40
Operator : MA/JU
Sample : PB155898BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK898

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Title : SVOA CALIBRATION

37	19.780	2832	2838	2844	rBV	2842204	3545452	94.19%	8.531%
38	21.557	3135	3140	3152	rBV	2316095	2974103	79.01%	7.157%
39	23.957	3541	3548	3558	rVB	1849761	3764176	100.00%	9.058%
40	24.127	3570	3577	3585	rVB	1496289	3157594	83.89%	7.598%




Sum of corrected areas: 41557781

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017468.D
Acq On : 30 Sep 2023 04:40
Operator : MA/JU
Sample : PB155898BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK898

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

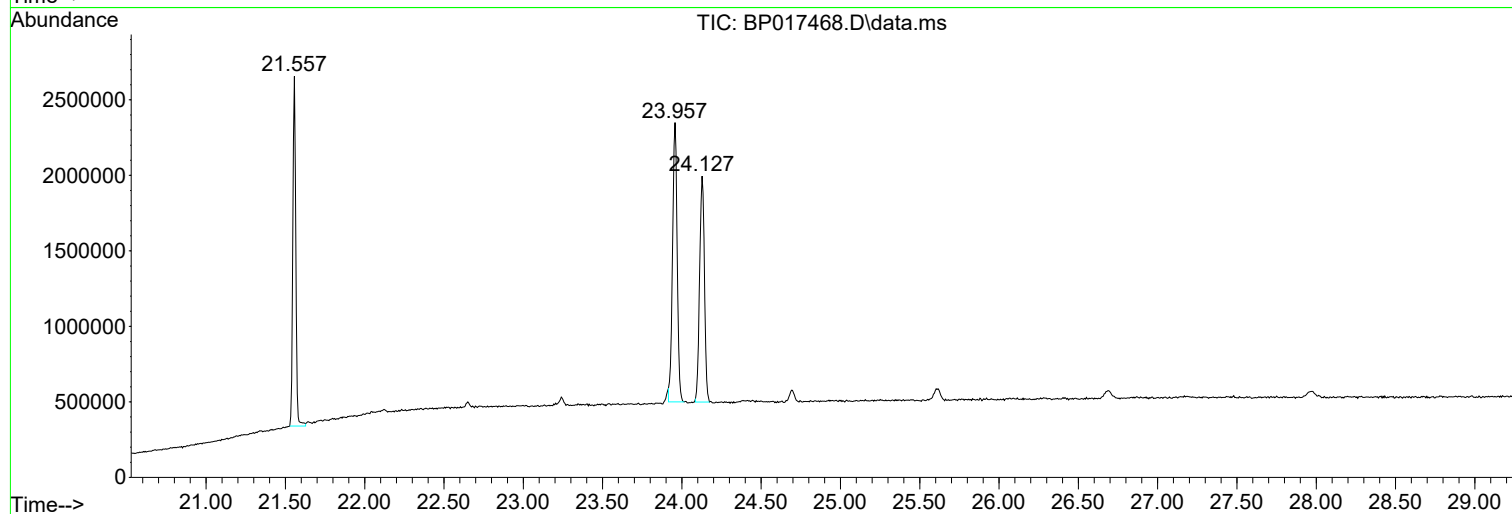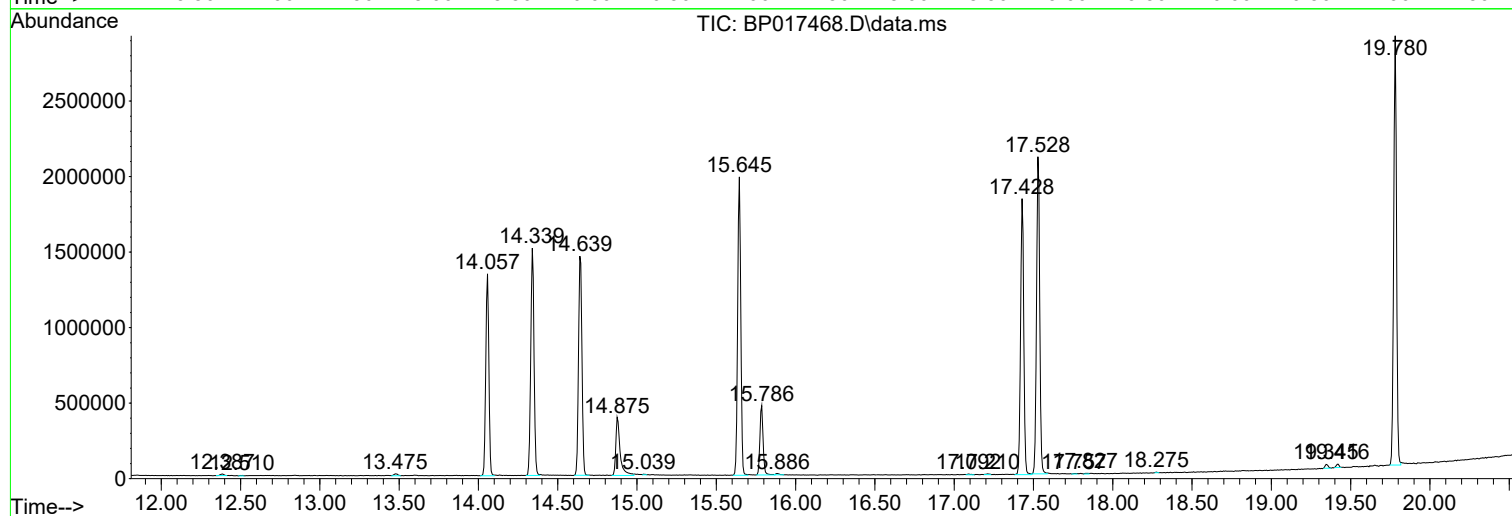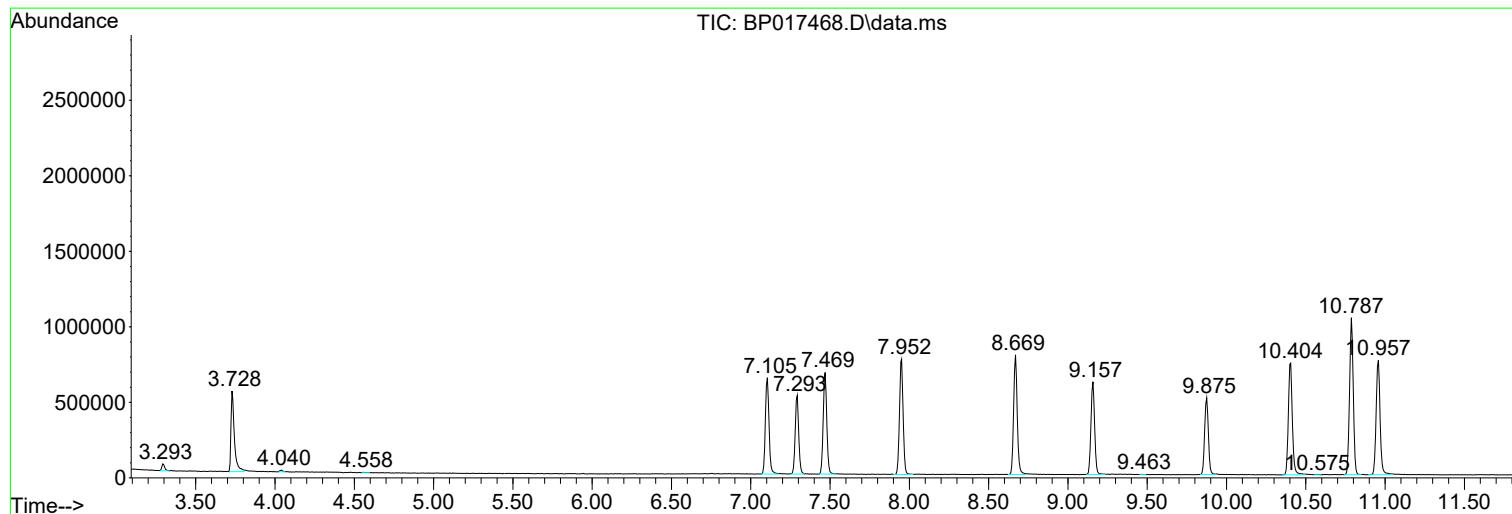

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017468.D
Acq On : 30 Sep 2023 04:40
Operator : MA/JU
Sample : PB155898BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK898

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP092923\
Data File : BP017468.D
Acq On : 30 Sep 2023 04:40
Operator : MA/JU
Sample : PB155898BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK898

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc