

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093022\
 Data File : BP011845.D
 Acq On : 30 Sep 2022 17:37
 Operator : CG/JU
 Sample : SST01057
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST010618

Quant Time: Oct 01 00:03:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 30 23:58:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	243482	20.000	ng/ul	0.00
20) Naphthalene-d8	10.704	136	1106137	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.539	164	742461	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.298	188	1581588	20.000	ng/ul	0.00
79) Chrysene-d12	21.380	240	1616724	20.000	ng/ul	0.00
88) Perylene-d12	23.821	264	1745787	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	22002	3.988	ng/uL	0.00
4) Pyridine-d5	3.734	84	146131	9.527	ng/ul	0.00
7) Phenol-d5	7.058	99	190836	9.470	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	113095	9.395	ng/ul	0.00
11) 2-Chlorophenol-d4	7.422	132	159950	10.395	ng/ul	0.00
15) 4-Methylphenol-d8	8.604	113	157458	10.191	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	80171	11.121	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	82702	13.525	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	161216	10.299	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131	248459	10.396	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	526387	10.533	ng/ul	0.00
49) Acenaphthylene-d8	14.234	160	593366	9.941	ng/ul	0.00
54) 4-Nitrophenol-d4	14.734	143	95430	10.848	ng/ul	0.00
60) Fluorene-d10	15.534	176	460818	10.388	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	78771	13.456	ng/ul	0.00
73) Anthracene-d10	17.398	188	713542	10.185	ng/ul	0.00
81) Pyrene-d10	19.627	212	818604	9.909	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.663	264	858367	10.121	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.340	88	23875	4.102	ng/uL#	93
5) Pyridine	3.752	79	143498	9.471	ng/ul	98
6) Benzaldehyde	7.034	77	96749	10.527	ng/ul	95
8) Phenol	7.081	94	199836	9.713	ng/ul	100
10) Bis(2-Chloroethyl)ether	7.316	93	167278	10.302	ng/ul	100
12) 2-Chlorophenol	7.457	128	170872	10.485	ng/ul	99
13) 2-Methylphenol	8.340	108	157085	10.030	ng/ul	100
14) 2,2'-oxybis(1-Chloropr...	8.434	45	168044	8.046	ng/ul	99
16) Acetophenone	8.722	105	261293	10.551	ng/ul	98
17) N-Nitroso-di-n-propyla...	8.704	70	122956	10.662	ng/ul	99
18) 4-Methylphenol	8.669	108	174075	10.379	ng/ul	100
19) Hexachloroethane	8.981	117	64627	10.032	ng/ul	99
22) Nitrobenzene	9.104	77	177303	10.417	ng/ul	100
23) Isophorone	9.634	82	359289	10.418	ng/ul	99
25) 2-Nitrophenol	9.816	139	98547	13.357	ng/ul	98
26) 2,4-Dimethylphenol	9.875	107	191304	10.286	ng/ul	97
27) Bis(2-Chloroethoxy)met...	10.116	93	238697	10.681	ng/ul	99
29) 2,4-Dichlorophenol	10.351	162	169690	10.599	ng/ul	99
30) Naphthalene	10.757	128	598850	10.521	ng/ul	100
32) 4-Chloroaniline	10.869	127	257106	10.530	ng/ul	95
33) Hexachlorobutadiene	11.040	225	101726	9.541	ng/ul	97
34) Caprolactam	11.651	113	53179	11.302	ng/ul	97
35) 4-Chloro-3-methylphenol	11.987	107	179449	11.274	ng/ul	98
36) 2-Methylnaphthalene	12.363	142	415653	10.899	ng/ul	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093022\
 Data File : BP011845.D
 Acq On : 30 Sep 2022 17:37
 Operator : CG/JU
 Sample : SST01057
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST010618

Quant Time: Oct 01 00:03:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 30 23:58:42 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.587	142	421774	11.034	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	12.728	216	211584	9.362	ng/ul	99
40) Hexachlorocyclopentadiene	12.710	237	110532	8.225	ng/ul	100
41) 2,4,6-Trichlorophenol	12.975	196	138144	10.808	ng/ul	97
42) 2,4,5-Trichlorophenol	13.040	196	147103	10.478	ng/ul	98
43) 1,1'-Biphenyl	13.375	154	549396	9.817	ng/ul	99
44) 2-Chloronaphthalene	13.416	162	428121	9.990	ng/ul	99
45) 2-Nitroaniline	13.622	65	97945	11.033	ng/ul	97
47) Dimethylphthalate	13.998	163	553499	10.821	ng/ul	99
48) 2,6-Dinitrotoluene	14.116	165	99868	12.183	ng/ul	93
50) Acenaphthylene	14.263	152	671319	9.852	ng/ul	99
51) 3-Nitroaniline	14.451	138	108730	11.088	ng/ul	98
52) Acenaphthene	14.604	153	475281	10.667	ng/ul	98
53) 2,4-Dinitrophenol	14.651	184	51209	14.269	ng/ul	98
55) 4-Nitrophenol	14.751	109	64884	9.700	ng/ul	97
56) Dibenzofuran	14.939	168	656961	10.394	ng/ul	98
57) 2,4-Dinitrotoluene	14.904	165	149253	13.076	ng/ul	100
58) 2,3,4,6-Tetrachlorophenol	15.163	232	129786	12.277	ng/ul	100
59) Diethylphthalate	15.363	149	554166	11.125	ng/ul	100
61) Fluorene	15.592	166	544809	10.664	ng/ul	98
62) 4-Chlorophenyl-phenyle...	15.586	204	266120	10.278	ng/ul	100
63) 4-Nitroaniline	15.610	138	108925	11.770	ng/ul	97
66) 4,6-Dinitro-2-methylph...	15.663	198	86161	13.589	ng/ul#	94
67) N-Nitrosodiphenylamine	15.798	169	469681	10.388	ng/ul	99
68) 4-Bromophenyl-phenylether	16.486	248	156351	9.584	ng/ul	99
69) Hexachlorobenzene	16.598	284	178863	9.241	ng/ul	98
70) Atrazine	16.757	200	160083	9.756	ng/ul	99
71) Pentachlorophenol	16.945	266	105434	10.194	ng/ul	99
72) Phenanthrene	17.339	178	875003	10.590	ng/ul	99
74) Anthracene	17.433	178	894558	10.813	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.340	216	214918	8.846	ng/ul	99
76) Pentachlorobenzene	14.857	250	233518	10.178	ng/ul	98
77) Carbazole	17.704	167	794540	10.899	ng/ul	100
78) Di-n-butylphthalate	18.251	149	952250	11.508	ng/ul	100
80) Fluoranthene	19.304	202	1007946	10.158	ng/ul	98
82) Pyrene	19.657	202	1056619	10.322	ng/ul	98
83) Butylbenzylphthalate	20.533	149	430859	12.982	ng/ul	100
84) 3,3'-Dichlorobenzidine	21.298	252	362442	12.887	ng/ul	99
85) Benzo(a)anthracene	21.369	228	1057142	10.803	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.286	149	664317	12.548	ng/ul	100
87) Chrysene	21.421	228	1000546	10.588	ng/ul	98
89) Di-n-octyl phthalate	22.221	149	1114703	11.621	ng/ul	100
90) Benzo(b)fluoranthene	23.074	252	1119559	10.264	ng/ul	99
91) Benzo(k)fluoranthene	23.121	252	1067421	10.223	ng/ul	98
93) Benzo(a)pyrene	23.710	252	985678	9.322	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.356	276	1233990	10.112	ng/ul	100
95) Dibenzo(a,h)anthracene	26.380	278	1111109	10.560	ng/ul	99
96) Benzo(g,h,i)perylene	27.139	276	1091190	10.719	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093022\
Data File : BP011845.D
Acq On : 30 Sep 2022 17:37
Operator : CG/JU
Sample : SST01057
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD010618

Quant Time: Oct 01 00:03:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 30 23:58:42 2022
Response via : Initial Calibration




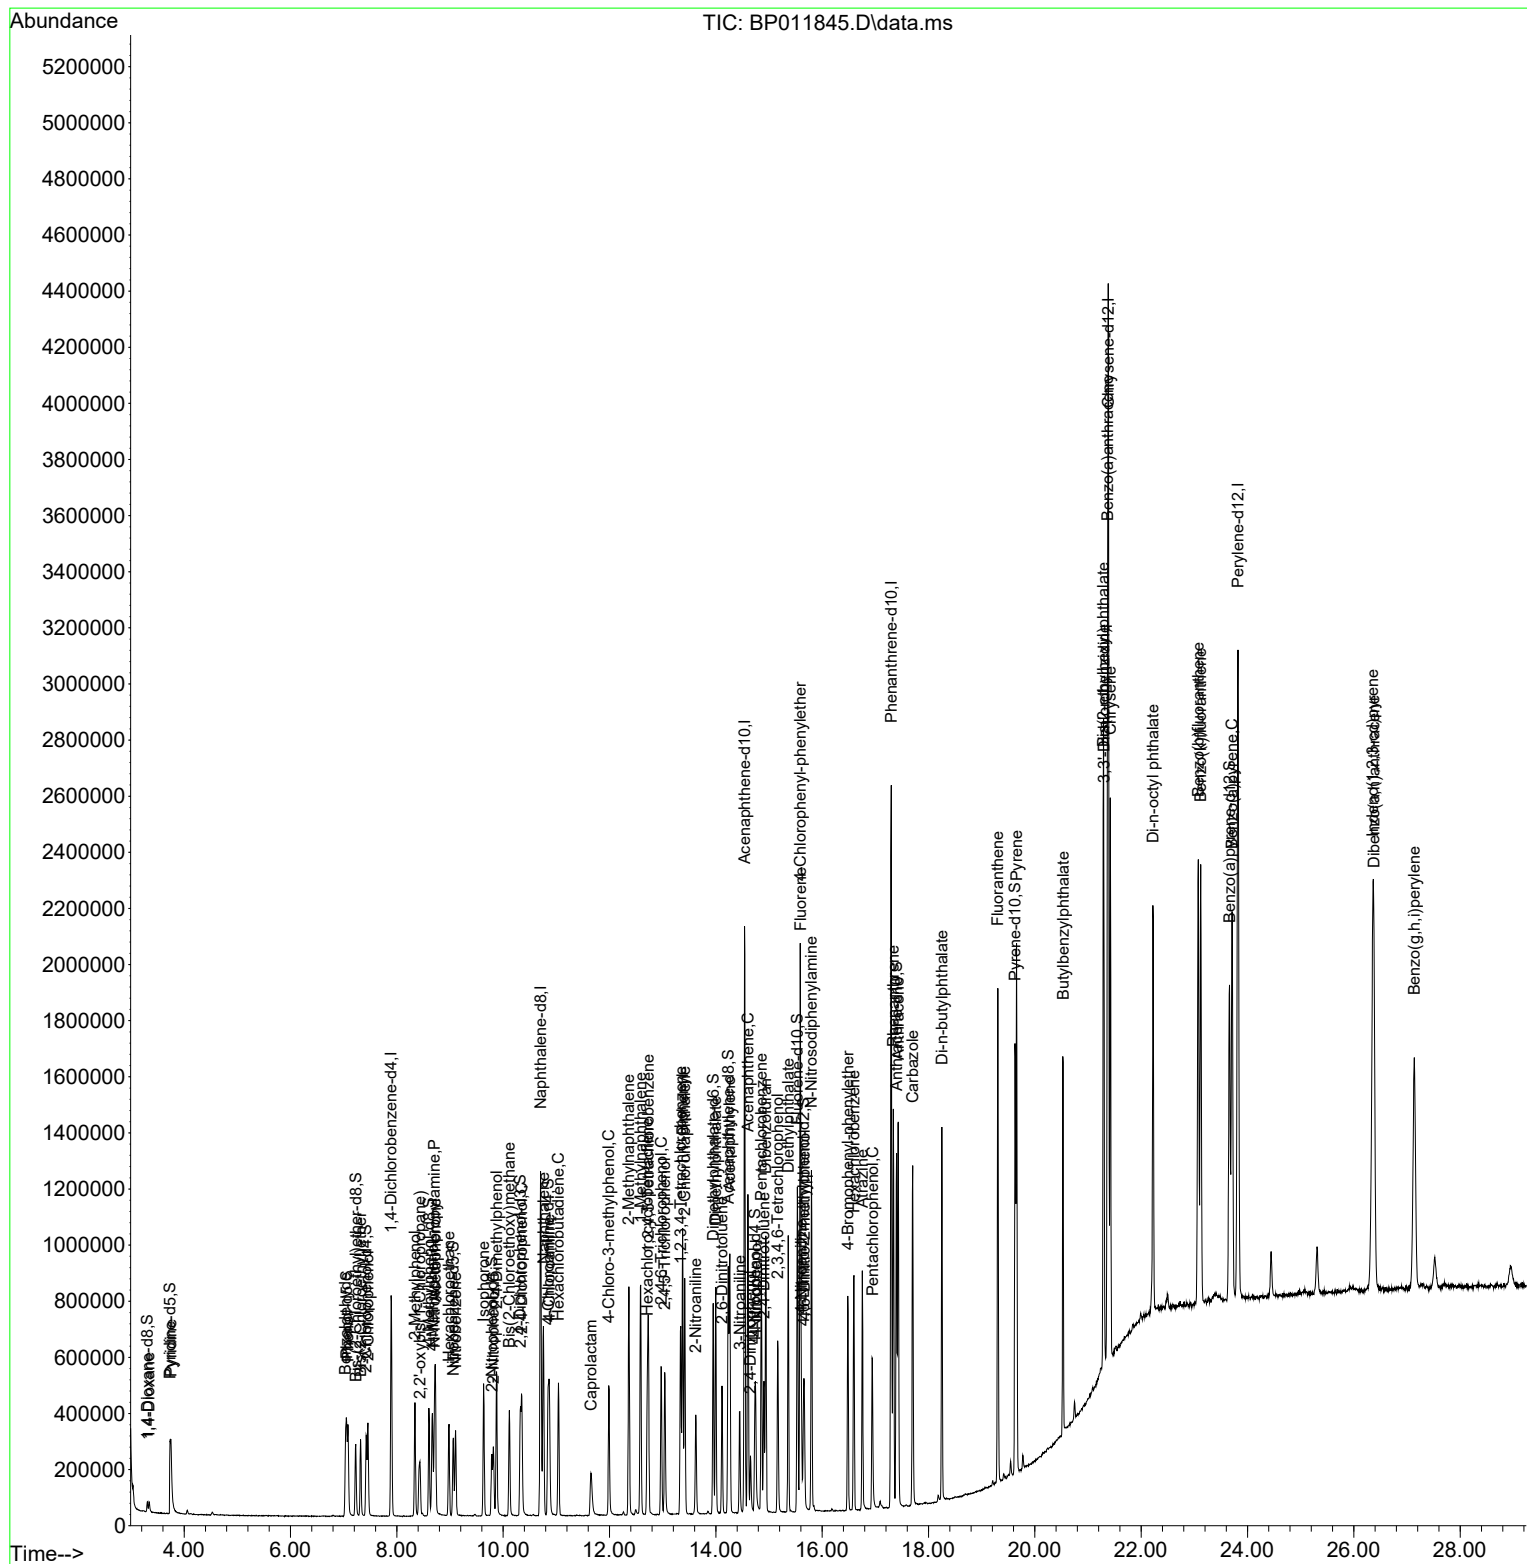


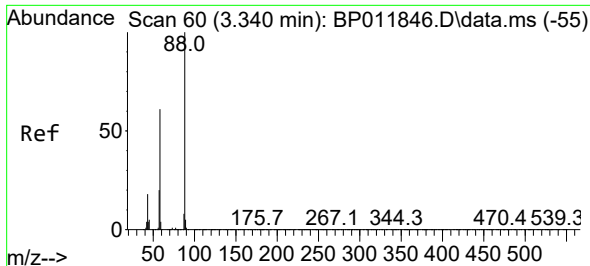

#2
1,4-Dioxane
Concen: 4.102 ng/uL
RT: 3.340 min Scan# 60
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion: 88 Resp: 23875
Ion Ratio Lower Upper
88 100
43 24.5 15.6 23.4#
58 65.2 48.6 72.8

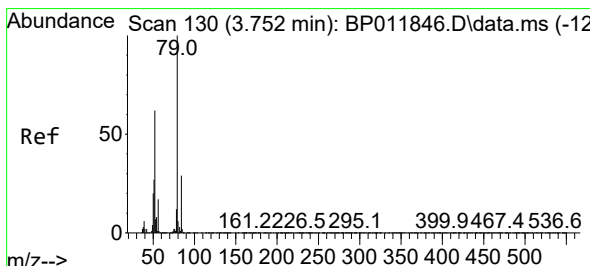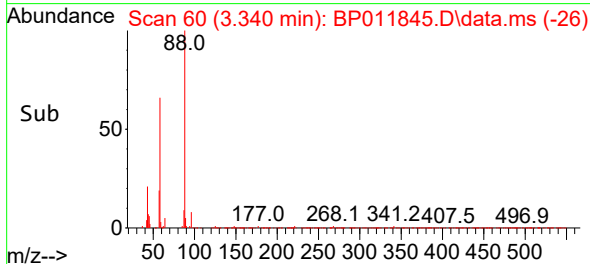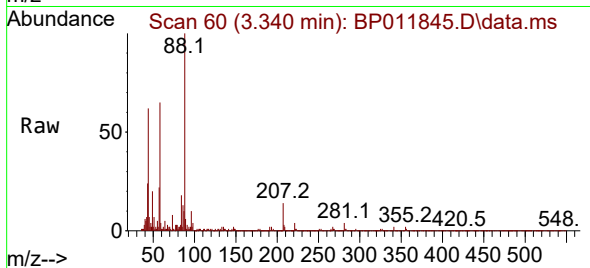

#5
Pyridine
Concen: 9.471 ng/uL
RT: 3.752 min Scan# 130
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion: 79 Resp: 143498
Ion Ratio Lower Upper
79 100
52 63.9 49.7 74.5
51 27.7 21.6 32.4


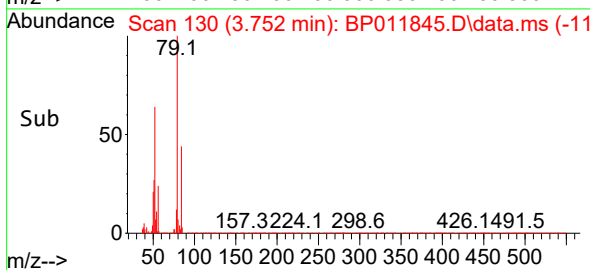

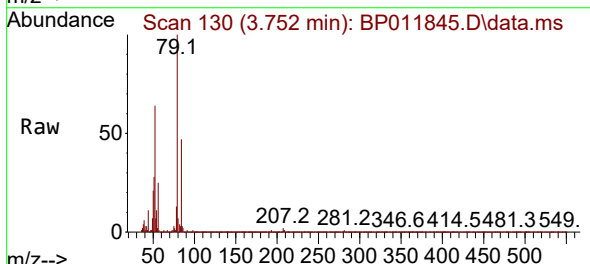




#6
Benzaldehyde
Concen: 10.527 ng/ul
RT: 7.034 min Scan# 688
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion: 77 Resp: 96749
Ion Ratio Lower Upper
77 100
105 103.1 87.0 130.6
106 100.4 83.8 125.6



#8
Phenol
Concen: 9.713 ng/ul
RT: 7.081 min Scan# 696
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion: 94 Resp: 199836
Ion Ratio Lower Upper
94 100
65 24.3 19.5 29.3
66 31.5 25.0 37.4



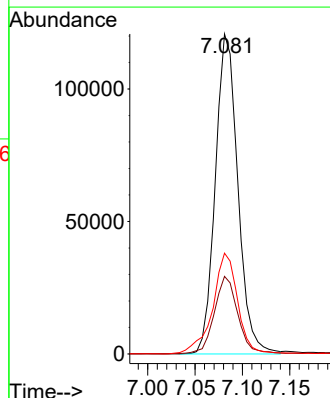





#10
Bis(2-Chloroethyl)ether
Concen: 10.302 ng/ul
RT: 7.316 min Scan# 71
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion: 93 Resp: 167278
Ion Ratio Lower Upper
93 100
63 70.3 56.2 84.4
95 33.2 25.9 38.9



#12
2-Chlorophenol
Concen: 10.485 ng/ul
RT: 7.457 min Scan# 760
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion:128 Resp: 170872
Ion Ratio Lower Upper
128 100
64 38.6 31.1 46.7
130 33.3 25.5 38.3



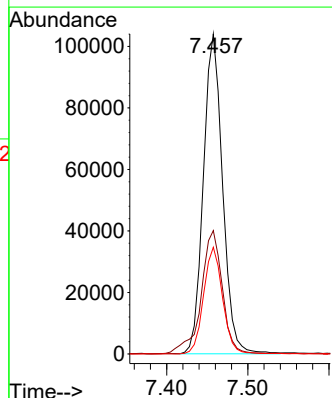





#13
2-Methylphenol
Concen: 10.030 ng/ul
RT: 8.340 min Scan# 910
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:108 Resp: 157085
Ion Ratio Lower Upper
108 100
107 87.4 70.2 105.2



#14
2,2'-oxybis(1-Chloropropane)
Concen: 8.046 ng/ul
RT: 8.434 min Scan# 926
Delta R.T. 0.006 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion: 45 Resp: 168044
Ion Ratio Lower Upper
45 100
77 19.4 16.0 24.0
79 15.3 12.5 18.7









#16
Acetophenone
Concen: 10.551 ng/ul
RT: 8.722 min Scan# 91
Delta R.T. -0.006 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:105 Resp: 261293
Ion Ratio Lower Upper
105 100
77 71.1 55.4 83.0
51 19.3 15.2 22.8

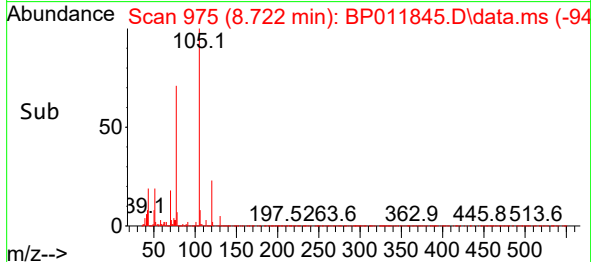

#17
N-Nitroso-di-n-propylamine
Concen: 10.662 ng/ul
RT: 8.704 min Scan# 972
Delta R.T. -0.006 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion: 70 Resp: 122956
Ion Ratio Lower Upper
70 100
42 40.2 32.7 49.1
101 10.4 8.4 12.6
130 24.8 19.4 29.2


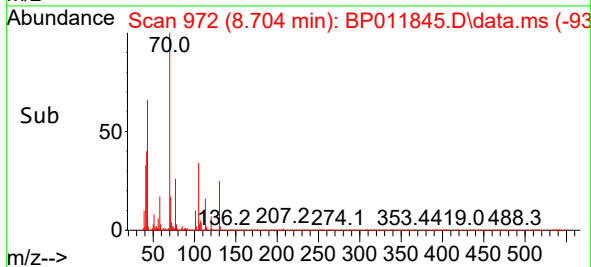

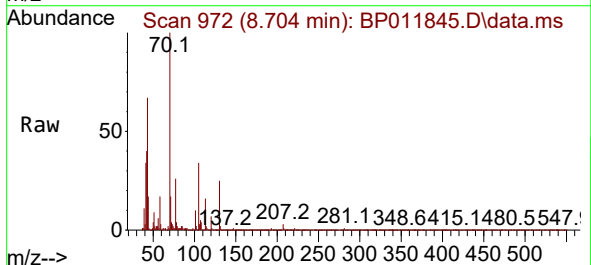




#18
4-Methylphenol
Concen: 10.379 ng/ul
RT: 8.669 min Scan# 966
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:108 Resp: 174075
Ion Ratio Lower Upper
108 100
107 110.1 88.0 132.0

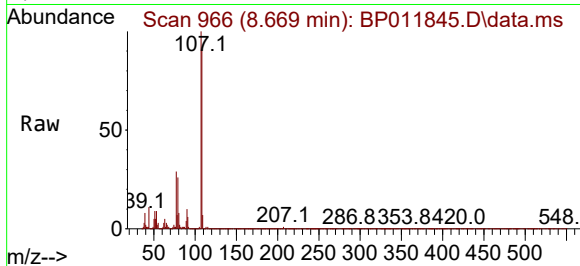

#19
Hexachloroethane
Concen: 10.032 ng/ul
RT: 8.981 min Scan# 1019
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion:117 Resp: 64627
Ion Ratio Lower Upper
117 100
201 101.9 82.4 123.6
199 64.3 51.6 77.4




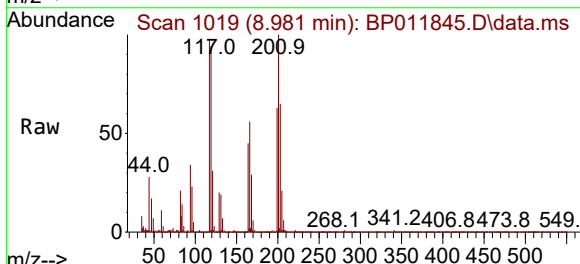




#22
Nitrobenzene
Concen: 10.417 ng/ul
RT: 9.104 min Scan# 1040
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion: 77 Resp: 177303
Ion Ratio Lower Upper
77 100
123 52.0 41.6 62.4
65 12.1 9.7 14.5

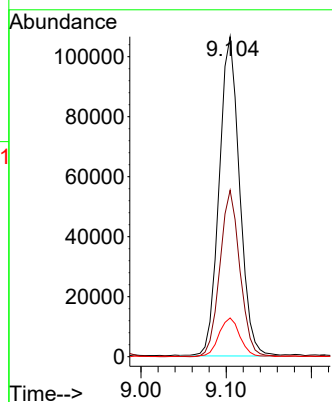

#23
Isophorone
Concen: 10.418 ng/ul
RT: 9.634 min Scan# 1130
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion: 82 Resp: 359289
Ion Ratio Lower Upper
82 100
95 6.8 5.4 8.2
138 20.2 15.8 23.8









#25
2-Nitrophenol
Concen: 13.357 ng/ul
RT: 9.816 min Scan# 1161
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion	Ratio	Lower	Upper
139	100		
65	41.9	32.2	48.4
109	25.0	19.6	29.4



#26
2,4-Dimethylphenol
Concen: 10.286 ng/ul
RT: 9.875 min Scan# 1171
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion	Ratio	Lower	Upper
107	100		
121	52.4	43.0	64.6
122	90.2	74.9	112.3



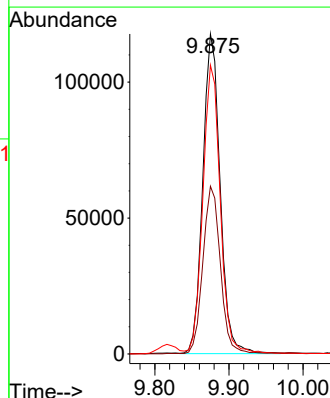





#27
 Bis(2-Chloroethoxy)methane
 Concen: 10.681 ng/ul
 RT: 10.116 min Scan# 1212
 Delta R.T. -0.000 min
 Lab File: BP011845.D
 Acq: 30 Sep 2022 17:37




Instrument :
 BNA_P
 ClientSampleId :
 SSTD010618


Tgt Ion: 93 Resp: 238697
 Ion Ratio Lower Upper
 93 100
 95 32.0 26.3 39.5
 123 12.1 9.5 14.3

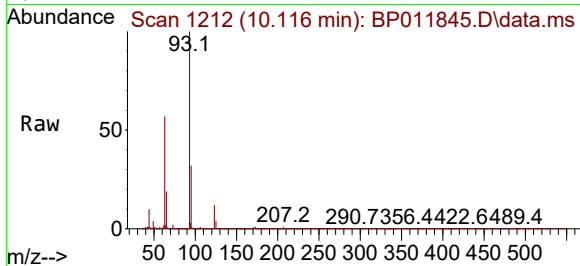

#29
 2,4-Dichlorophenol
 Concen: 10.599 ng/ul
 RT: 10.351 min Scan# 1252
 Delta R.T. -0.000 min
 Lab File: BP011845.D
 Acq: 30 Sep 2022 17:37

Tgt Ion:162 Resp: 169690
 Ion Ratio Lower Upper
 162 100
 164 66.5 52.2 78.4
 98 33.2 27.0 40.4




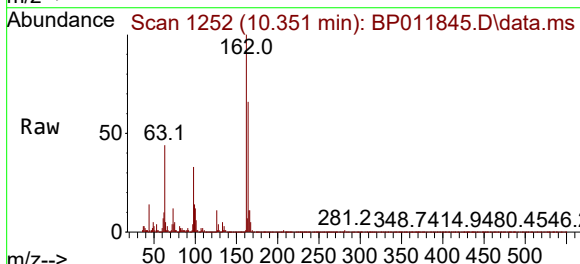




#30
Naphthalene
Concen: 10.521 ng/ul
RT: 10.757 min Scan# 11
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:128 Resp: 598850
Ion Ratio Lower Upper
128 100
129 11.2 8.9 13.3
127 13.1 10.5 15.7



#32
4-Chloroaniline
Concen: 10.530 ng/ul
RT: 10.869 min Scan# 1340
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion:127 Resp: 257106
Ion Ratio Lower Upper
127 100
129 30.6 26.6 39.8









#33
Hexachlorobutadiene
Concen: 9.541 ng/ul
RT: 11.040 min Scan# 11
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:225 Resp: 101726
Ion Ratio Lower Upper
225 100
223 63.2 52.1 78.1
227 62.3 52.3 78.5



#34
Caprolactam
Concen: 11.302 ng/ul
RT: 11.651 min Scan# 1473
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion:113 Resp: 53179
Ion Ratio Lower Upper
113 100
55 129.3 106.0 159.0
56 94.9 78.7 118.1









#35
4-Chloro-3-methylphenol
Concen: 11.274 ng/ul
RT: 11.987 min Scan# 1530
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:107 Resp: 179449
Ion Ratio Lower Upper
107 100
144 29.1 22.5 33.7
142 85.2 70.0 105.0



#36
2-Methylnaphthalene
Concen: 10.899 ng/ul
RT: 12.363 min Scan# 1594
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion:142 Resp: 415653
Ion Ratio Lower Upper
142 100
141 90.1 70.6 106.0





#37

1-Methylnaphthalene

Concen: 11.034 ng/ul

RT: 12.587 min Scan# 1

Delta R.T. -0.000 min

Lab File: BP011845.D

Acq: 30 Sep 2022 17:37

Instrument :

BNA_P

ClientSampleId :

SSTD010618





Tgt Ion:142 Resp: 421774

Ion Ratio Lower Upper

142 100

141 91.9 74.8 112.2

116 3.4 2.9 4.3

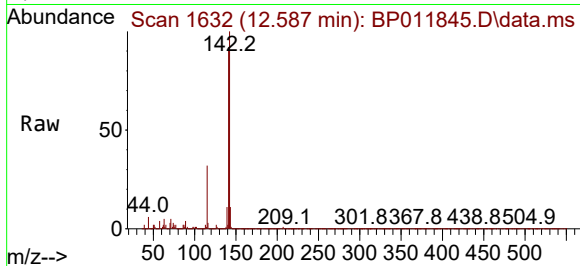

#39

1,2,4,5-Tetrachlorobenzene

Concen: 9.362 ng/ul

RT: 12.728 min Scan# 1656

Delta R.T. -0.006 min

Lab File: BP011845.D

Acq: 30 Sep 2022 17:37

Tgt Ion:216 Resp: 211584




Ion Ratio Lower Upper


216 100

214 79.5 62.6 94.0

179 20.9 16.6 24.8

108 17.1 12.6 19.0

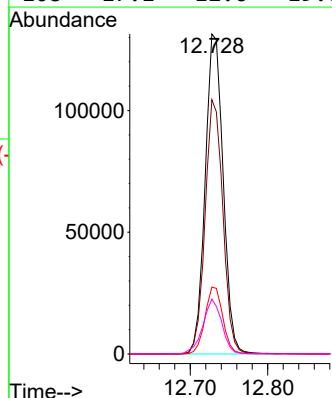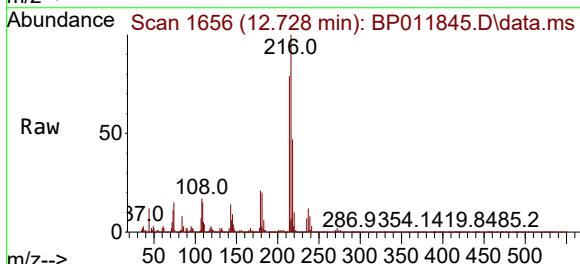



#40

Hexachlorocyclopentadiene

Concen: 8.225 ng/ul

RT: 12.710 min Scan# 1653

Delta R.T. -0.000 min

Lab File: BP011845.D

Acq: 30 Sep 2022 17:37

Instrument :

BNA_P

ClientSampleId :

SSTD010618





Tgt Ion:237 Resp: 110532

Ion Ratio Lower Upper

237 100

235 63.8 51.0 76.6

272 13.6 10.5 15.7

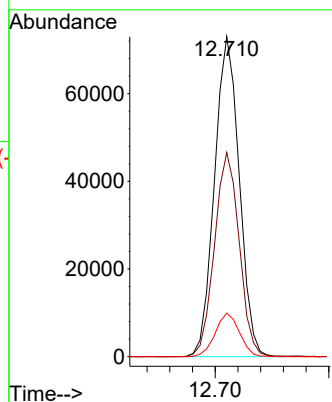

#41

2,4,6-Trichlorophenol

Concen: 10.808 ng/ul

RT: 12.975 min Scan# 1698

Delta R.T. -0.000 min

Lab File: BP011845.D

Acq: 30 Sep 2022 17:37




Tgt Ion:196 Resp: 138144


Ion Ratio Lower Upper

196 100

198 95.0 78.7 118.1

200 30.8 24.5 36.7



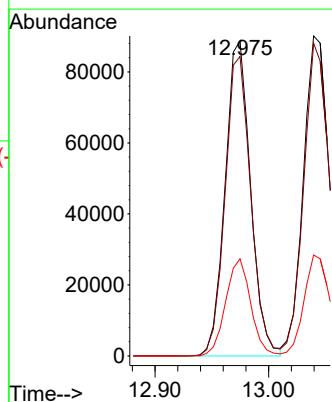





#42
2,4,5-Trichlorophenol
Concen: 10.478 ng/ul
RT: 13.040 min Scan# 1710
Delta R.T. -0.006 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:196 Resp: 147103
Ion Ratio Lower Upper
196 100
198 97.8 76.6 114.8
200 31.5 25.6 38.4



#43
1,1'-Biphenyl
Concen: 9.817 ng/ul
RT: 13.375 min Scan# 1766
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion:154 Resp: 549396
Ion Ratio Lower Upper
154 100
153 40.5 31.8 47.6
76 12.3 9.5 14.3







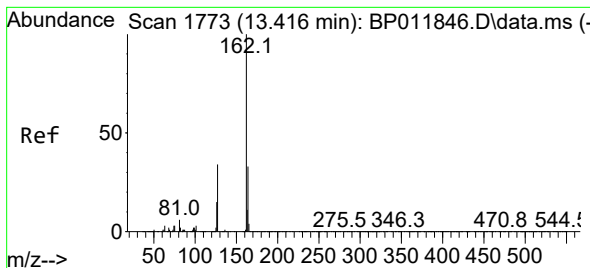

#44
2-Chloronaphthalene
Concen: 9.990 ng/ul
RT: 13.416 min Scan# 1773
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument : BNA_P
ClientSampleId : SSTD010618


Tgt Ion:162 Resp: 428121
Ion Ratio Lower Upper
162 100
164 32.8 26.5 39.7
127 38.0 29.7 44.5

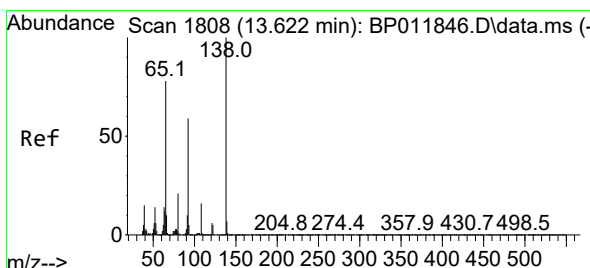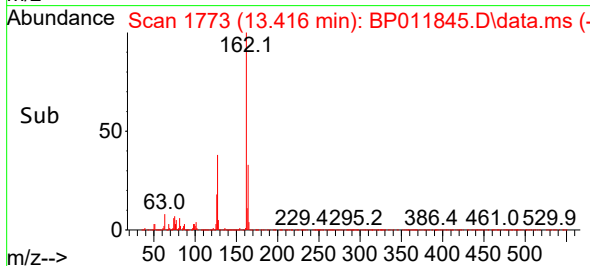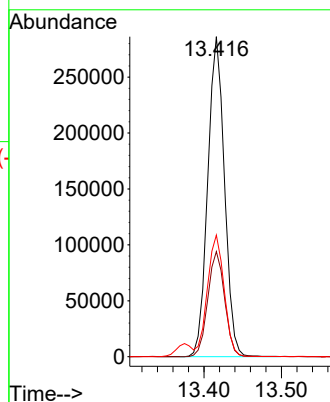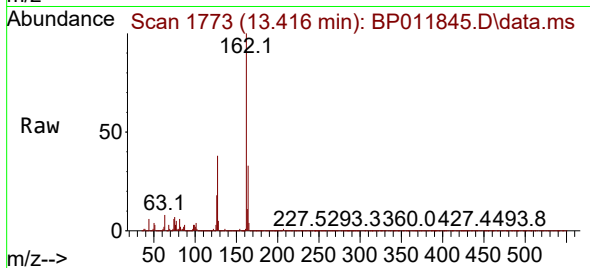

#45
2-Nitroaniline
Concen: 11.033 ng/ul
RT: 13.622 min Scan# 1808
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion: 65 Resp: 97945
Ion Ratio Lower Upper
65 100
92 77.6 61.2 91.8
138 134.0 103.0 154.4


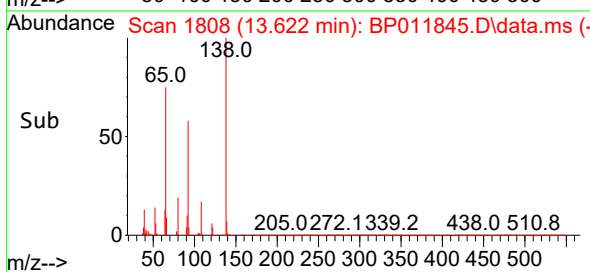
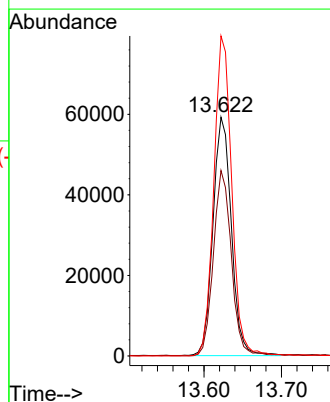
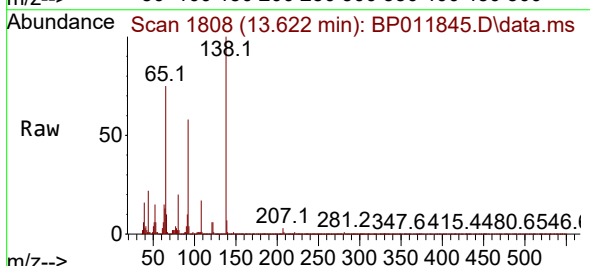




#47
Dimethylphthalate
Concen: 10.821 ng/ul
RT: 13.998 min Scan# 1872
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:163 Resp: 553499
Ion Ratio Lower Upper
163 100
194 4.0 3.3 4.9
164 9.9 8.5 12.7

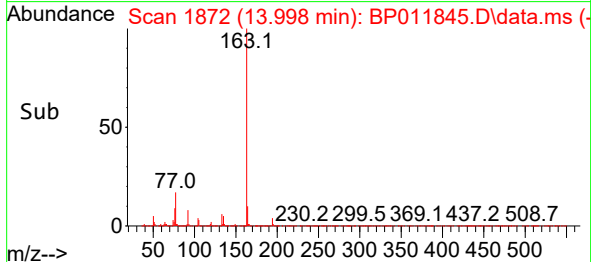

#48
2,6-Dinitrotoluene
Concen: 12.183 ng/ul
RT: 14.116 min Scan# 1892
Delta R.T. -0.006 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion:165 Resp: 99868
Ion Ratio Lower Upper
165 100
89 54.5 39.1 58.7
121 22.8 16.7 25.1


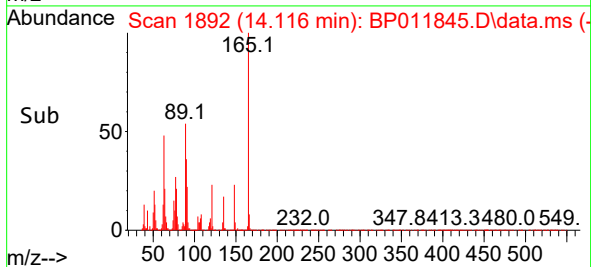

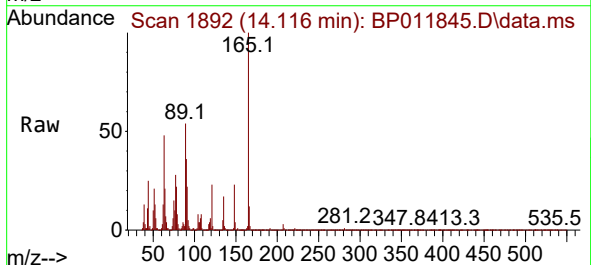




#50
Acenaphthylene
Concen: 9.852 ng/ul
RT: 14.263 min Scan# 1917
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:152 Resp: 671319
Ion Ratio Lower Upper
152 100
151 19.9 16.0 24.0
153 13.1 10.8 16.2



#51
3-Nitroaniline
Concen: 11.088 ng/ul
RT: 14.451 min Scan# 1949
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion:138 Resp: 108730
Ion Ratio Lower Upper
138 100
108 10.8 8.2 12.4
92 105.1 85.6 128.4



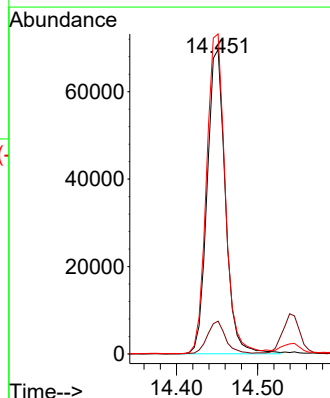





#52
Acenaphthene
Concen: 10.667 ng/ul
RT: 14.604 min Scan# 1975
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:153 Resp: 475281
Ion Ratio Lower Upper
153 100
152 46.9 38.4 57.6
154 89.9 70.6 105.8



#53
2,4-Dinitrophenol
Concen: 14.269 ng/ul
RT: 14.651 min Scan# 1983
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion:184 Resp: 51209
Ion Ratio Lower Upper
184 100
63 56.7 44.2 66.4
154 56.1 45.8 68.6



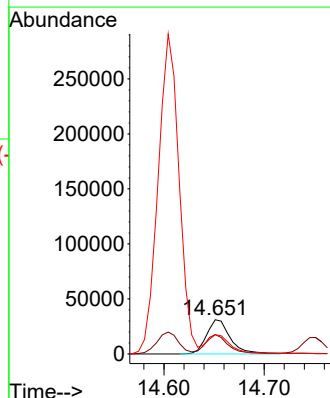





#55
4-Nitrophenol
Concen: 9.700 ng/ul
RT: 14.751 min Scan# 2000
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:109 Resp: 64884
Ion Ratio Lower Upper
109 100
139 162.0 125.0 187.6
65 128.3 101.9 152.9

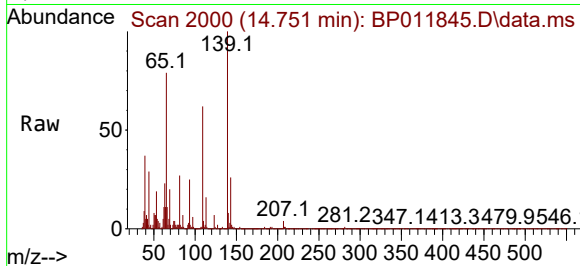

#56
Dibenzofuran
Concen: 10.394 ng/ul
RT: 14.939 min Scan# 2032
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion:168 Resp: 656961
Ion Ratio Lower Upper
168 100
139 35.4 29.4 44.2



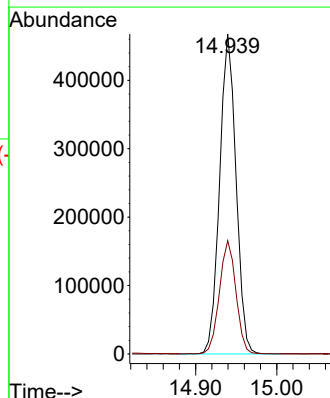
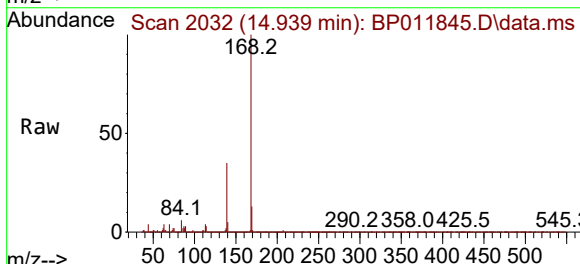




#57
2,4-Dinitrotoluene
Concen: 13.076 ng/ul
RT: 14.904 min Scan# 2026
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:165 Resp: 149253
Ion Ratio Lower Upper
165 100
63 35.4 28.2 42.2
182 2.6 2.2 3.4



#58
2,3,4,6-Tetrachlorophenol
Concen: 12.277 ng/ul
RT: 15.163 min Scan# 2070
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion:232 Resp: 129786
Ion Ratio Lower Upper
232 100
131 44.9 36.2 54.2
130 2.5 1.7 2.5
166 31.3 25.0 37.4



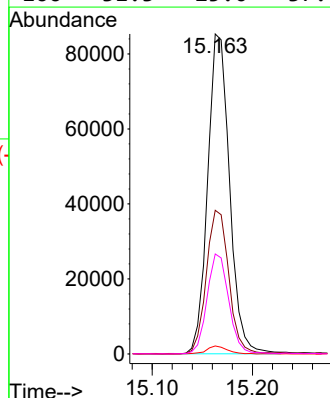





#59
Diethylphthalate
Concen: 11.125 ng/ul
RT: 15.363 min Scan# 2104
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:149 Resp: 554166
Ion Ratio Lower Upper
149 100
177 22.2 17.8 26.8
150 12.4 9.9 14.9

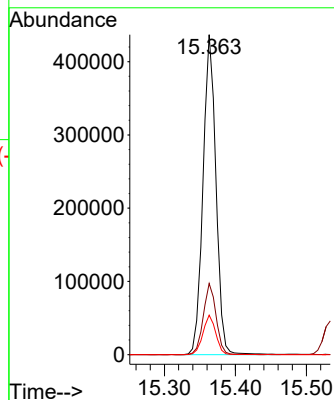

#61
Fluorene
Concen: 10.664 ng/ul
RT: 15.592 min Scan# 2143
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion:166 Resp: 544809
Ion Ratio Lower Upper
166 100
165 98.9 77.2 115.8
167 13.6 10.7 16.1



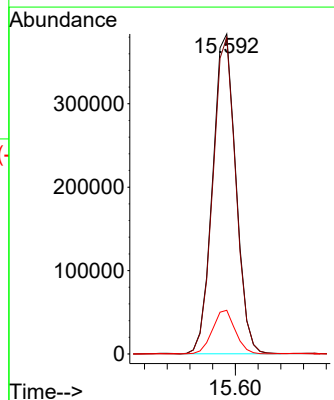





#62
4-Chlorophenyl-phenylether
Concen: 10.278 ng/ul
RT: 15.586 min Scan# 2142
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:204 Resp: 266120
Ion Ratio Lower Upper
204 100
206 33.1 26.8 40.2
141 55.5 44.5 66.7



#63
4-Nitroaniline
Concen: 11.770 ng/ul
RT: 15.610 min Scan# 2146
Delta R.T. -0.006 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion:138 Resp: 108925
Ion Ratio Lower Upper
138 100
92 47.6 35.9 53.9
108 66.0 51.6 77.4


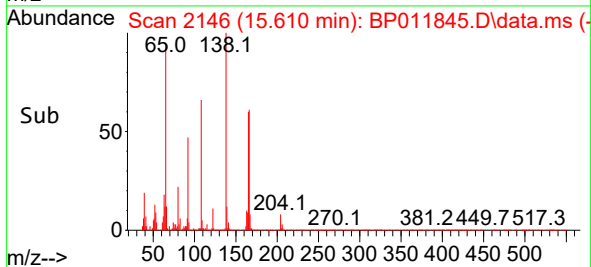

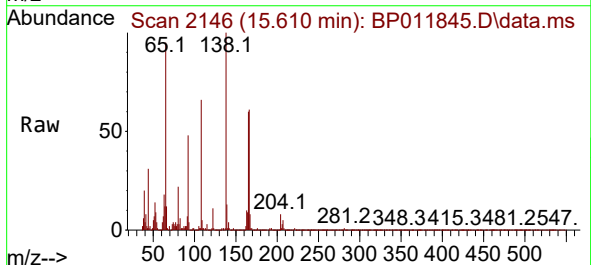




#66
4,6-Dinitro-2-methylphenol
Concen: 13.589 ng/ul
RT: 15.663 min Scan# 2156
Delta R.T. -0.006 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:198 Resp: 86161
Ion Ratio Lower Upper
198 100
182 6.3 3.7 5.5#
77 23.6 16.6 24.8

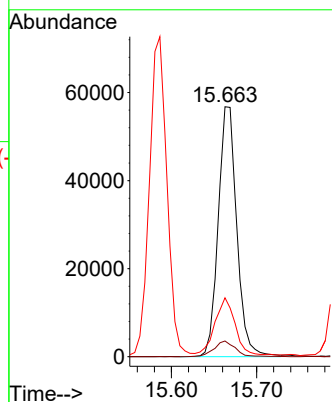

#67
N-Nitrosodiphenylamine
Concen: 10.388 ng/ul
RT: 15.798 min Scan# 2178
Delta R.T. -0.006 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion:169 Resp: 469681
Ion Ratio Lower Upper
169 100
168 66.3 53.7 80.5
167 36.6 29.9 44.9


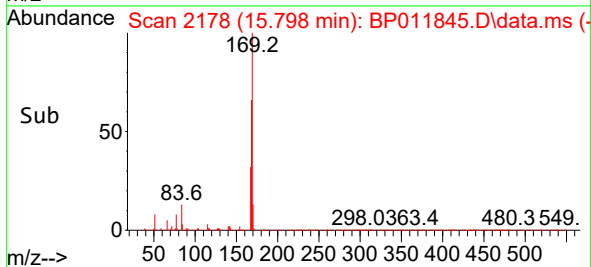
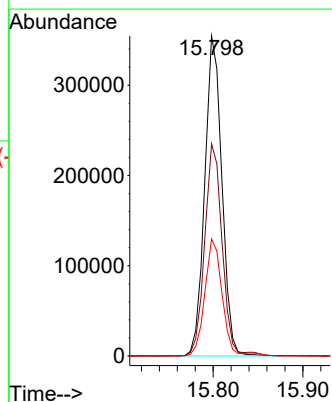
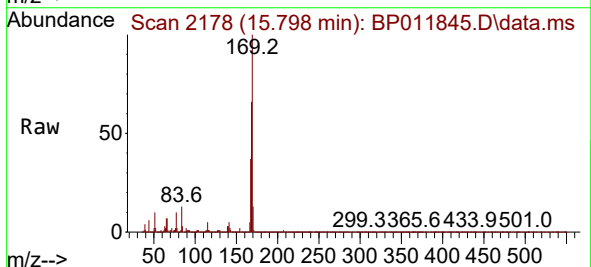




#68
4-Bromophenyl-phenylether
Concen: 9.584 ng/ul
RT: 16.486 min Scan# 2295
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:248 Resp: 156351
Ion Ratio Lower Upper
248 100
250 99.9 78.6 118.0
141 69.9 56.0 84.0



#69
Hexachlorobenzene
Concen: 9.241 ng/ul
RT: 16.598 min Scan# 2314
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion:284 Resp: 178863
Ion Ratio Lower Upper
284 100
142 33.8 27.3 40.9
249 30.0 25.2 37.8









#70
Atrazine
Concen: 9.756 ng/ul
RT: 16.757 min Scan# 21
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:200 Resp: 160083
Ion Ratio Lower Upper
200 100
173 26.9 21.6 32.4
215 49.9 38.9 58.3

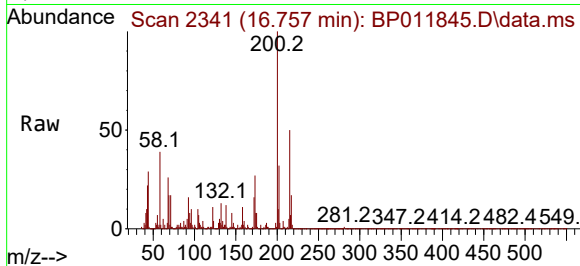

#71
Pentachlorophenol
Concen: 10.194 ng/ul
RT: 16.945 min Scan# 2373
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion:266 Resp: 105434
Ion Ratio Lower Upper
266 100
264 63.3 49.8 74.8
268 65.0 51.9 77.9

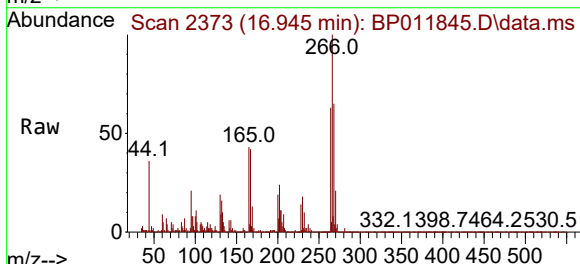



#72

Phenanthrene

Concen: 10.590 ng/ul

RT: 17.339 min Scan# 2440

Delta R.T. -0.000 min

Lab File: BP011845.D

Acq: 30 Sep 2022 17:37

Instrument :

BNA_P

ClientSampleId :

SSTD010618





Tgt Ion:178 Resp: 875003

Ion Ratio Lower Upper

178 100

179 15.1 12.5 18.7

176 18.9 15.4 23.2

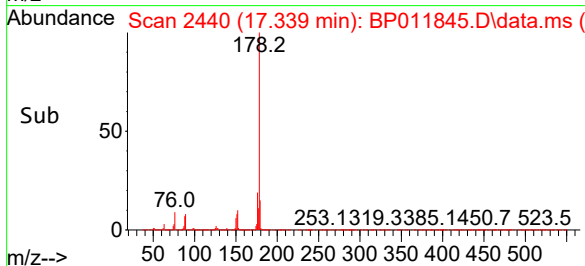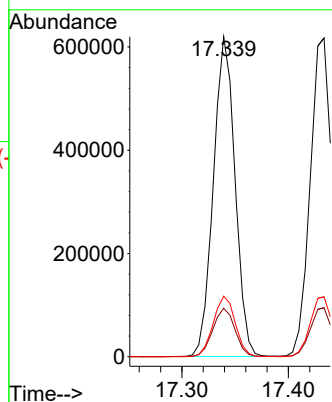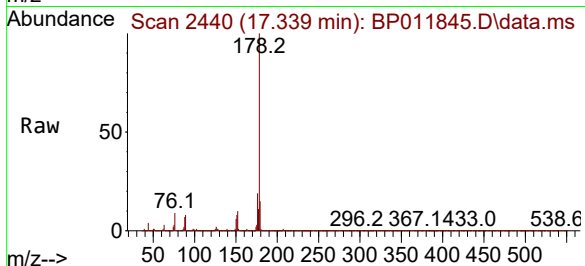

#74

Anthracene

Concen: 10.813 ng/ul

RT: 17.433 min Scan# 2456

Delta R.T. -0.000 min

Lab File: BP011845.D

Acq: 30 Sep 2022 17:37




Tgt Ion:178 Resp: 894558


Ion Ratio Lower Upper

178 100

179 15.4 12.3 18.5

176 18.8 15.4 23.2

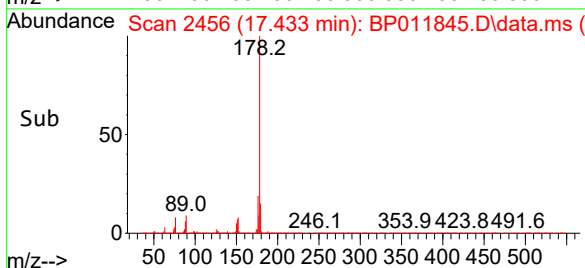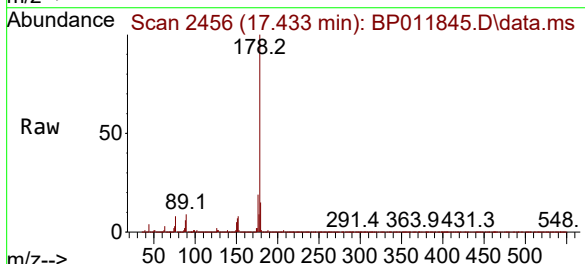



#75

1,2,3,4-Tetrachlorobenzene

Concen: 8.846 ng/uL

RT: 13.340 min Scan# 1760

Delta R.T. -0.000 min

Lab File: BP011845.D

Acq: 30 Sep 2022 17:37

Instrument :

BNA_P

ClientSampleId :

SSTD010618





Tgt Ion:216 Resp: 214918

Ion Ratio Lower Upper

216 100

214 77.5 62.6 93.8

218 48.2 37.4 56.0

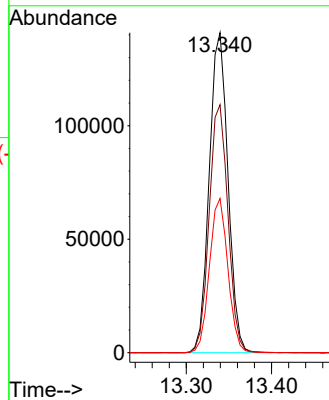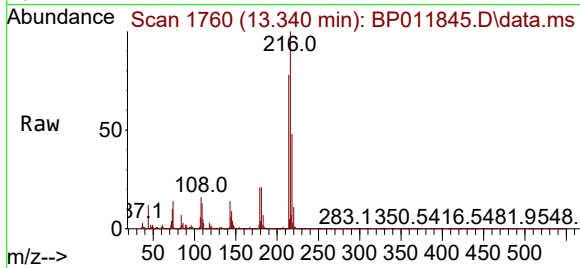

#76

Pentachlorobenzene

Concen: 10.178 ng/uL

RT: 14.857 min Scan# 2018

Delta R.T. -0.000 min

Lab File: BP011845.D

Acq: 30 Sep 2022 17:37




Tgt Ion:250 Resp: 233518


Ion Ratio Lower Upper

250 100

248 62.5 51.4 77.0

252 63.1 51.5 77.3

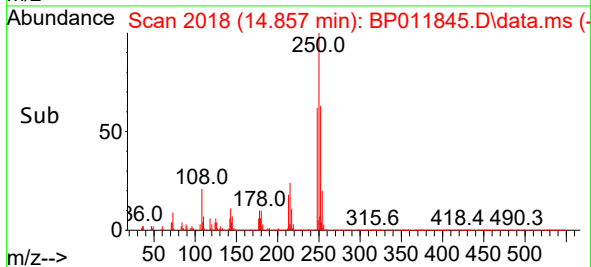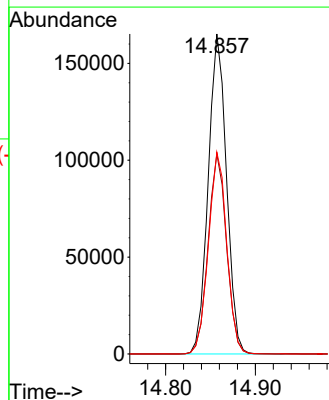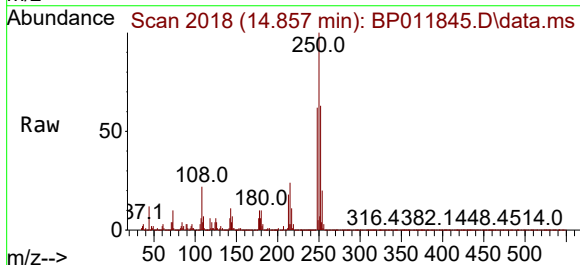



#77

Carbazole

Concen: 10.899 ng/ul

RT: 17.704 min Scan# 2502

Delta R.T. -0.000 min

Lab File: BP011845.D

Acq: 30 Sep 2022 17:37

Instrument :

BNA_P

ClientSampleId :

SSTD010618





Tgt Ion:167 Resp: 794540

Ion Ratio Lower Upper

167 100

166 21.3 17.1 25.7

139 12.8 10.1 15.1

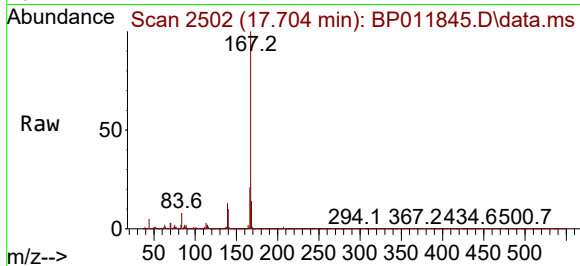

#78

Di-n-butylphthalate

Concen: 11.508 ng/ul

RT: 18.251 min Scan# 2595

Delta R.T. -0.000 min

Lab File: BP011845.D

Acq: 30 Sep 2022 17:37




Tgt Ion:149 Resp: 952250


Ion Ratio Lower Upper

149 100

150 9.3 7.5 11.3

104 4.3 3.6 5.4

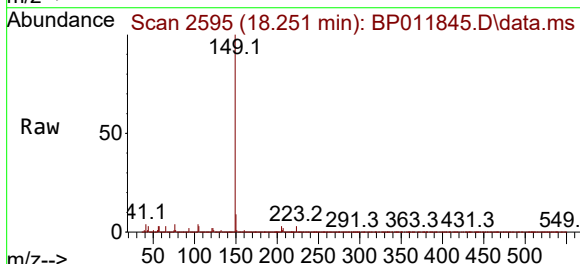



#80

Fluoranthene

Concen: 10.158 ng/ul

RT: 19.304 min Scan# 21

Delta R.T. -0.000 min

Lab File: BP011845.D

Acq: 30 Sep 2022 17:37

Instrument :

BNA_P

ClientSampleId :

SSTD010618





Tgt Ion:202 Resp: 1007946

Ion Ratio Lower Upper

202 100

101 11.6 9.8 14.6

100 8.7 7.4 11.0

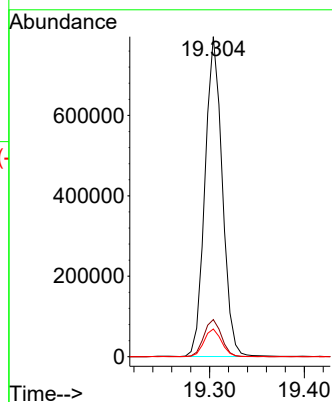

#82

Pyrene

Concen: 10.322 ng/ul

RT: 19.657 min Scan# 2834

Delta R.T. -0.000 min

Lab File: BP011845.D

Acq: 30 Sep 2022 17:37




Tgt Ion:202 Resp: 1056619


Ion Ratio Lower Upper

202 100

101 13.6 11.6 17.4

100 11.3 9.4 14.0





#83

Butylbenzylphthalate

Concen: 12.982 ng/ul

RT: 20.533 min Scan# 2983

Delta R.T. -0.000 min

Lab File: BP011845.D

Acq: 30 Sep 2022 17:37

Instrument :

BNA_P

ClientSampleId :

SSTD010618





Tgt Ion:149 Resp: 430859

Ion Ratio Lower Upper

149 100

91 62.9 50.2 75.4

206 20.7 16.9 25.3

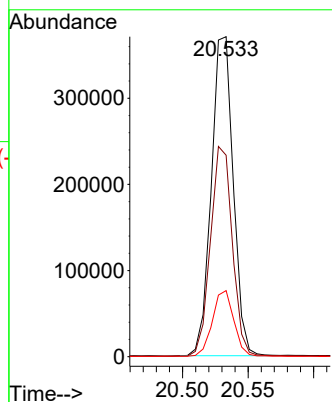

#84

3,3'-Dichlorobenzidine

Concen: 12.887 ng/ul

RT: 21.298 min Scan# 3113

Delta R.T. -0.006 min

Lab File: BP011845.D

Acq: 30 Sep 2022 17:37




Tgt Ion:252 Resp: 362442


Ion Ratio Lower Upper

252 100

254 63.6 51.4 77.0

126 12.6 8.9 13.3









#85
Benzo(a)anthracene
Concen: 10.803 ng/ul
RT: 21.369 min Scan# 3111
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:228 Resp: 1057142
Ion Ratio Lower Upper
228 100
229 20.1 15.8 23.6
226 27.1 22.0 33.0

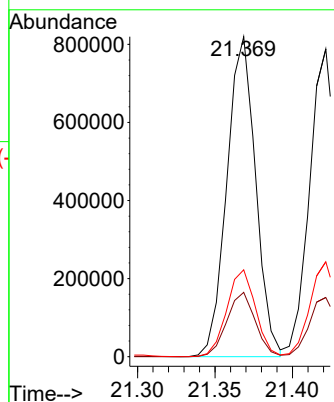

#86
Bis(2-ethylhexyl)phthalate
Concen: 12.548 ng/ul
RT: 21.286 min Scan# 3111
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion:149 Resp: 664317
Ion Ratio Lower Upper
149 100
167 26.3 21.2 31.8
279 3.9 2.9 4.3



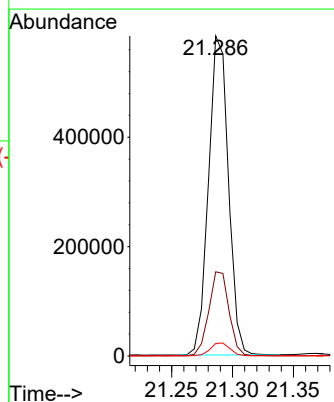





#87
Chrysene
Concen: 10.588 ng/ul
RT: 21.421 min Scan# 3134
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:228 Resp: 1000546
Ion Ratio Lower Upper
228 100
226 30.8 25.3 37.9
229 19.3 16.2 24.2



#89
Di-n-octyl phthalate
Concen: 11.621 ng/ul
RT: 22.221 min Scan# 3270
Delta R.T. -0.006 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion:149 Resp: 1114703









#90
Benzo(b)fluoranthene
Concen: 10.264 ng/ul
RT: 23.074 min Scan# 3415
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37




Instrument :
BNA_P
ClientSampleId :
SSTD010618


Tgt Ion:252 Resp: 1119559
Ion Ratio Lower Upper
252 100
253 22.1 17.8 26.8
125 11.1 9.2 13.8



#91
Benzo(k)fluoranthene
Concen: 10.223 ng/ul
RT: 23.121 min Scan# 3423
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion:252 Resp: 1067421
Ion Ratio Lower Upper
252 100
253 21.6 18.0 27.0
125 11.1 9.2 13.8





#93

Benzo(a)pyrene

Concen: 9.322 ng/ul

RT: 23.710 min Scan# 3

Delta R.T. -0.006 min

Lab File: BP011845.D

Acq: 30 Sep 2022 17:37

Instrument :

BNA_P

ClientSampleId :

SSTD010618





Tgt Ion:252 Resp: 985678

Ion Ratio Lower Upper

252 100

253 22.0 17.7 26.5

125 12.7 9.8 14.8

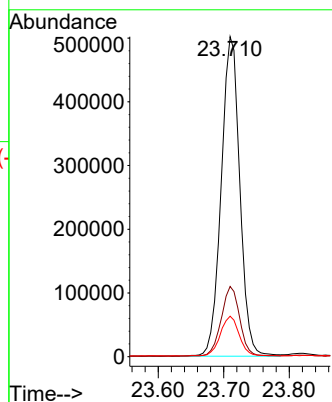

#94

Indeno(1,2,3-cd)pyrene

Concen: 10.112 ng/ul

RT: 26.356 min Scan# 3973

Delta R.T. -0.006 min

Lab File: BP011845.D

Acq: 30 Sep 2022 17:37




Tgt Ion:276 Resp: 1233990


Ion Ratio Lower Upper

276 100

138 26.4 21.4 32.0

277 24.8 19.9 29.9









#95
Dibenzo(a,h)anthracene
Concen: 10.560 ng/ul
RT: 26.380 min Scan# 3977
Delta R.T. -0.000 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Instrument :
BNA_P
ClientSampleId :
SSTD010618

Tgt Ion:278 Resp: 1111109
Ion Ratio Lower Upper
278 100
139 18.3 15.0 22.6
279 24.1 19.0 28.6



#96
Benzo(g,h,i)perylene
Concen: 10.719 ng/ul
RT: 27.139 min Scan# 4106
Delta R.T. -0.006 min
Lab File: BP011845.D
Acq: 30 Sep 2022 17:37

Tgt Ion:276 Resp: 1091190
Ion Ratio Lower Upper
276 100
138 24.5 19.8 29.6
277 23.3 18.6 27.8

