

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093022\
 Data File : BP011846.D
 Acq On : 30 Sep 2022 18:12
 Operator : CG/JU
 Sample : SST02058
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST020619

Quant Time: Oct 01 00:03:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 30 23:58:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	235951	20.000	ng/u1	0.00
20) Naphthalene-d8	10.704	136	1099376	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.540	164	725838	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.298	188	1537351	20.000	ng/u1	0.00
79) Chrysene-d12	21.386	240	1586654	20.000	ng/u1	0.00
88) Perylene-d12	23.821	264	1728712	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	46726	8.740	ng/uL	0.00
4) Pyridine-d5	3.734	84	337961	22.736	ng/u1	0.00
7) Phenol-d5	7.058	99	434766	22.264	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	250980	21.516	ng/u1	0.00
11) 2-Chlorophenol-d4	7.422	132	355171	23.818	ng/u1	0.00
15) 4-Methylphenol-d8	8.605	113	366605	24.486	ng/u1	0.00
21) Nitrobenzene-d5	9.063	128	185562	25.899	ng/u1	0.00
24) 2-Nitrophenol-d4	9.787	143	199975	32.904	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	369550	23.752	ng/u1	0.00
31) 4-Chloroaniline-d4	10.846	131	558919	23.530	ng/u1	0.00
46) Dimethylphthalate-d6	13.951	166	1154712	23.635	ng/u1	0.00
49) Acenaphthylene-d8	14.234	160	1332849	22.842	ng/u1	0.00
54) 4-Nitrophenol-d4	14.740	143	232805	27.070	ng/u1	0.00
60) Fluorene-d10	15.534	176	999986	23.058	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	195615	34.379	ng/u1	0.00
73) Anthracene-d10	17.398	188	1576228	23.146	ng/u1	0.00
81) Pyrene-d10	19.633	212	1782517	21.986	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.663	264	1927558	22.953	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.340	88	49969	8.859	ng/uL	100
5) Pyridine	3.752	79	328839	22.397	ng/u1	100
6) Benzaldehyde	7.034	77	228858	25.695	ng/u1	100
8) Phenol	7.081	94	457373	22.941	ng/u1	100
10) Bis(2-Chloroethyl)ether	7.316	93	372569	23.678	ng/u1	100
12) 2-Chlorophenol	7.458	128	380865	24.117	ng/u1	100
13) 2-Methylphenol	8.340	108	362702	23.897	ng/u1	100
14) 2,2'-oxybis(1-Chloropr...	8.428	45	372581	18.408	ng/u1	100
16) Acetophenone	8.728	105	583435	24.312	ng/u1	100
17) N-Nitroso-di-n-propyla...	8.710	70	275724	24.673	ng/u1	100
18) 4-Methylphenol	8.669	108	402432	24.760	ng/u1	100
19) Hexachloroethane	8.981	117	140030	22.431	ng/u1	100
22) Nitrobenzene	9.105	77	400458	23.672	ng/u1	100
23) Isophorone	9.634	82	818382	23.877	ng/u1	100
25) 2-Nitrophenol	9.816	139	230859	31.483	ng/u1	100
26) 2,4-Dimethylphenol	9.875	107	428212	23.166	ng/u1	100
27) Bis(2-Chloroethoxy)met...	10.116	93	526112	23.686	ng/u1	100
29) 2,4-Dichlorophenol	10.352	162	382890	24.063	ng/u1	100
30) Naphthalene	10.757	128	1308500	23.131	ng/u1	100
32) 4-Chloroaniline	10.869	127	575411	23.710	ng/u1	100
33) Hexachlorobutadiene	11.040	225	219721	20.734	ng/u1	100
34) Caprolactam	11.651	113	130219	27.846	ng/u1	100
35) 4-Chloro-3-methylphenol	11.987	107	405580	25.638	ng/u1	100
36) 2-Methylnaphthalene	12.363	142	915438	24.152	ng/u1	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093022\
 Data File : BP011846.D
 Acq On : 30 Sep 2022 18:12
 Operator : CG/JU
 Sample : SST02058
 Misc :
 ALS Vial : 4 Sample Multiplier: 1


Instrument :
 BNA_P
 ClientSampleId :
 SST020619


Quant Time: Oct 01 00:03:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 30 23:58:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.587	142	919649	24.207	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.734	216	464398	21.018	ng/ul	100
40) Hexachlorocyclopentadiene	12.710	237	255281	19.432	ng/ul	100
41) 2,4,6-Trichlorophenol	12.975	196	311423	24.923	ng/ul	100
42) 2,4,5-Trichlorophenol	13.045	196	339991	24.773	ng/ul	100
43) 1,1'-Biphenyl	13.375	154	1198633	21.909	ng/ul	100
44) 2-Chloronaphthalene	13.416	162	947611	22.619	ng/ul	100
45) 2-Nitroaniline	13.622	65	236080	27.203	ng/ul	100
47) Dimethylphthalate	13.998	163	1204055	24.078	ng/ul	100
48) 2,6-Dinitrotoluene	14.122	165	235738	29.417	ng/ul	100
50) Acenaphthylene	14.263	152	1484022	22.279	ng/ul	100
51) 3-Nitroaniline	14.451	138	273256	28.504	ng/ul	100
52) Acenaphthene	14.604	153	1033894	23.735	ng/ul	100
53) 2,4-Dinitrophenol	14.651	184	140397	40.016	ng/ul	100
55) 4-Nitrophenol	14.751	109	158854	24.292	ng/ul	100
56) Dibenzofuran	14.940	168	1413762	22.880	ng/ul	100
57) 2,4-Dinitrotoluene	14.904	165	346857	31.083	ng/ul	100
58) 2,3,4,6-Tetrachlorophenol	15.163	232	295621	28.605	ng/ul	100
59) Diethylphthalate	15.363	149	1216954	24.991	ng/ul	100
61) Fluorene	15.592	166	1168986	23.405	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.587	204	570464	22.536	ng/ul	100
63) 4-Nitroaniline	15.616	138	275840	30.488	ng/ul	100
66) 4,6-Dinitro-2-methylph...	15.669	198	211501	34.317	ng/ul	100
67) N-Nitrosodiphenylamine	15.804	169	1020628	23.222	ng/ul	100
68) 4-Bromophenyl-phenylether	16.486	248	343249	21.647	ng/ul	100
69) Hexachlorobenzene	16.598	284	389782	20.719	ng/ul	100
70) Atrazine	16.757	200	363037	22.762	ng/ul	100
71) Pentachlorophenol	16.945	266	247406	24.608	ng/ul	100
72) Phenanthrene	17.339	178	1892257	23.560	ng/ul	100
74) Anthracene	17.433	178	1923676	23.923	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.340	216	468359	19.832	ng/ul	100
76) Pentachlorobenzene	14.857	250	501846	22.502	ng/ul	100
77) Carbazole	17.704	167	1773427	25.026	ng/ul	100
78) Di-n-butylphthalate	18.251	149	2131692	26.502	ng/ul	100
80) Fluoranthene	19.304	202	2196924	22.560	ng/ul	100
82) Pyrene	19.657	202	2288921	22.785	ng/ul	100
83) Butylbenzylphthalate	20.533	149	999719	30.694	ng/ul	100
84) 3,3'-Dichlorobenzidine	21.304	252	825872	29.921	ng/ul	100
85) Benzo(a)anthracene	21.369	228	2314931	24.105	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.286	149	1510834	29.077	ng/ul	100
87) Chrysene	21.422	228	2188350	23.597	ng/ul	100
89) Di-n-octyl phthalate	22.227	149	2609622	27.475	ng/ul	100
90) Benzo(b)fluoranthene	23.074	252	2444917	22.636	ng/ul	100
91) Benzo(k)fluoranthene	23.121	252	2432288	23.524	ng/ul	100
93) Benzo(a)pyrene	23.715	252	2203385	21.044	ng/ul	100
94) Indeno(1,2,3-cd)pyrene	26.362	276	2788465	23.075	ng/ul	100
95) Dibenzo(a,h)anthracene	26.380	278	2497548	23.972	ng/ul	100
96) Benzo(g,h,i)perylene	27.145	276	2453591	24.340	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Oct 01 00:03:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 30 23:58:42 2022
Response via : Initial Calibration




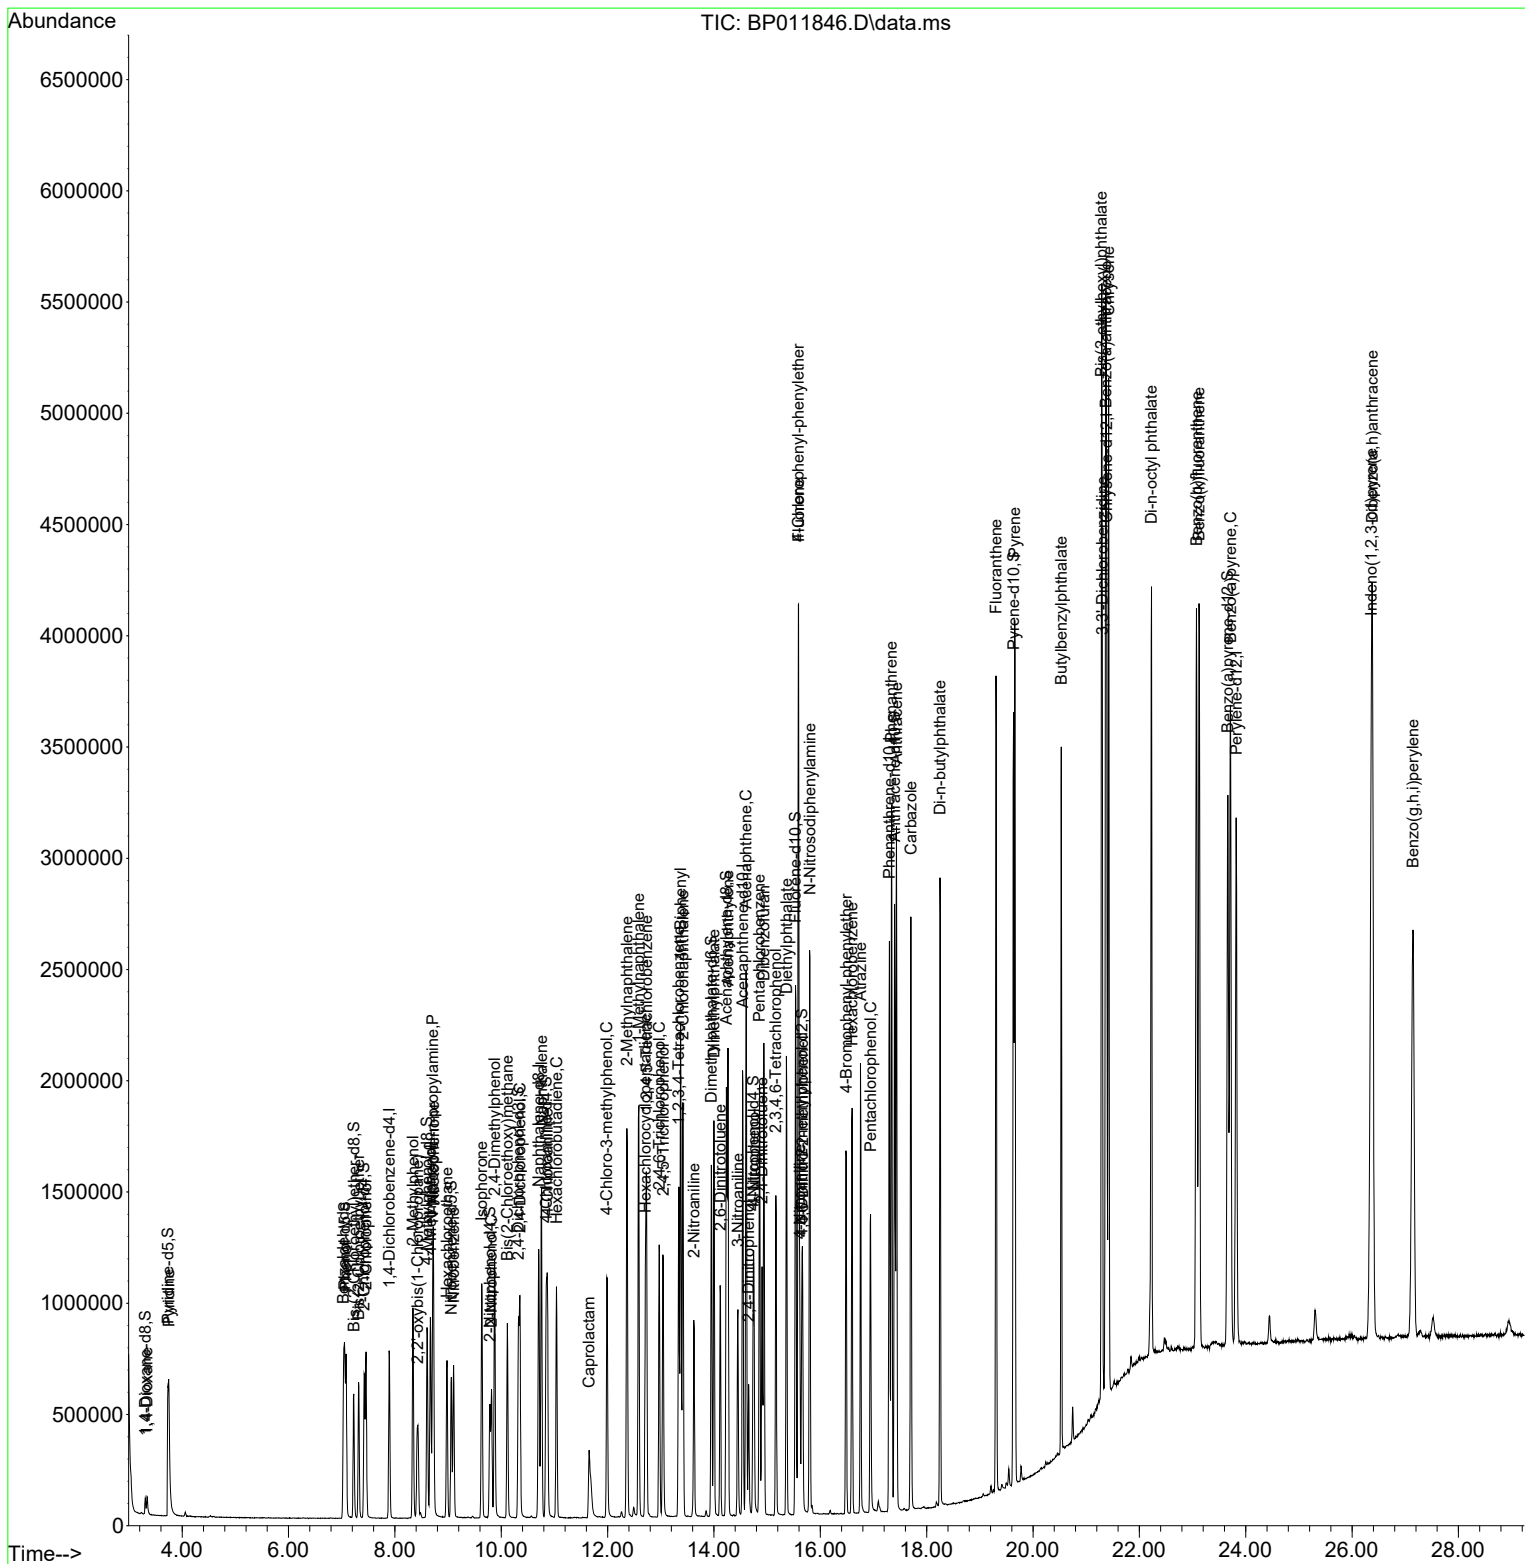


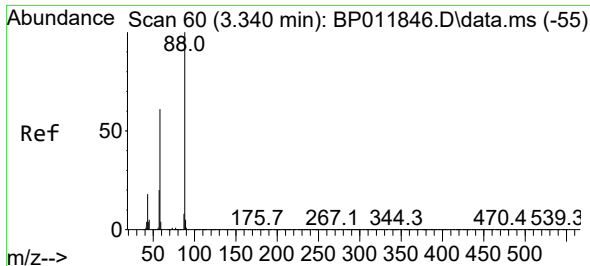

#2
 1,4-Dioxane
 Concen: 8.859 ng/uL
 RT: 3.340 min Scan# 60
 Delta R.T. 0.000 min
 Lab File: BP011846.D
 Acq: 30 Sep 2022 18:12




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020619


Tgt Ion: 88 Resp: 49969
 Ion Ratio Lower Upper
 88 100
 43 19.5 15.6 23.4
 58 60.7 48.6 72.8

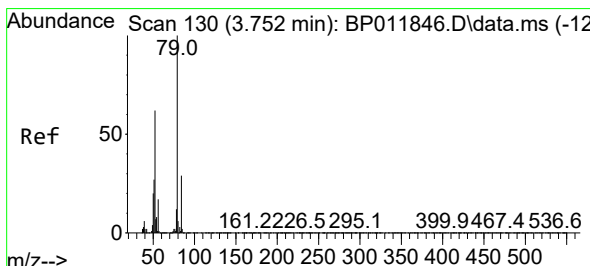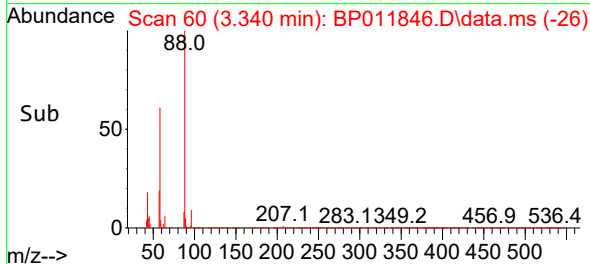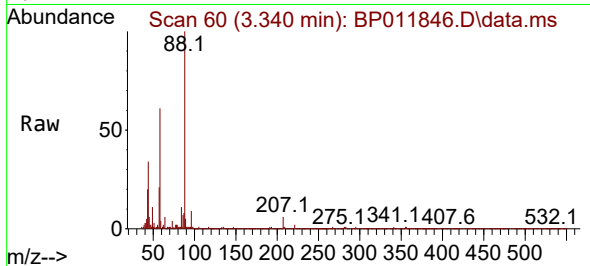

#5
 Pyridine
 Concen: 22.397 ng/uL
 RT: 3.752 min Scan# 130
 Delta R.T. 0.000 min
 Lab File: BP011846.D
 Acq: 30 Sep 2022 18:12

Tgt Ion: 79 Resp: 328839
 Ion Ratio Lower Upper
 79 100
 52 62.1 49.7 74.5
 51 27.0 21.6 32.4


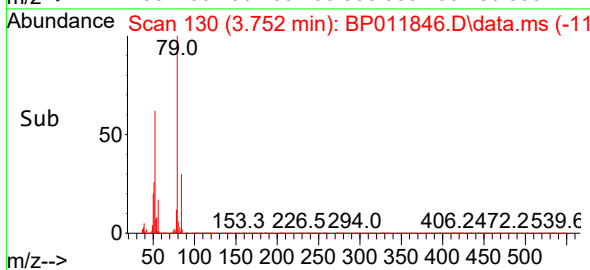

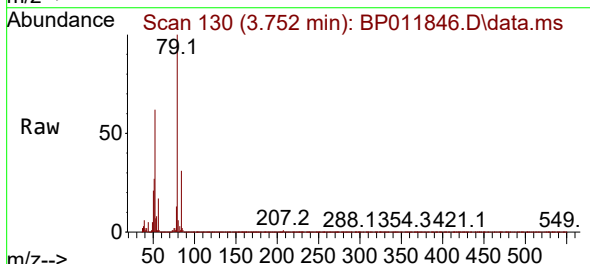


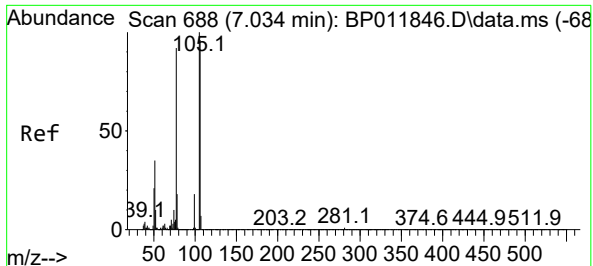

#6
Benzaldehyde
Concen: 25.695 ng/ul
RT: 7.034 min Scan# 688
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion: 77 Resp: 228858
Ion Ratio Lower Upper
77 100
105 108.8 87.0 130.6
106 104.7 83.8 125.6

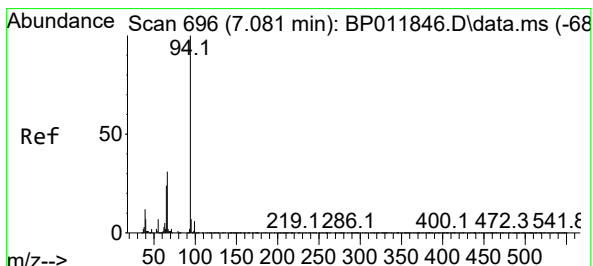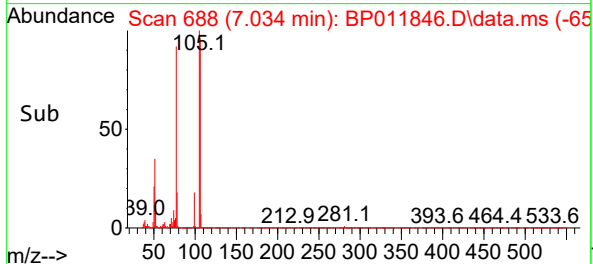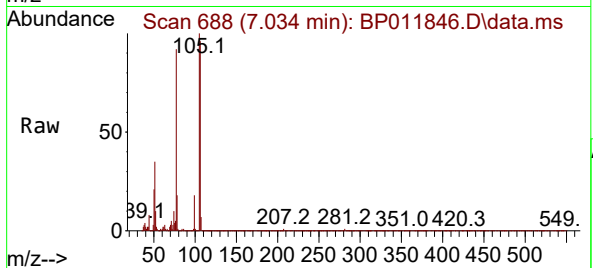

#8
Phenol
Concen: 22.941 ng/ul
RT: 7.081 min Scan# 696
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12

Tgt Ion: 94 Resp: 457373
Ion Ratio Lower Upper
94 100
65 24.4 19.5 29.3
66 31.2 25.0 37.4


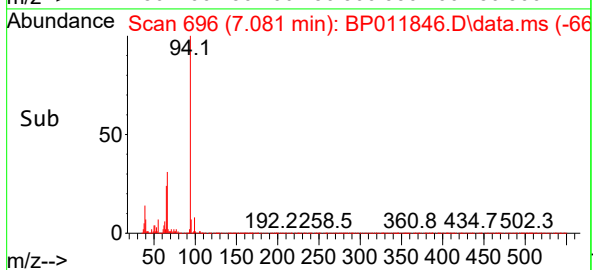

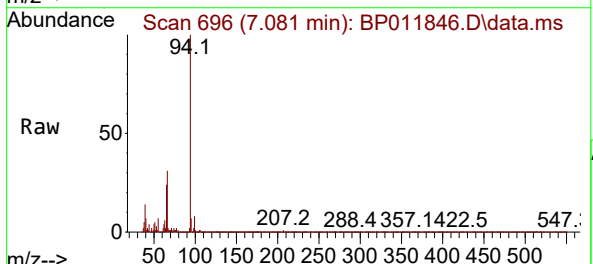




#10
Bis(2-Chloroethyl)ether
Concen: 23.678 ng/ul
RT: 7.316 min Scan# 736
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion: 93 Resp: 372569
Ion Ratio Lower Upper
93 100
63 70.3 56.2 84.4
95 32.4 25.9 38.9



#12
2-Chlorophenol
Concen: 24.117 ng/ul
RT: 7.458 min Scan# 760
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12

Tgt Ion:128 Resp: 380865
Ion Ratio Lower Upper
128 100
64 38.9 31.1 46.7
130 31.9 25.5 38.3



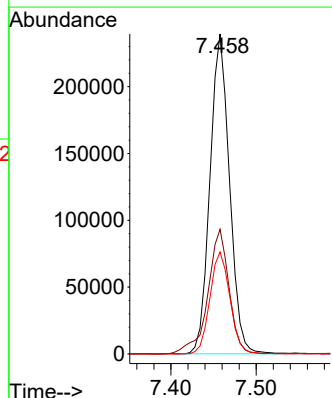





#13
2-Methylphenol
Concen: 23.897 ng/ul
RT: 8.340 min Scan# 910
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:108 Resp: 362702
Ion Ratio Lower Upper
108 100
107 87.7 70.2 105.2



#14
2,2'-oxybis(1-Chloropropane)
Concen: 18.408 ng/ul
RT: 8.428 min Scan# 925
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12

Tgt Ion: 45 Resp: 372581
Ion Ratio Lower Upper
45 100
77 20.0 16.0 24.0
79 15.6 12.5 18.7









#16
Acetophenone
Concen: 24.312 ng/ul
RT: 8.728 min Scan# 91
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:105 Resp: 583435
Ion Ratio Lower Upper
105 100
77 69.2 55.4 83.0
51 19.0 15.2 22.8



#17
N-Nitroso-di-n-propylamine
Concen: 24.673 ng/ul
RT: 8.710 min Scan# 973
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12

Tgt Ion: 70 Resp: 275724
Ion Ratio Lower Upper
70 100
42 40.9 32.7 49.1
101 10.5 8.4 12.6
130 24.3 19.4 29.2



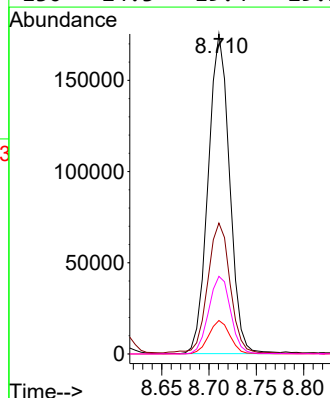





#18
4-Methylphenol
Concen: 24.760 ng/ul
RT: 8.669 min Scan# 966
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:108 Resp: 402432
Ion Ratio Lower Upper
108 100
107 110.0 88.0 132.0



#19
Hexachloroethane
Concen: 22.431 ng/ul
RT: 8.981 min Scan# 1019
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12

Tgt Ion:117 Resp: 140030
Ion Ratio Lower Upper
117 100
201 103.0 82.4 123.6
199 64.5 51.6 77.4



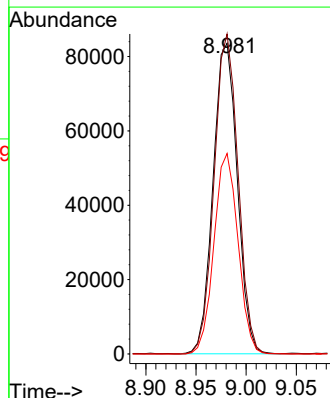





#22
Nitrobenzene
Concen: 23.672 ng/ul
RT: 9.105 min Scan# 1040
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion: 77 Resp: 400458
Ion Ratio Lower Upper
77 100
123 52.0 41.6 62.4
65 12.1 9.7 14.5



#23
Isophorone
Concen: 23.877 ng/ul
RT: 9.634 min Scan# 1130
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12

Tgt Ion: 82 Resp: 818382
Ion Ratio Lower Upper
82 100
95 6.8 5.4 8.2
138 19.8 15.8 23.8



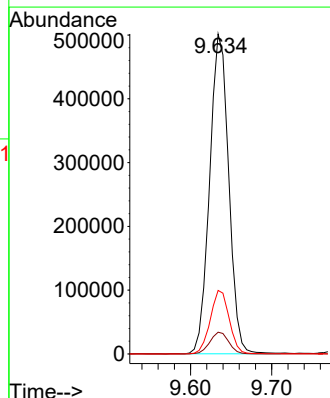





#25
2-Nitrophenol
Concen: 31.483 ng/ul
RT: 9.816 min Scan# 1161
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:139 Resp: 230859
Ion Ratio Lower Upper
139 100
65 40.3 32.2 48.4
109 24.5 19.6 29.4



#26
2,4-Dimethylphenol
Concen: 23.166 ng/ul
RT: 9.875 min Scan# 1171
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12

Tgt Ion:107 Resp: 428212
Ion Ratio Lower Upper
107 100
121 53.8 43.0 64.6
122 93.6 74.9 112.3



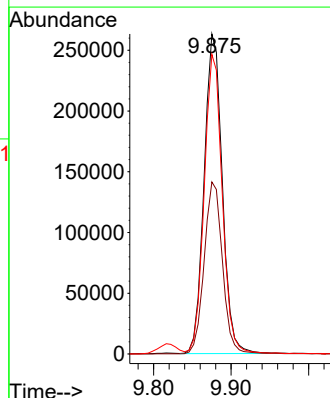





#27
 Bis(2-Chloroethoxy)methane
 Concen: 23.686 ng/ul
 RT: 10.116 min Scan# 1212
 Delta R.T. 0.000 min
 Lab File: BP011846.D
 Acq: 30 Sep 2022 18:12




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020619


Tgt Ion: 93 Resp: 526112
 Ion Ratio Lower Upper
 93 100
 95 32.9 26.3 39.5
 123 11.9 9.5 14.3

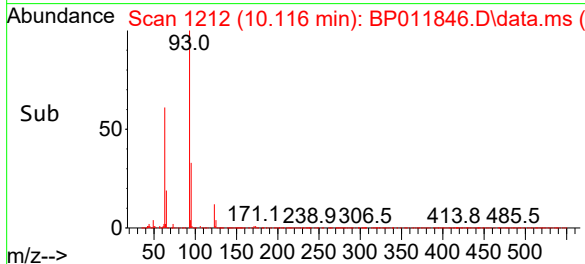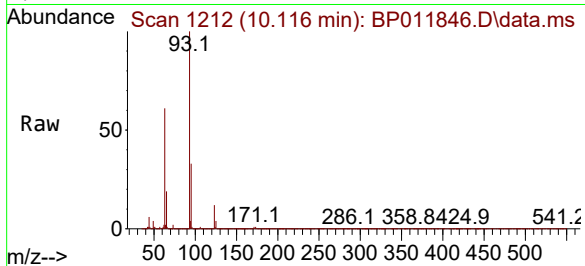

#29
 2,4-Dichlorophenol
 Concen: 24.063 ng/ul
 RT: 10.352 min Scan# 1252
 Delta R.T. 0.000 min
 Lab File: BP011846.D
 Acq: 30 Sep 2022 18:12

Tgt Ion:162 Resp: 382890
 Ion Ratio Lower Upper
 162 100
 164 65.3 52.2 78.4
 98 33.7 27.0 40.4


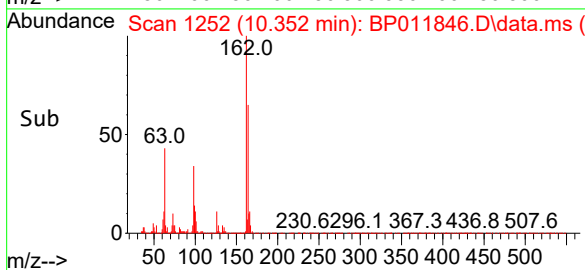

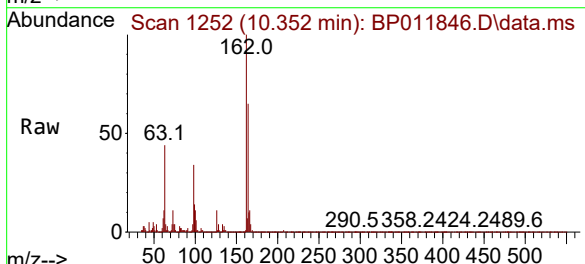




#30
Naphthalene
Concen: 23.131 ng/ul
RT: 10.757 min Scan# 1321
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:128 Resp: 1308500
Ion Ratio Lower Upper
128 100
129 11.1 8.9 13.3
127 13.1 10.5 15.7

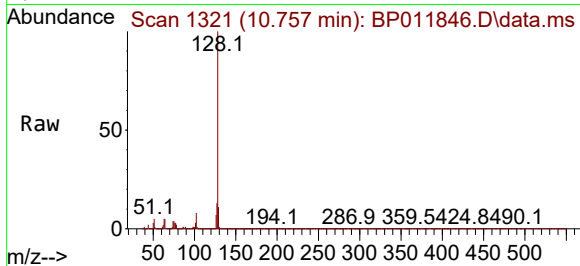

#32
4-Chloroaniline
Concen: 23.710 ng/ul
RT: 10.869 min Scan# 1340
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12

Tgt Ion:127 Resp: 575411
Ion Ratio Lower Upper
127 100
129 33.2 26.6 39.8




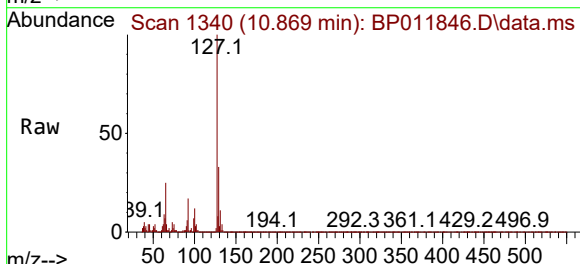




#33
Hexachlorobutadiene
Concen: 20.734 ng/ul
RT: 11.040 min Scan# 1369
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:225 Resp: 219721
Ion Ratio Lower Upper
225 100
223 65.1 52.1 78.1
227 65.4 52.3 78.5



#34
Caprolactam
Concen: 27.846 ng/ul
RT: 11.651 min Scan# 1473
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12

Tgt Ion:113 Resp: 130219
Ion Ratio Lower Upper
113 100
55 132.5 106.0 159.0
56 98.4 78.7 118.1









#35
4-Chloro-3-methylphenol
Concen: 25.638 ng/ul
RT: 11.987 min Scan# 1530
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:107 Resp: 405580
Ion Ratio Lower Upper
107 100
144 28.1 22.5 33.7
142 87.5 70.0 105.0

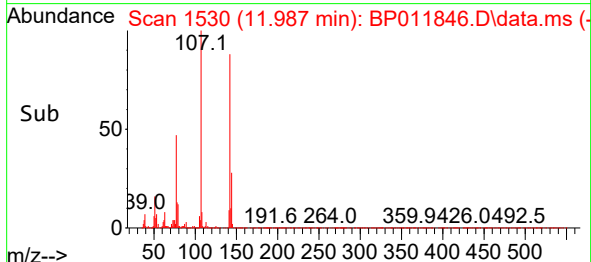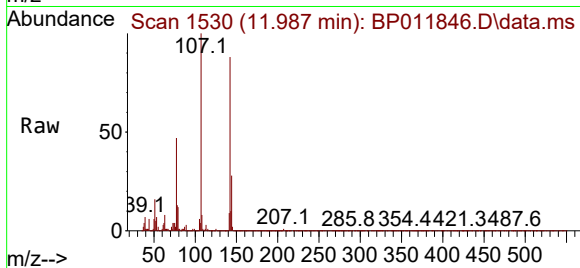

#36
2-Methylnaphthalene
Concen: 24.152 ng/ul
RT: 12.363 min Scan# 1594
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12

Tgt Ion:142 Resp: 915438
Ion Ratio Lower Upper
142 100
141 88.3 70.6 106.0


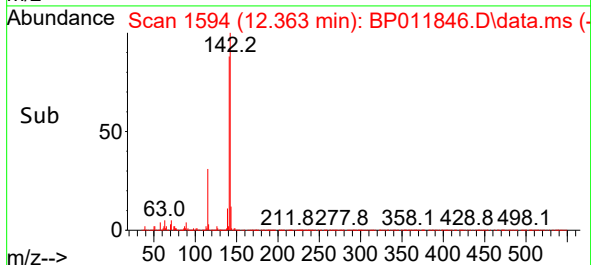

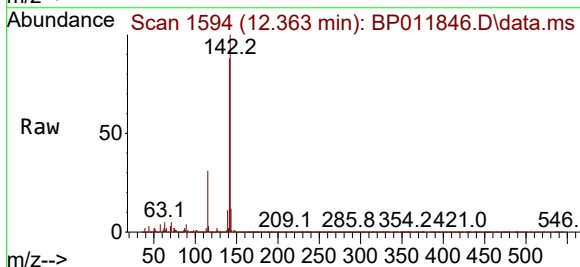


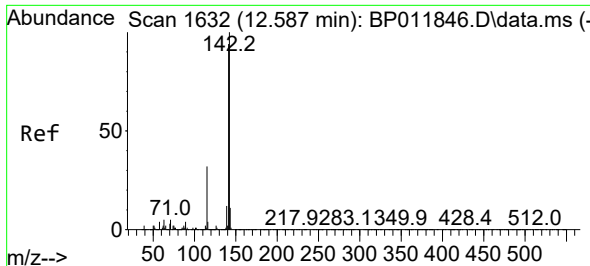

#37
1-Methylnaphthalene
Concen: 24.207 ng/ul
RT: 12.587 min Scan# 1632
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:142 Resp: 919649
Ion Ratio Lower Upper
142 100
141 93.5 74.8 112.2
116 3.6 2.9 4.3

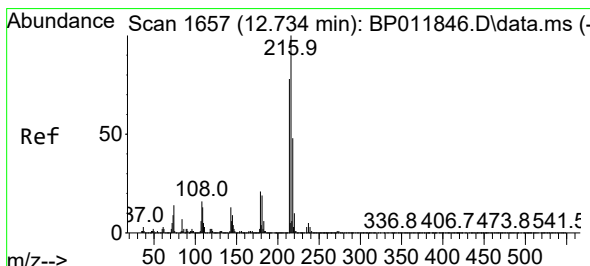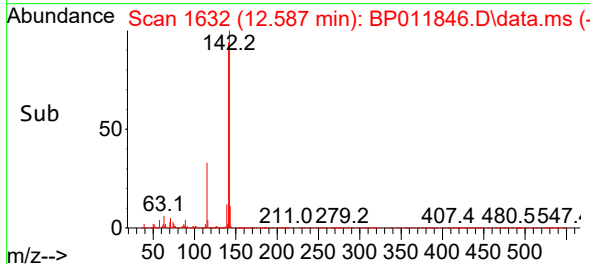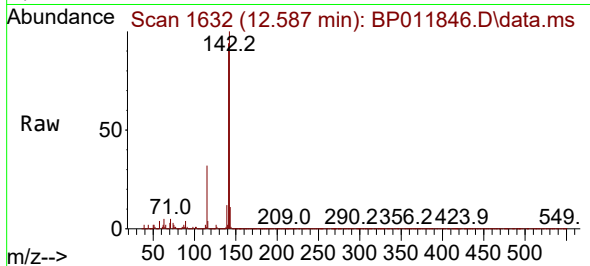

#39
1,2,4,5-Tetrachlorobenzene
Concen: 21.018 ng/ul
RT: 12.734 min Scan# 1657
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12

Tgt Ion:216 Resp: 464398
Ion Ratio Lower Upper
216 100
214 78.3 62.6 94.0
179 20.7 16.6 24.8
108 15.8 12.6 19.0

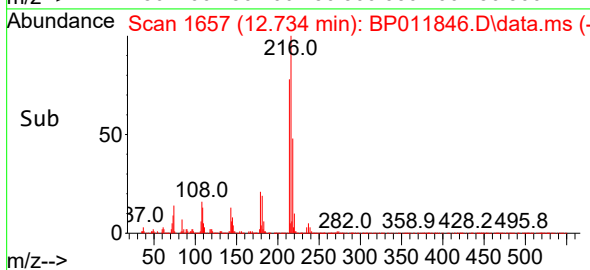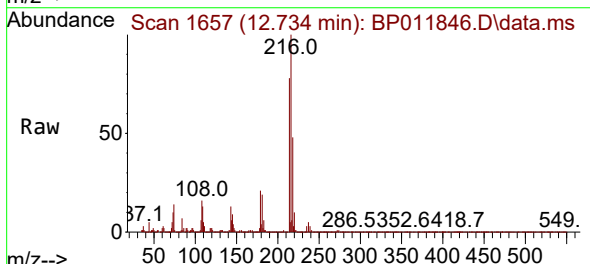



#40

Hexachlorocyclopentadiene

Concen: 19.432 ng/ul

RT: 12.710 min Scan# 1653

Delta R.T. 0.000 min

Lab File: BP011846.D

Acq: 30 Sep 2022 18:12

Instrument :

BNA_P

ClientSampleId :

SSTD020619





Tgt Ion:237 Resp: 255281

Ion Ratio Lower Upper

237 100

235 63.8 51.0 76.6

272 13.1 10.5 15.7



#41

2,4,6-Trichlorophenol

Concen: 24.923 ng/ul

RT: 12.975 min Scan# 1698

Delta R.T. 0.000 min

Lab File: BP011846.D

Acq: 30 Sep 2022 18:12




Tgt Ion:196 Resp: 311423


Ion Ratio Lower Upper

196 100

198 98.4 78.7 118.1

200 30.6 24.5 36.7


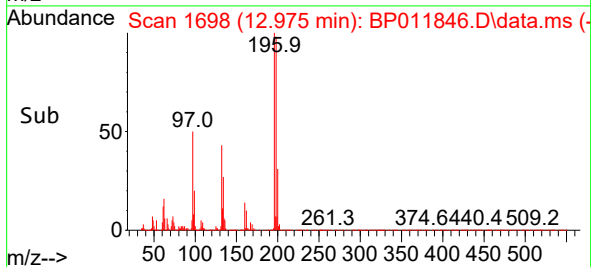

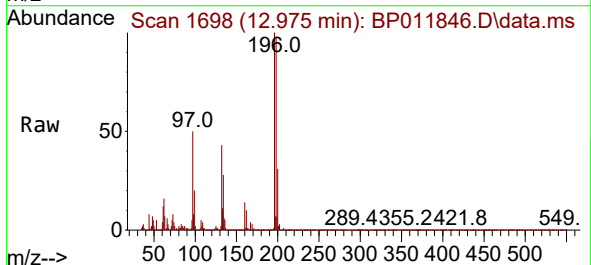


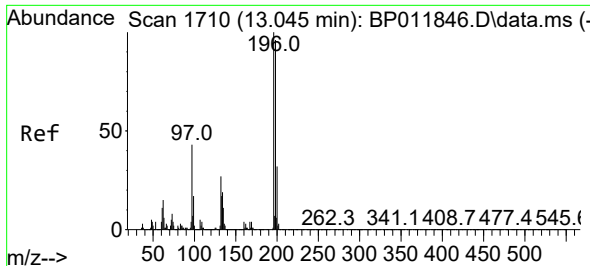

#42
2,4,5-Trichlorophenol
Concen: 24.773 ng/ul
RT: 13.045 min Scan# 1710
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:196 Resp: 339991
Ion Ratio Lower Upper
196 100
198 95.7 76.6 114.8
200 32.0 25.6 38.4

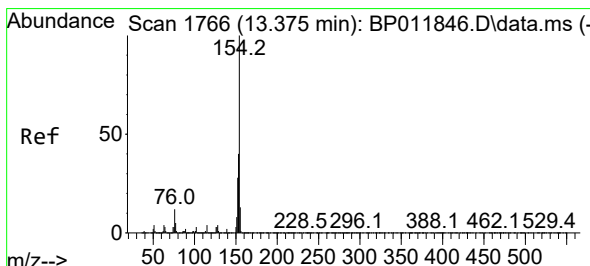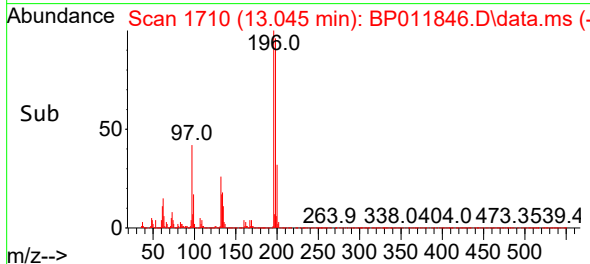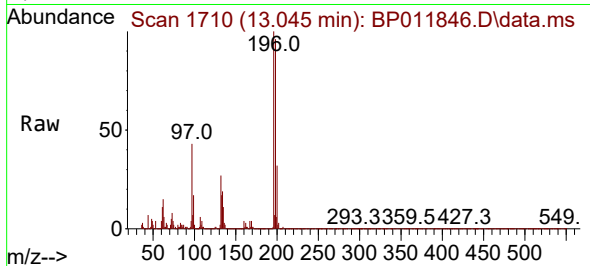

#43
1,1'-Biphenyl
Concen: 21.909 ng/ul
RT: 13.375 min Scan# 1766
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12

Tgt Ion:154 Resp: 1198633
Ion Ratio Lower Upper
154 100
153 39.7 31.8 47.6
76 11.9 9.5 14.3

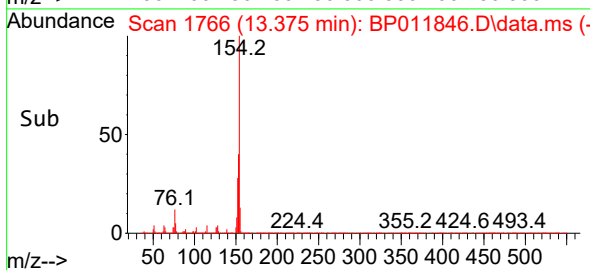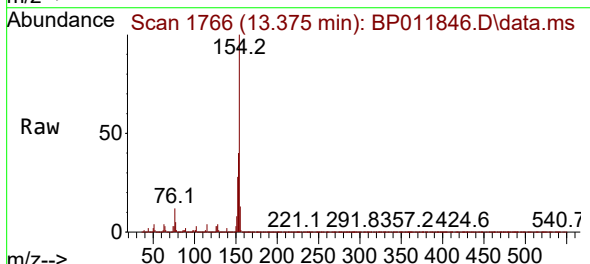




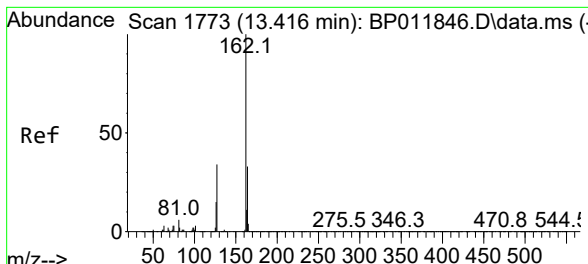


#44
 2-Chloronaphthalene
 Concen: 22.619 ng/ul
 RT: 13.416 min Scan# 1773
 Delta R.T. 0.000 min
 Lab File: BP011846.D
 Acq: 30 Sep 2022 18:12

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020619

Tgt Ion: 162 Resp: 947611




Ion	Ratio	Lower	Upper
162	100		
164	33.1	26.5	39.7
127	37.1	29.7	44.5

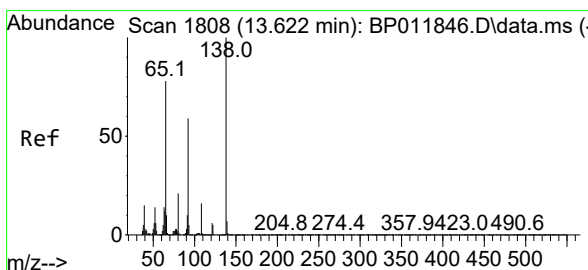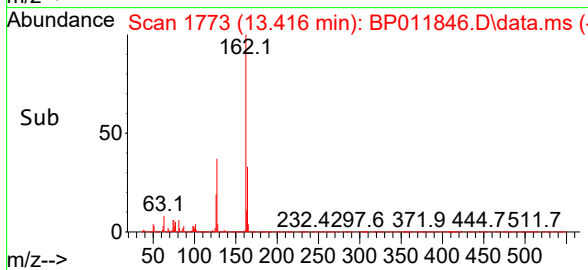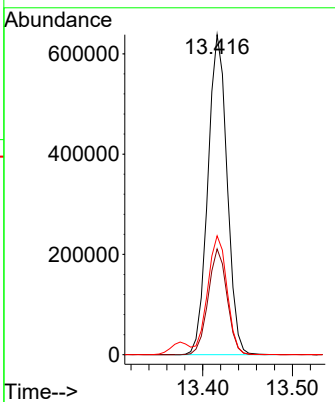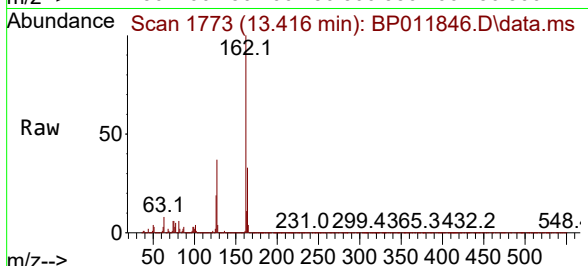


#45
 2-Nitroaniline
 Concen: 27.203 ng/ul
 RT: 13.622 min Scan# 1808
 Delta R.T. 0.000 min
 Lab File: BP011846.D
 Acq: 30 Sep 2022 18:12

Tgt Ion: 65 Resp: 236080

Ion	Ratio	Lower	Upper
65	100		
92	76.5	61.2	91.8
138	128.7	103.0	154.4


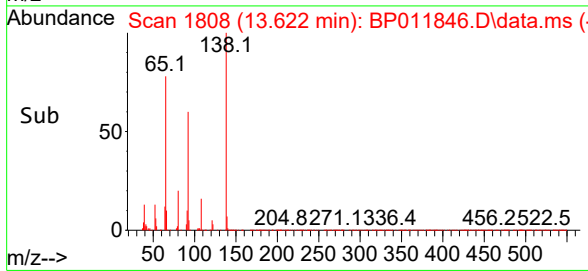
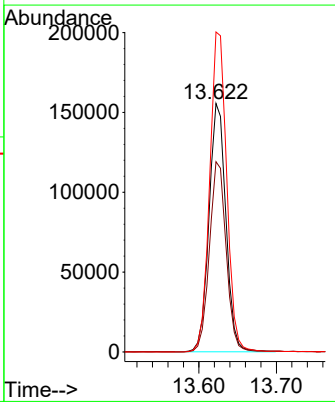
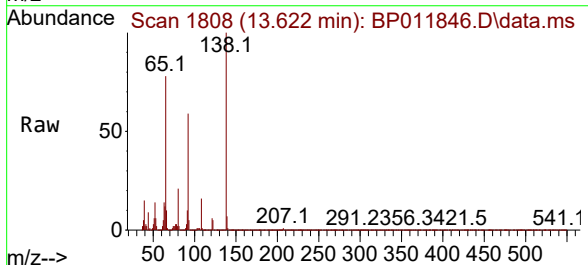




#47
Dimethylphthalate
Concen: 24.078 ng/ul
RT: 13.998 min Scan# 1872
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:163 Resp: 1204055
Ion Ratio Lower Upper
163 100
194 4.1 3.3 4.9
164 10.6 8.5 12.7

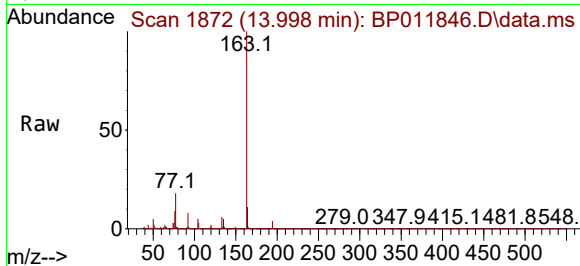

#48
2,6-Dinitrotoluene
Concen: 29.417 ng/ul
RT: 14.122 min Scan# 1893
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12

Tgt Ion:165 Resp: 235738
Ion Ratio Lower Upper
165 100
89 48.9 39.1 58.7
121 20.9 16.7 25.1

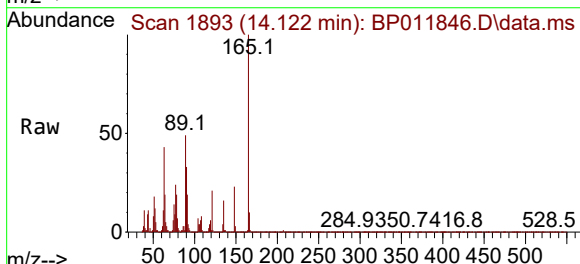



#50

Acenaphthylene

Concen: 22.279 ng/ul

RT: 14.263 min Scan# 1917

Delta R.T. 0.000 min

Lab File: BP011846.D

Acq: 30 Sep 2022 18:12

Instrument :

BNA_P

ClientSampleId :

SSTD020619





Tgt Ion:152 Resp: 1484022

Ion Ratio Lower Upper

152 100

151 20.0 16.0 24.0

153 13.5 10.8 16.2

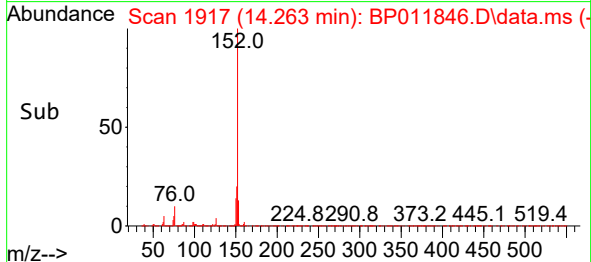

#51

3-Nitroaniline

Concen: 28.504 ng/ul

RT: 14.451 min Scan# 1949

Delta R.T. 0.000 min

Lab File: BP011846.D

Acq: 30 Sep 2022 18:12




Tgt Ion:138 Resp: 273256


Ion Ratio Lower Upper

138 100

108 10.3 8.2 12.4

92 107.0 85.6 128.4

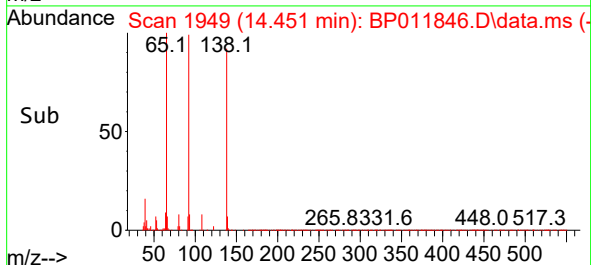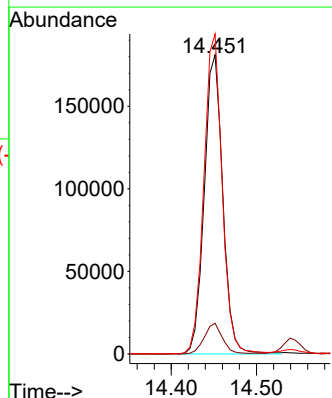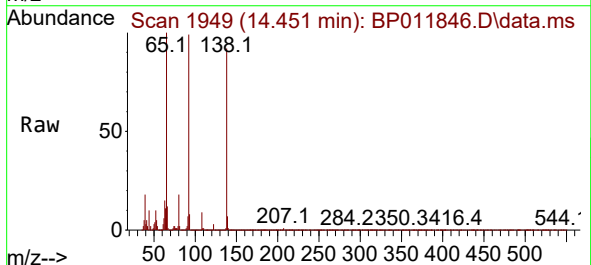



#52

Acenaphthene

Concen: 23.735 ng/ul

RT: 14.604 min Scan# 1975

Delta R.T. 0.000 min

Lab File: BP011846.D

Acq: 30 Sep 2022 18:12

Instrument :

BNA_P

ClientSampleId :

SSTD020619





Tgt Ion:153 Resp: 1033894

Ion Ratio Lower Upper

153 100

152 48.0 38.4 57.6

154 88.2 70.6 105.8



#53

2,4-Dinitrophenol

Concen: 40.016 ng/ul

RT: 14.651 min Scan# 1983

Delta R.T. 0.000 min

Lab File: BP011846.D

Acq: 30 Sep 2022 18:12




Tgt Ion:184 Resp: 140397


Ion Ratio Lower Upper

184 100

63 55.3 44.2 66.4

154 57.2 45.8 68.6



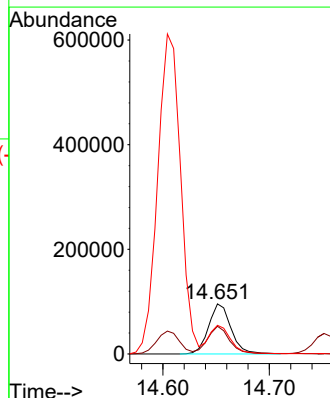
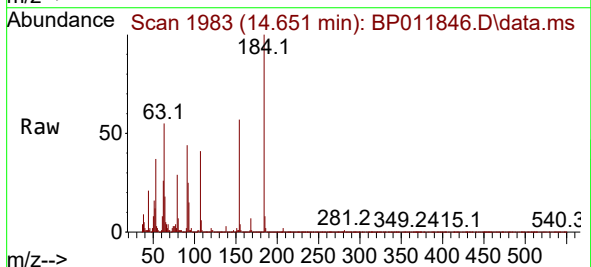




#55
4-Nitrophenol
Concen: 24.292 ng/ul
RT: 14.751 min Scan# 2000
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:109 Resp: 158854
Ion Ratio Lower Upper
109 100
139 156.3 125.0 187.6
65 127.4 101.9 152.9

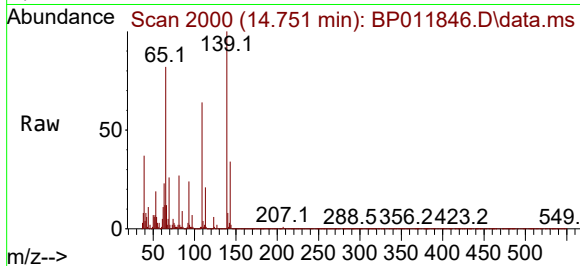

#56
Dibenzofuran
Concen: 22.880 ng/ul
RT: 14.940 min Scan# 2032
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12

Tgt Ion:168 Resp: 1413762
Ion Ratio Lower Upper
168 100
139 36.8 29.4 44.2




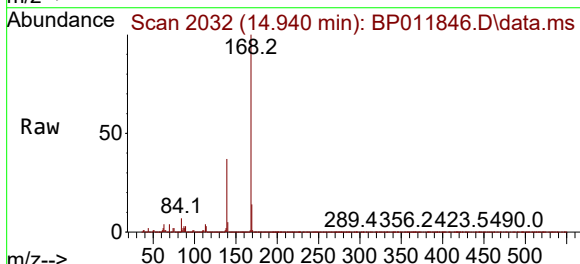




#57
2,4-Dinitrotoluene
Concen: 31.083 ng/ul
RT: 14.904 min Scan# 2026
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:165 Resp: 346857
Ion Ratio Lower Upper
165 100
63 35.2 28.2 42.2
182 2.8 2.2 3.4



#58
2,3,4,6-Tetrachlorophenol
Concen: 28.605 ng/ul
RT: 15.163 min Scan# 2070
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12

Tgt Ion:232 Resp: 295621
Ion Ratio Lower Upper
232 100
131 45.2 36.2 54.2
130 2.1 1.7 2.5
166 31.2 25.0 37.4



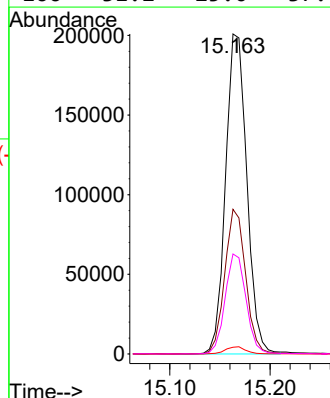





#59
Diethylphthalate
Concen: 24.991 ng/ul
RT: 15.363 min Scan# 2104
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:149 Resp: 1216954
Ion Ratio Lower Upper
149 100
177 22.3 17.8 26.8
150 12.4 9.9 14.9

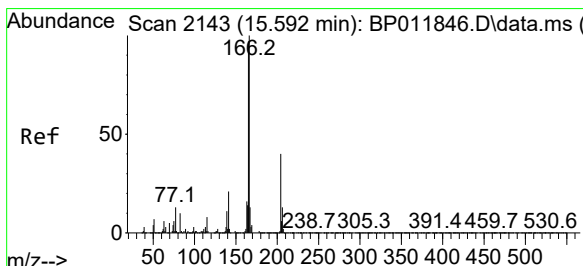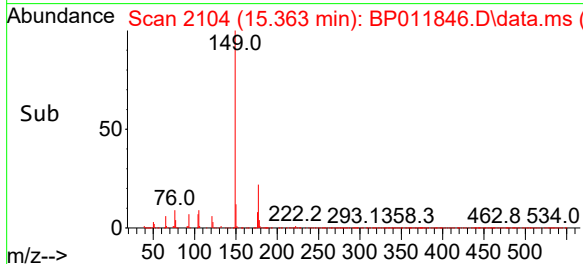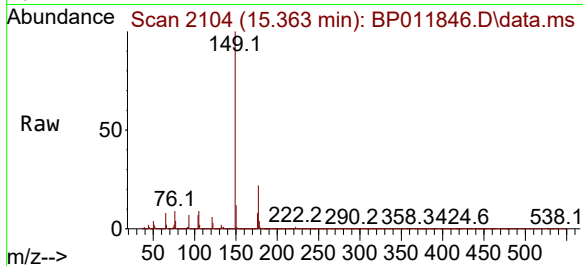

#61
Fluorene
Concen: 23.405 ng/ul
RT: 15.592 min Scan# 2143
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12

Tgt Ion:166 Resp: 1168986
Ion Ratio Lower Upper
166 100
165 96.5 77.2 115.8
167 13.4 10.7 16.1


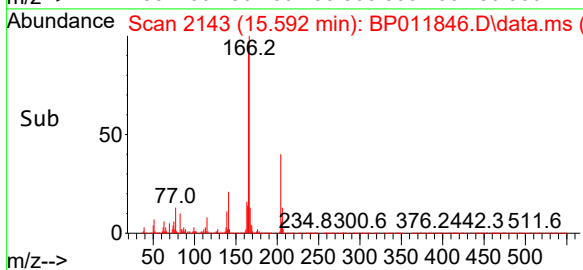

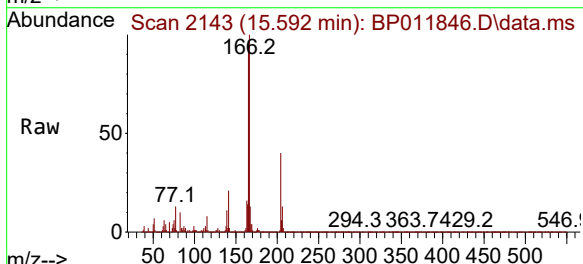




#62
4-Chlorophenyl-phenylether
Concen: 22.536 ng/ul
RT: 15.587 min Scan# 2142
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:204 Resp: 570464
Ion Ratio Lower Upper
204 100
206 33.5 26.8 40.2
141 55.6 44.5 66.7

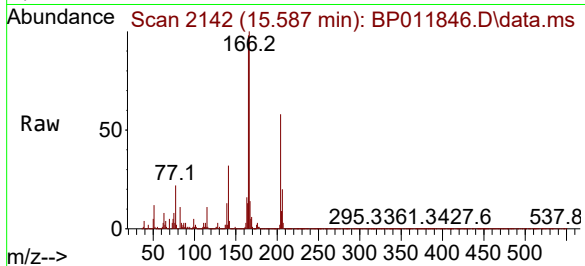

#63
4-Nitroaniline
Concen: 30.488 ng/ul
RT: 15.616 min Scan# 2147
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12

Tgt Ion:138 Resp: 275840
Ion Ratio Lower Upper
138 100
92 44.9 35.9 53.9
108 64.5 51.6 77.4



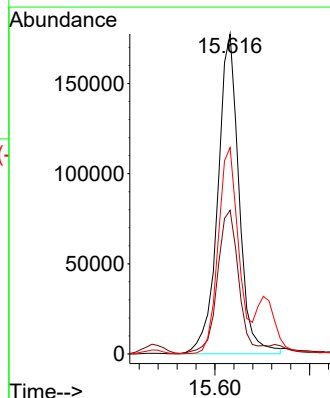
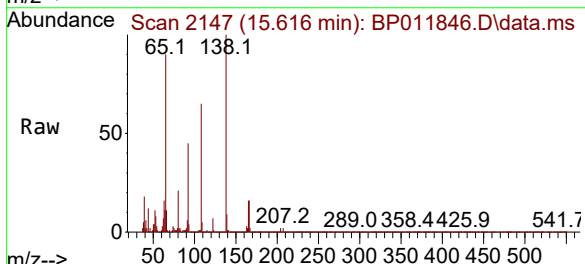




#66
4,6-Dinitro-2-methylphenol
Concen: 34.317 ng/ul
RT: 15.669 min Scan# 2156
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:198 Resp: 211501
Ion Ratio Lower Upper
198 100
182 4.6 3.7 5.5
77 20.7 16.6 24.8

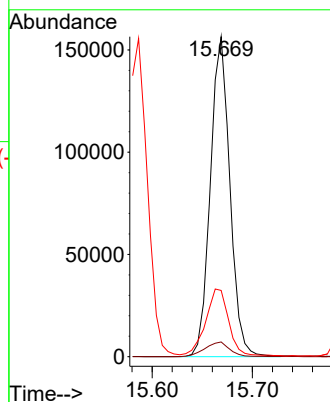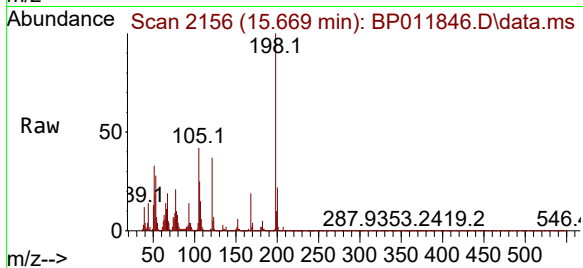

#67
N-Nitrosodiphenylamine
Concen: 23.222 ng/ul
RT: 15.804 min Scan# 2179
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12

Tgt Ion:169 Resp: 1020628
Ion Ratio Lower Upper
169 100
168 67.1 53.7 80.5
167 37.4 29.9 44.9




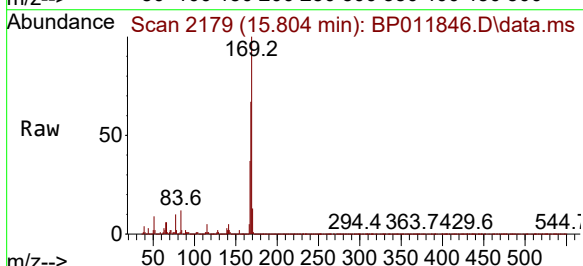




#68
4-Bromophenyl-phenylether
Concen: 21.647 ng/ul
RT: 16.486 min Scan# 2295
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:248 Resp: 343249
Ion Ratio Lower Upper
248 100
250 98.3 78.6 118.0
141 70.0 56.0 84.0



#69
Hexachlorobenzene
Concen: 20.719 ng/ul
RT: 16.598 min Scan# 2314
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12

Tgt Ion:284 Resp: 389782
Ion Ratio Lower Upper
284 100
142 34.1 27.3 40.9
249 31.5 25.2 37.8









#70
Atrazine
Concen: 22.762 ng/ul
RT: 16.757 min Scan# 21
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:200 Resp: 363037
Ion Ratio Lower Upper
200 100
173 27.0 21.6 32.4
215 48.6 38.9 58.3



#71
Pentachlorophenol
Concen: 24.608 ng/ul
RT: 16.945 min Scan# 2373
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12

Tgt Ion:266 Resp: 247406
Ion Ratio Lower Upper
266 100
264 62.3 49.8 74.8
268 64.9 51.9 77.9





#72

Phenanthrene

Concen: 23.560 ng/ul

RT: 17.339 min Scan# 2440

Delta R.T. 0.000 min

Lab File: BP011846.D

Acq: 30 Sep 2022 18:12

Instrument :

BNA_P

ClientSampleId :

SSTD020619





Tgt Ion:178 Resp: 1892257

Ion Ratio Lower Upper

178 100

179 15.6 12.5 18.7

176 19.3 15.4 23.2

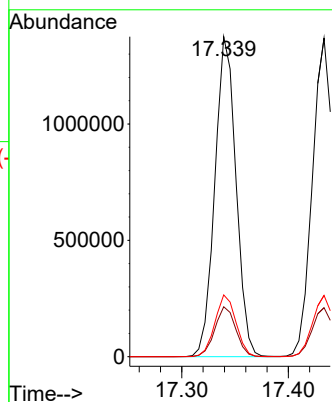

#74

Anthracene

Concen: 23.923 ng/ul

RT: 17.433 min Scan# 2456

Delta R.T. 0.000 min

Lab File: BP011846.D

Acq: 30 Sep 2022 18:12




Tgt Ion:178 Resp: 1923676


Ion Ratio Lower Upper

178 100

179 15.4 12.3 18.5

176 19.3 15.4 23.2









#75
1,2,3,4-Tetrachlorobenzene
Concen: 19.832 ng/uL
RT: 13.340 min Scan# 1760
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:216 Resp: 468359
Ion Ratio Lower Upper
216 100
214 78.2 62.6 93.8
218 46.7 37.4 56.0

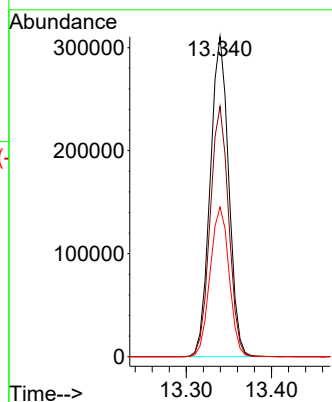

#76
Pentachlorobenzene
Concen: 22.502 ng/uL
RT: 14.857 min Scan# 2018
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12

Tgt Ion:250 Resp: 501846
Ion Ratio Lower Upper
250 100
248 64.2 51.4 77.0
252 64.4 51.5 77.3





#77

Carbazole

Concen: 25.026 ng/ul

RT: 17.704 min Scan# 2502

Delta R.T. 0.000 min

Lab File: BP011846.D

Acq: 30 Sep 2022 18:12

Instrument :

BNA_P

ClientSampleId :

SSTD020619





Tgt Ion:167 Resp: 1773427

Ion Ratio Lower Upper

167 100

166 21.4 17.1 25.7

139 12.6 10.1 15.1

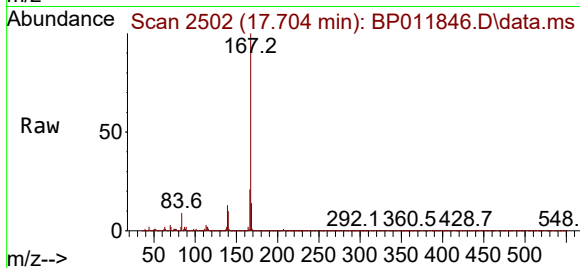

#78

Di-n-butylphthalate

Concen: 26.502 ng/ul

RT: 18.251 min Scan# 2595

Delta R.T. 0.000 min

Lab File: BP011846.D

Acq: 30 Sep 2022 18:12




Tgt Ion:149 Resp: 2131692


Ion Ratio Lower Upper

149 100

150 9.4 7.5 11.3

104 4.5 3.6 5.4

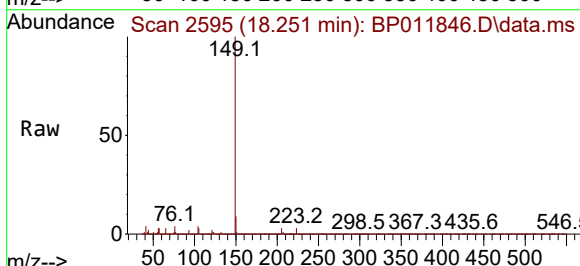

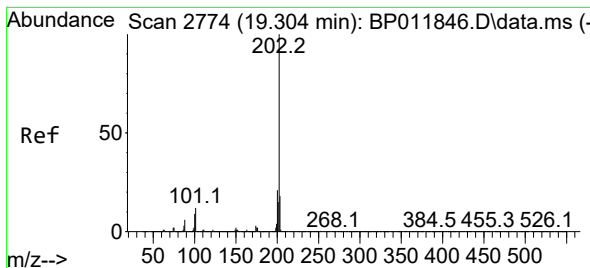

#80

Fluoranthene

Concen: 22.560 ng/ul

RT: 19.304 min Scan# 21

Delta R.T. 0.000 min

Lab File: BP011846.D

Acq: 30 Sep 2022 18:12

Instrument :

BNA_P

ClientSampleId :

SSTD020619





Tgt Ion:202 Resp: 2196924

Ion Ratio Lower Upper

202 100

101 12.2 9.8 14.6

100 9.2 7.4 11.0

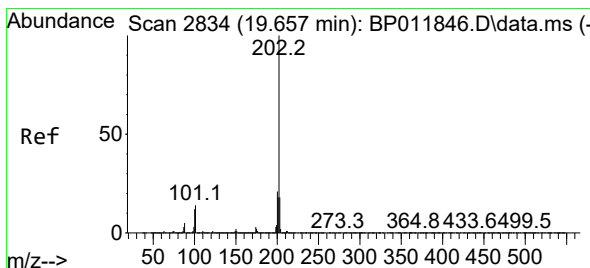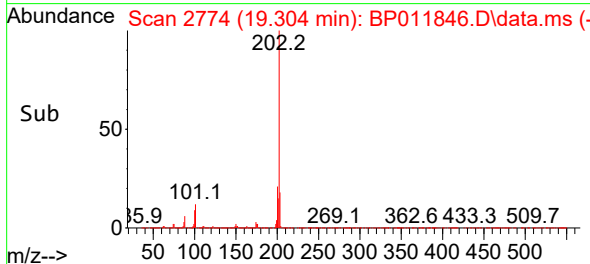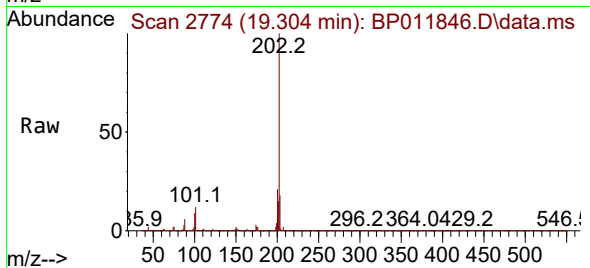

#82

Pyrene

Concen: 22.785 ng/ul

RT: 19.657 min Scan# 2834

Delta R.T. 0.000 min

Lab File: BP011846.D

Acq: 30 Sep 2022 18:12




Tgt Ion:202 Resp: 2288921


Ion Ratio Lower Upper

202 100

101 14.5 11.6 17.4

100 11.7 9.4 14.0

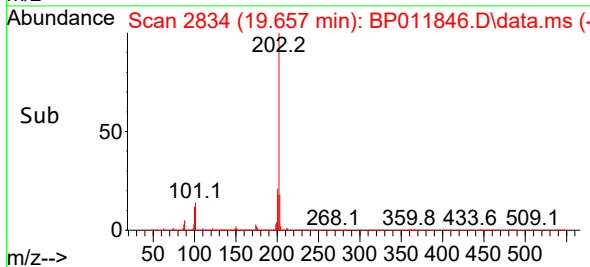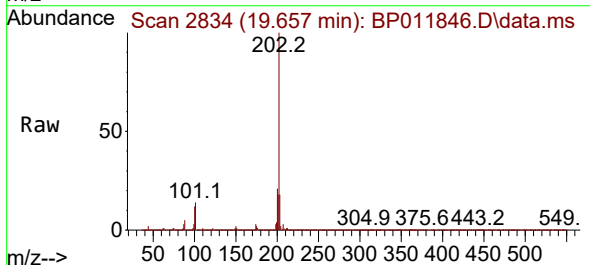



#83

Butylbenzylphthalate

Concen: 30.694 ng/ul

RT: 20.533 min Scan# 2983

Delta R.T. 0.000 min

Lab File: BP011846.D

Acq: 30 Sep 2022 18:12

Instrument :

BNA_P

ClientSampleId :

SSTD020619





Tgt Ion:149 Resp: 999719

Ion Ratio Lower Upper

149 100

91 62.8 50.2 75.4

206 21.1 16.9 25.3



#84

3,3'-Dichlorobenzidine

Concen: 29.921 ng/ul

RT: 21.304 min Scan# 3114

Delta R.T. 0.000 min

Lab File: BP011846.D

Acq: 30 Sep 2022 18:12




Tgt Ion:252 Resp: 825872


Ion Ratio Lower Upper

252 100

254 64.2 51.4 77.0

126 11.1 8.9 13.3





#85

Benzo(a)anthracene

Concen: 24.105 ng/ul

RT: 21.369 min Scan# 3125

Delta R.T. 0.000 min

Lab File: BP011846.D

Acq: 30 Sep 2022 18:12

Instrument :

BNA_P

ClientSampleId :

SSTD020619





Tgt Ion:228 Resp: 2314931

Ion Ratio Lower Upper

228 100

229 19.7 15.8 23.6

226 27.5 22.0 33.0

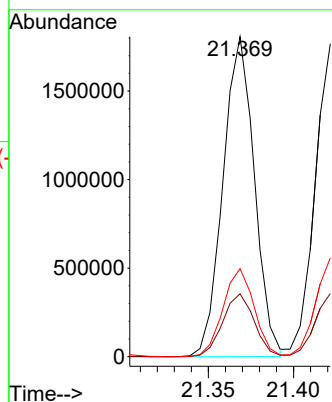

#86

Bis(2-ethylhexyl)phthalate

Concen: 29.077 ng/ul

RT: 21.286 min Scan# 3111

Delta R.T. 0.000 min

Lab File: BP011846.D

Acq: 30 Sep 2022 18:12




Tgt Ion:149 Resp: 1510834


Ion Ratio Lower Upper

149 100

167 26.5 21.2 31.8

279 3.6 2.9 4.3

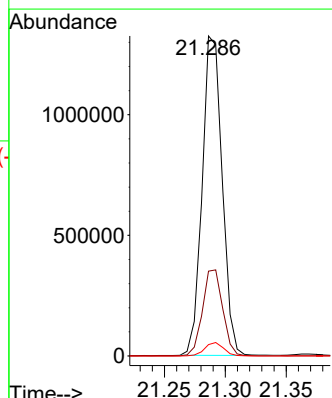



#87

Chrysene

Concen: 23.597 ng/ul

RT: 21.422 min Scan# 3134

Delta R.T. 0.000 min

Lab File: BP011846.D

Acq: 30 Sep 2022 18:12

Instrument :

BNA_P

ClientSampleId :

SSTD020619





Tgt Ion:228 Resp: 2188350

Ion Ratio Lower Upper

228 100

226 31.6 25.3 37.9

229 20.2 16.2 24.2



#89

Di-n-octyl phthalate

Concen: 27.475 ng/ul




RT: 22.227 min Scan# 3271


Delta R.T. 0.000 min

Lab File: BP011846.D

Acq: 30 Sep 2022 18:12

Tgt Ion:149 Resp: 2609622


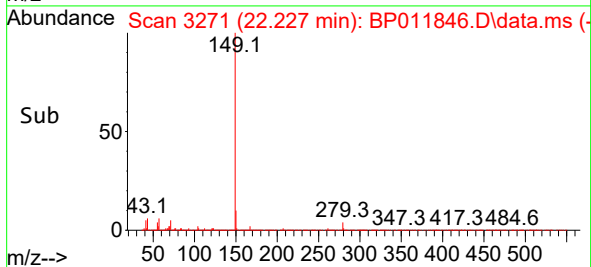

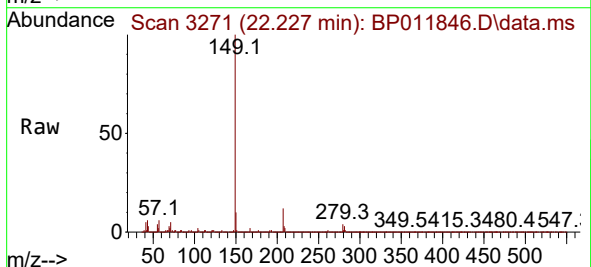




#90
Benzo(b)fluoranthene
Concen: 22.636 ng/ul
RT: 23.074 min Scan# 3415
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12




Instrument :
BNA_P
ClientSampleId :
SSTD020619


Tgt Ion:252 Resp: 2444917
Ion Ratio Lower Upper
252 100
253 22.3 17.8 26.8
125 11.5 9.2 13.8

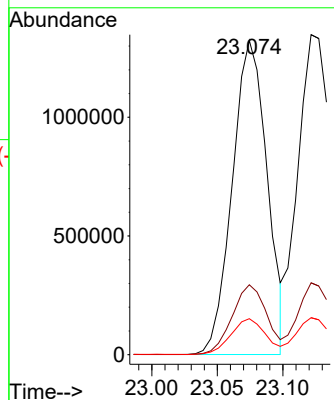

#91
Benzo(k)fluoranthene
Concen: 23.524 ng/ul
RT: 23.121 min Scan# 3423
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12

Tgt Ion:252 Resp: 2432288
Ion Ratio Lower Upper
252 100
253 22.5 18.0 27.0
125 11.5 9.2 13.8

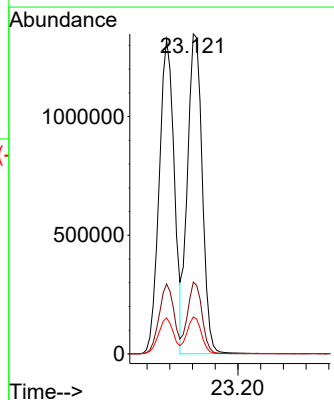



#93

Benzo(a)pyrene

Concen: 21.044 ng/ul

RT: 23.715 min Scan# 3524

Delta R.T. 0.000 min

Lab File: BP011846.D

Acq: 30 Sep 2022 18:12

Instrument :

BNA_P

ClientSampleId :

SSTD020619





Tgt Ion:252 Resp: 2203385

Ion Ratio Lower Upper

252 100

253 22.1 17.7 26.5

125 12.3 9.8 14.8



#94

Indeno(1,2,3-cd)pyrene

Concen: 23.075 ng/ul

RT: 26.362 min Scan# 3974

Delta R.T. 0.000 min

Lab File: BP011846.D

Acq: 30 Sep 2022 18:12




Tgt Ion:276 Resp: 2788465


Ion Ratio Lower Upper

276 100

138 26.7 21.4 32.0

277 24.9 19.9 29.9



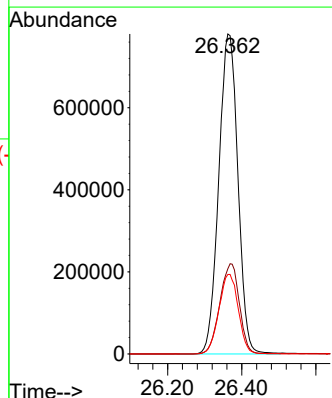





#95
Dibenzo(a,h)anthracene
Concen: 23.972 ng/ul
RT: 26.380 min Scan# 3977
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12

Instrument :
BNA_P
ClientSampleId :
SSTD020619

Tgt Ion:278 Resp: 2497548
Ion Ratio Lower Upper
278 100
139 18.8 15.0 22.6
279 23.8 19.0 28.6



#96
Benzo(g,h,i)perylene
Concen: 24.340 ng/ul
RT: 27.145 min Scan# 4107
Delta R.T. 0.000 min
Lab File: BP011846.D
Acq: 30 Sep 2022 18:12

Tgt Ion:276 Resp: 2453591
Ion Ratio Lower Upper
276 100
138 24.7 19.8 29.6
277 23.2 18.6 27.8

