

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093022\
 Data File : BP011848.D
 Acq On : 30 Sep 2022 19:21
 Operator : CG/JU
 Sample : SST08060
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST080621

Quant Time: Oct 01 00:04:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 30 23:58:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	234292	20.000	ng/u1	0.00
20) Naphthalene-d8	10.704	136	1101661	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.545	164	711426	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.304	188	1519235	20.000	ng/u1	0.00
79) Chrysene-d12	21.386	240	1531685	20.000	ng/u1	0.00
88) Perylene-d12	23.827	264	1751528	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	161792	30.476	ng/uL	0.00
4) Pyridine-d5	3.728	84	1235872	83.730	ng/u1	0.00
7) Phenol-d5	7.063	99	1634576	84.298	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	877808	75.784	ng/u1	0.00
11) 2-Chlorophenol-d4	7.428	132	1317527	88.979	ng/u1	0.00
15) 4-Methylphenol-d8	8.616	113	1349928	90.800	ng/u1	0.01
21) Nitrobenzene-d5	9.069	128	698342	97.265	ng/u1	0.00
24) 2-Nitrophenol-d4	9.787	143	781072	128.250	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	1366385	87.641	ng/u1	0.00
31) 4-Chloroaniline-d4	10.851	131	1971267	82.817	ng/u1	0.00
46) Dimethylphthalate-d6	13.957	166	3925283	81.971	ng/u1	0.00
49) Acenaphthylene-d8	14.239	160	4528432	79.178	ng/u1	0.00
54) 4-Nitrophenol-d4	14.757	143	852815	101.173	ng/u1	0.02
60) Fluorene-d10	15.539	176	3358090	79.000	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.663	200	774979	137.823	ng/u1	0.01
73) Anthracene-d10	17.404	188	5240618	77.875	ng/u1	0.00
81) Pyrene-d10	19.633	212	6028683	77.028	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.674	264	6908360	81.191	ng/u1	0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.340	88	170360	30.418	ng/uL	96
5) Pyridine	3.746	79	1209859	82.987	ng/u1	98
6) Benzaldehyde	7.034	77	591874	66.924	ng/u1	99
8) Phenol	7.087	94	1694015	85.569	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.322	93	1313225	84.051	ng/u1	98
12) 2-Chlorophenol	7.457	128	1397631	89.128	ng/u1	99
13) 2-Methylphenol	8.340	108	1335365	88.604	ng/u1	100
14) 2,2'-oxybis(1-Chloropr...	8.434	45	1290444	64.207	ng/u1	99
16) Acetophenone	8.728	105	1990565	83.535	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.728	70	926348	83.481	ng/u1	97
18) 4-Methylphenol	8.681	108	1457642	90.317	ng/u1	98
19) Hexachloroethane	8.981	117	510836	82.409	ng/u1	97
22) Nitrobenzene	9.110	77	1434482	84.619	ng/u1	97
23) Isophorone	9.646	82	2890009	84.143	ng/u1	99
25) 2-Nitrophenol	9.822	139	857445	116.690	ng/u1	98
26) 2,4-Dimethylphenol	9.881	107	1520154	82.068	ng/u1	97
27) Bis(2-Chloroethoxy)met...	10.122	93	1800423	80.888	ng/u1	100
29) 2,4-Dichlorophenol	10.357	162	1389304	87.130	ng/u1	99
30) Naphthalene	10.757	128	4475824	78.957	ng/u1	100
32) 4-Chloroaniline	10.875	127	2021809	83.138	ng/u1	99
33) Hexachlorobutadiene	11.040	225	797654	75.116	ng/u1	97
34) Caprolactam	11.687	113	267500	57.083	ng/u1	99
35) 4-Chloro-3-methylphenol	11.998	107	1456890	91.905	ng/u1	100
36) 2-Methylnaphthalene	12.369	142	3132813	82.483	ng/u1	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093022\
 Data File : BP011848.D
 Acq On : 30 Sep 2022 19:21
 Operator : CG/JU
 Sample : SST08060
 Misc :
 ALS Vial : 6 Sample Multiplier: 1


Instrument :
 BNA_P
 ClientSampleId :
 SST080621


Quant Time: Oct 01 00:04:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 30 23:58:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.587	142	3133439	82.309	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.734	216	1630384	75.284	ng/ul	98
40) Hexachlorocyclopentadiene	12.716	237	962155	74.723	ng/ul	99
41) 2,4,6-Trichlorophenol	12.975	196	1151694	94.036	ng/ul	97
42) 2,4,5-Trichlorophenol	13.045	196	1254328	93.246	ng/ul	99
43) 1,1'-Biphenyl	13.375	154	3965651	73.953	ng/ul	99
44) 2-Chloronaphthalene	13.422	162	3195885	77.828	ng/ul	99
45) 2-Nitroaniline	13.628	65	861423	101.270	ng/ul	94
47) Dimethylphthalate	14.010	163	4053980	82.711	ng/ul	99
48) 2,6-Dinitrotoluene	14.128	165	907680	115.562	ng/ul	98
50) Acenaphthylene	14.269	152	4891547	74.921	ng/ul	99
51) 3-Nitroaniline	14.457	138	953620	101.489	ng/ul	96
52) Acenaphthene	14.610	153	3414294	79.968	ng/ul	100
53) 2,4-Dinitrophenol	14.657	184	622965	181.154	ng/ul	95
55) 4-Nitrophenol	14.769	109	570323	88.981	ng/ul	97
56) Dibenzofuran	14.945	168	4634173	76.518	ng/ul	99
57) 2,4-Dinitrotoluene	14.916	165	1290914	118.026	ng/ul	94
58) 2,3,4,6-Tetrachlorophenol	15.169	232	1078076	106.429	ng/ul	98
59) Diethylphthalate	15.375	149	4113533	86.184	ng/ul	99
61) Fluorene	15.598	166	3637147	74.298	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.586	204	1857350	74.860	ng/ul	100
63) 4-Nitroaniline	15.628	138	851011	95.965	ng/ul	98
66) 4,6-Dinitro-2-methylph...	15.681	198	811101	133.175	ng/ul#	96
67) N-Nitrosodiphenylamine	15.804	169	3349340	77.115	ng/ul	100
68) 4-Bromophenyl-phenylether	16.486	248	1231829	78.610	ng/ul	99
69) Hexachlorobenzene	16.604	284	1392818	74.917	ng/ul	98
70) Atrazine	16.769	200	1282670	81.380	ng/ul	99
71) Pentachlorophenol	16.945	266	955610	96.184	ng/ul	98
72) Phenanthrene	17.345	178	6193518	78.034	ng/ul	98
74) Anthracene	17.439	178	6146007	77.342	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	13.339	216	1655819	70.948	ng/ul	98
76) Pentachlorobenzene	14.863	250	1737406	78.831	ng/ul	100
77) Carbazole	17.710	167	5858969	83.667	ng/ul	98
78) Di-n-butylphthalate	18.257	149	7115749	89.521	ng/ul	99
80) Fluoranthene	19.310	202	7204309	76.635	ng/ul	97
82) Pyrene	19.663	202	7299257	75.268	ng/ul	96
83) Butylbenzylphthalate	20.533	149	3498847	111.277	ng/ul	96
84) 3,3'-Dichlorobenzidine	21.304	252	2776167	104.189	ng/ul	99
85) Benzo(a)anthracene	21.374	228	7474428	80.623	ng/ul	97
86) Bis(2-ethylhexyl)phtha...	21.292	149	4778000	95.257	ng/ul#	94
87) Chrysene	21.427	228	6913572	77.225	ng/ul	98
89) Di-n-octyl phthalate	22.227	149	8889977	92.377	ng/ul	100
90) Benzo(b)fluoranthene	23.086	252	8640935	78.958	ng/ul	98
91) Benzo(k)fluoranthene	23.133	252	7937187	75.765	ng/ul	98
93) Benzo(a)pyrene	23.727	252	7639491	72.013	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.386	276	9954995	81.308	ng/ul	99
95) Dibenzo(a,h)anthracene	26.409	278	8557517	81.067	ng/ul	97
96) Benzo(g,h,i)perylene	27.180	276	8970479	87.829	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Oct 01 00:04:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Sep 30 23:58:42 2022
Response via : Initial Calibration









#2
 1,4-Dioxane
 Concen: 30.418 ng/uL
 RT: 3.340 min Scan# 60
 Delta R.T. -0.000 min
 Lab File: BP011848.D
 Acq: 30 Sep 2022 19:21




Instrument :
 BNA_P
 ClientSampleId :
 SSTD080621


Tgt Ion: 88 Resp: 170360
 Ion Ratio Lower Upper
 88 100
 43 19.5 15.6 23.4
 58 64.9 48.6 72.8

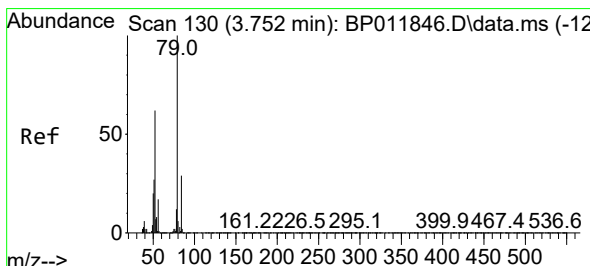

#5
 Pyridine
 Concen: 82.987 ng/uL
 RT: 3.746 min Scan# 129
 Delta R.T. -0.006 min
 Lab File: BP011848.D
 Acq: 30 Sep 2022 19:21

Tgt Ion: 79 Resp: 1209859
 Ion Ratio Lower Upper
 79 100
 52 60.5 49.7 74.5
 51 26.1 21.6 32.4









#6
Benzaldehyde
Concen: 66.924 ng/ul
RT: 7.034 min Scan# 611
Delta R.T. -0.000 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21




Instrument :
BNA_P
ClientSampleId :
SSTD080621


Tgt Ion: 77 Resp: 591874
Ion Ratio Lower Upper
77 100
105 109.4 87.0 130.6
106 105.4 83.8 125.6



#8
Phenol
Concen: 85.569 ng/ul
RT: 7.087 min Scan# 697
Delta R.T. 0.006 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21

Tgt Ion: 94 Resp: 1694015
Ion Ratio Lower Upper
94 100
65 23.8 19.5 29.3
66 31.8 25.0 37.4









#10
Bis(2-Chloroethyl)ether
Concen: 84.051 ng/ul
RT: 7.322 min Scan# 71
Delta R.T. 0.006 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21




Instrument :
BNA_P
ClientSampleId :
SSTD080621


Tgt Ion: 93 Resp: 1313225
Ion Ratio Lower Upper
93 100
63 67.8 56.2 84.4
95 32.2 25.9 38.9



#12
2-Chlorophenol
Concen: 89.128 ng/ul
RT: 7.457 min Scan# 760
Delta R.T. -0.000 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21

Tgt Ion: 128 Resp: 1397631
Ion Ratio Lower Upper
128 100
64 39.2 31.1 46.7
130 32.4 25.5 38.3





#13

2-Methylphenol

Concen: 88.604 ng/ul

RT: 8.340 min Scan# 910

Delta R.T. -0.000 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21

Instrument :

BNA_P

ClientSampleId :





SSTD080621

Tgt Ion:108 Resp: 1335365

Ion Ratio Lower Upper

108 100

107 87.9 70.2 105.2



#14

2,2'-oxybis(1-Chloropropane)

Concen: 64.207 ng/ul

RT: 8.434 min Scan# 926

Delta R.T. 0.006 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21




Tgt Ion: 45 Resp: 1290444


Ion Ratio Lower Upper

45 100

77 19.7 16.0 24.0

79 15.2 12.5 18.7









#16
Acetophenone
Concen: 83.535 ng/ul
RT: 8.728 min Scan# 976
Delta R.T. -0.000 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21




Instrument :
BNA_P
ClientSampleId :
SSTD080621


Tgt Ion:105 Resp: 1990565
Ion Ratio Lower Upper
105 100
77 70.0 55.4 83.0
51 18.6 15.2 22.8



#17
N-Nitroso-di-n-propylamine
Concen: 83.481 ng/ul
RT: 8.728 min Scan# 976
Delta R.T. 0.018 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21

Tgt Ion: 70 Resp: 926348
Ion Ratio Lower Upper
70 100
42 39.2 32.7 49.1
101 11.0 8.4 12.6
130 26.2 19.4 29.2









#18
4-Methylphenol
Concen: 90.317 ng/ul
RT: 8.681 min Scan# 90
Delta R.T. 0.012 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21




Instrument :
BNA_P
ClientSampleId :
SSTD080621


Tgt Ion:108 Resp: 1457642
Ion Ratio Lower Upper
108 100
107 108.3 88.0 132.0



#19
Hexachloroethane
Concen: 82.409 ng/ul
RT: 8.981 min Scan# 1019
Delta R.T. -0.000 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21

Tgt Ion:117 Resp: 510836
Ion Ratio Lower Upper
117 100
201 106.5 82.4 123.6
199 65.5 51.6 77.4









#22
Nitrobenzene
Concen: 84.619 ng/ul
RT: 9.110 min Scan# 1040
Delta R.T. 0.006 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21




Instrument :
BNA_P
ClientSampleId :
SSTD080621


Tgt Ion: 77 Resp: 1434482
Ion Ratio Lower Upper
77 100
123 54.4 41.6 62.4
65 12.7 9.7 14.5



#23
Isophorone
Concen: 84.143 ng/ul
RT: 9.646 min Scan# 1132
Delta R.T. 0.012 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21

Tgt Ion: 82 Resp: 2890009
Ion Ratio Lower Upper
82 100
95 7.0 5.4 8.2
138 20.4 15.8 23.8









#25
2-Nitrophenol
Concen: 116.690 ng/ul
RT: 9.822 min Scan# 1162
Delta R.T. 0.006 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21




Instrument :
BNA_P
ClientSampleId :
SSTD080621


Tgt Ion:139 Resp: 857445
Ion Ratio Lower Upper
139 100
65 39.7 32.2 48.4
109 25.8 19.6 29.4



#26
2,4-Dimethylphenol
Concen: 82.068 ng/ul
RT: 9.881 min Scan# 1172
Delta R.T. 0.006 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21

Tgt Ion:107 Resp: 1520154
Ion Ratio Lower Upper
107 100
121 52.2 43.0 64.6
122 90.6 74.9 112.3









#27
 Bis(2-Chloroethoxy)methane
 Concen: 80.888 ng/ul
 RT: 10.122 min Scan# 1213
 Delta R.T. 0.006 min
 Lab File: BP011848.D
 Acq: 30 Sep 2022 19:21




Instrument :
 BNA_P
 ClientSampleId :
 SSTD080621


Tgt Ion: 93 Resp: 1800423
 Ion Ratio Lower Upper
 93 100
 95 32.7 26.3 39.5
 123 11.7 9.5 14.3



#29
 2,4-Dichlorophenol
 Concen: 87.130 ng/ul
 RT: 10.357 min Scan# 1253
 Delta R.T. 0.006 min
 Lab File: BP011848.D
 Acq: 30 Sep 2022 19:21

Tgt Ion:162 Resp: 1389304
 Ion Ratio Lower Upper
 162 100
 164 64.6 52.2 78.4
 98 32.7 27.0 40.4









#30
Naphthalene
Concen: 78.957 ng/ul
RT: 10.757 min Scan# 1321
Delta R.T. -0.000 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21




Instrument :
BNA_P
ClientSampleId :
SSTD080621


Tgt Ion:128 Resp: 4475824
Ion Ratio Lower Upper
128 100
129 11.1 8.9 13.3
127 13.1 10.5 15.7



#32
4-Chloroaniline
Concen: 83.138 ng/ul
RT: 10.875 min Scan# 1341
Delta R.T. 0.006 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21

Tgt Ion:127 Resp: 2021809
Ion Ratio Lower Upper
127 100
129 32.4 26.6 39.8









#33
Hexachlorobutadiene
Concen: 75.116 ng/ul
RT: 11.040 min Scan# 11
Delta R.T. -0.000 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21




Instrument :
BNA_P
ClientSampleId :
SSTD080621


Tgt Ion:225 Resp: 797654
Ion Ratio Lower Upper
225 100
223 63.0 52.1 78.1
227 63.1 52.3 78.5



#34
Caprolactam
Concen: 57.083 ng/ul
RT: 11.687 min Scan# 1479
Delta R.T. 0.035 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21

Tgt Ion:113 Resp: 267500
Ion Ratio Lower Upper
113 100
55 132.7 106.0 159.0
56 96.7 78.7 118.1









#35
4-Chloro-3-methylphenol
Concen: 91.905 ng/ul
RT: 11.998 min Scan# 11
Delta R.T. 0.012 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21




Instrument :
BNA_P
ClientSampleId :
SSTD080621


Tgt Ion:107 Resp: 1456890
Ion Ratio Lower Upper
107 100
144 28.2 22.5 33.7
142 87.4 70.0 105.0



#36
2-Methylnaphthalene
Concen: 82.483 ng/ul
RT: 12.369 min Scan# 1595
Delta R.T. 0.006 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21

Tgt Ion:142 Resp: 3132813
Ion Ratio Lower Upper
142 100
141 88.4 70.6 106.0





#37

1-Methylnaphthalene

Concen: 82.309 ng/ul

RT: 12.587 min Scan# 1632

Delta R.T. -0.000 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21

Instrument :

BNA_P

ClientSampleId :

SSTD080621





Tgt Ion:142 Resp: 3133439

Ion Ratio Lower Upper

142 100

141 92.4 74.8 112.2

116 3.6 2.9 4.3



#39

1,2,4,5-Tetrachlorobenzene

Concen: 75.284 ng/ul

RT: 12.734 min Scan# 1657

Delta R.T. -0.000 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21

Tgt Ion:216 Resp: 1630384




Ion Ratio Lower Upper


216 100

214 80.1 62.6 94.0

179 21.1 16.6 24.8

108 16.3 12.6 19.0





#40

Hexachlorocyclopentadiene

Concen: 74.723 ng/ul

RT: 12.716 min Scan# 1653

Delta R.T. 0.006 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21

Instrument :

BNA_P

ClientSampleId :

SSTD080621





Tgt Ion:237 Resp: 962155

Ion Ratio Lower Upper

237 100

235 63.1 51.0 76.6

272 13.1 10.5 15.7



#41

2,4,6-Trichlorophenol

Concen: 94.036 ng/ul

RT: 12.975 min Scan# 1698

Delta R.T. -0.000 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21




Tgt Ion:196 Resp: 1151694


Ion Ratio Lower Upper

196 100

198 95.0 78.7 118.1

200 30.5 24.5 36.7





#42

2,4,5-Trichlorophenol

Concen: 93.246 ng/ul

RT: 13.045 min Scan# 1710

Delta R.T. -0.000 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21

Instrument :

BNA_P

ClientSampleId :

SSTD080621





Tgt Ion:196 Resp: 1254328

Ion Ratio Lower Upper

196 100

198 94.7 76.6 114.8

200 31.1 25.6 38.4



#43

1,1'-Biphenyl

Concen: 73.953 ng/ul

RT: 13.375 min Scan# 1766

Delta R.T. -0.000 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21




Tgt Ion:154 Resp: 3965651


Ion Ratio Lower Upper

154 100

153 40.3 31.8 47.6

76 11.9 9.5 14.3





#44

2-Chloronaphthalene

Concen: 77.828 ng/ul

RT: 13.422 min Scan# 11

Delta R.T. 0.006 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21

Instrument :

BNA_P

ClientSampleId :

SSTD080621





Tgt Ion:162 Resp: 3195885

Ion Ratio Lower Upper

162 100

164 33.3 26.5 39.7

127 37.6 29.7 44.5



#45

2-Nitroaniline

Concen: 101.270 ng/ul

RT: 13.628 min Scan# 1809

Delta R.T. 0.006 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21




Tgt Ion: 65 Resp: 861423


Ion Ratio Lower Upper

65 100

92 78.7 61.2 91.8

138 137.6 103.0 154.4





#47

Dimethylphthalate

Concen: 82.711 ng/ul

RT: 14.010 min Scan# 1874

Delta R.T. 0.012 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21

Instrument :

BNA_P

ClientSampleId :

SSTD080621





Tgt Ion:163 Resp: 4053980

Ion Ratio Lower Upper

163 100

194 4.1 3.3 4.9

164 10.1 8.5 12.7



#48

2,6-Dinitrotoluene

Concen: 115.562 ng/ul

RT: 14.128 min Scan# 1894

Delta R.T. 0.006 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21




Tgt Ion:165 Resp: 907680


Ion Ratio Lower Upper

165 100

89 48.1 39.1 58.7

121 19.8 16.7 25.1









#50
Acenaphthylene
Concen: 74.921 ng/ul
RT: 14.269 min Scan# 1917
Delta R.T. 0.006 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21




Instrument :
BNA_P
ClientSampleId :
SSTD080621


Tgt Ion:152 Resp: 4891547
Ion Ratio Lower Upper
152 100
151 20.5 16.0 24.0
153 13.4 10.8 16.2



#51
3-Nitroaniline
Concen: 101.489 ng/ul
RT: 14.457 min Scan# 1950
Delta R.T. 0.006 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21

Tgt Ion:138 Resp: 953620
Ion Ratio Lower Upper
138 100
108 9.3 8.2 12.4
92 102.7 85.6 128.4









#52
Acenaphthene
Concen: 79.968 ng/ul
RT: 14.610 min Scan# 1976
Delta R.T. 0.006 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21




Instrument :
BNA_P
ClientSampleId :
SSTD080621


Tgt Ion:153 Resp: 3414294
Ion Ratio Lower Upper
153 100
152 48.0 38.4 57.6
154 87.9 70.6 105.8



#53
2,4-Dinitrophenol
Concen: 181.154 ng/ul
RT: 14.657 min Scan# 1984
Delta R.T. 0.006 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21

Tgt Ion:184 Resp: 622965
Ion Ratio Lower Upper
184 100
63 49.4 44.2 66.4
154 58.0 45.8 68.6









#55
4-Nitrophenol
Concen: 88.981 ng/ul
RT: 14.769 min Scan# 2000
Delta R.T. 0.018 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21




Instrument :
BNA_P
ClientSampleId :
SSTD080621


Tgt Ion:109 Resp: 570323
Ion Ratio Lower Upper
109 100
139 158.4 125.0 187.6
65 122.8 101.9 152.9



#56
Dibenzofuran
Concen: 76.518 ng/ul
RT: 14.945 min Scan# 2033
Delta R.T. 0.006 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21

Tgt Ion:168 Resp: 4634173
Ion Ratio Lower Upper
168 100
139 37.5 29.4 44.2





#57

2,4-Dinitrotoluene

Concen: 118.026 ng/ul

RT: 14.916 min Scan# 2026

Delta R.T. 0.012 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21

Instrument :

BNA_P

ClientSampleId :

SSTD080621





Tgt Ion:165 Resp: 1290914

Ion Ratio Lower Upper

165 100

63 31.7 28.2 42.2

182 2.6 2.2 3.4



#58

2,3,4,6-Tetrachlorophenol

Concen: 106.429 ng/ul

RT: 15.169 min Scan# 2071

Delta R.T. 0.006 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21

Tgt Ion:232 Resp: 1078076




Ion Ratio Lower Upper


232 100

131 43.5 36.2 54.2

130 2.1 1.7 2.5

166 30.7 25.0 37.4









#59
Diethylphthalate
Concen: 86.184 ng/ul
RT: 15.375 min Scan# 2106
Delta R.T. 0.012 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21




Instrument :
BNA_P
ClientSampleId :
SSTD080621


Tgt Ion:149 Resp: 4113533
Ion Ratio Lower Upper
149 100
177 22.9 17.8 26.8
150 12.6 9.9 14.9



#61
Fluorene
Concen: 74.298 ng/ul
RT: 15.598 min Scan# 2144
Delta R.T. 0.006 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21

Tgt Ion:166 Resp: 3637147
Ion Ratio Lower Upper
166 100
165 96.4 77.2 115.8
167 13.4 10.7 16.1









#62
4-Chlorophenyl-phenylether
Concen: 74.860 ng/ul
RT: 15.586 min Scan# 2142
Delta R.T. -0.000 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21




Instrument :
BNA_P
ClientSampleId :
SSTD080621


Tgt Ion:204 Resp: 1857350
Ion Ratio Lower Upper
204 100
206 33.2 26.8 40.2
141 55.4 44.5 66.7



#63
4-Nitroaniline
Concen: 95.965 ng/ul
RT: 15.628 min Scan# 2149
Delta R.T. 0.012 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21

Tgt Ion:138 Resp: 851011
Ion Ratio Lower Upper
138 100
92 45.6 35.9 53.9
108 66.4 51.6 77.4









#66
4,6-Dinitro-2-methylphenol
Concen: 133.175 ng/ul
RT: 15.681 min Scan# 2156
Delta R.T. 0.012 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21




Instrument :
BNA_P
ClientSampleId :
SSTD080621


Tgt Ion:198 Resp: 811101
Ion Ratio Lower Upper
198 100
182 3.1 3.7 5.5#
77 19.0 16.6 24.8



#67
N-Nitrosodiphenylamine
Concen: 77.115 ng/ul
RT: 15.804 min Scan# 2179
Delta R.T. -0.000 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21

Tgt Ion:169 Resp: 3349340
Ion Ratio Lower Upper
169 100
168 66.8 53.7 80.5
167 37.6 29.9 44.9









#68
4-Bromophenyl-phenylether
Concen: 78.610 ng/ul
RT: 16.486 min Scan# 21
Delta R.T. -0.000 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21




Instrument :
BNA_P
ClientSampleId :
SSTD080621


Tgt Ion:248 Resp: 1231829
Ion Ratio Lower Upper
248 100
250 97.4 78.6 118.0
141 69.2 56.0 84.0



#69
Hexachlorobenzene
Concen: 74.917 ng/ul
RT: 16.604 min Scan# 2315
Delta R.T. 0.006 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21

Tgt Ion:284 Resp: 1392818
Ion Ratio Lower Upper
284 100
142 32.2 27.3 40.9
249 31.1 25.2 37.8









#70
Atrazine
Concen: 81.380 ng/ul
RT: 16.769 min Scan# 21
Delta R.T. 0.012 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21




Instrument :
BNA_P
ClientSampleId :
SSTD080621


Tgt Ion:200 Resp: 1282670
Ion Ratio Lower Upper
200 100
173 26.6 21.6 32.4
215 49.0 38.9 58.3



#71
Pentachlorophenol
Concen: 96.184 ng/ul
RT: 16.945 min Scan# 2373
Delta R.T. -0.000 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21

Tgt Ion:266 Resp: 955610
Ion Ratio Lower Upper
266 100
264 64.1 49.8 74.8
268 64.0 51.9 77.9





#72

Phenanthrene

Concen: 78.034 ng/ul

RT: 17.345 min Scan# 2441

Delta R.T. 0.006 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21

Instrument :

BNA_P

ClientSampleId :

SSTD080621





Tgt Ion:178 Resp: 6193518

Ion Ratio Lower Upper

178 100

179 16.2 12.5 18.7

176 20.6 15.4 23.2



#74

Anthracene

Concen: 77.342 ng/ul

RT: 17.439 min Scan# 2457

Delta R.T. 0.006 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21




Tgt Ion:178 Resp: 6146007


Ion Ratio Lower Upper

178 100

179 16.3 12.3 18.5

176 20.0 15.4 23.2









#75
1,2,3,4-Tetrachlorobenzene
Concen: 70.948 ng/uL
RT: 13.339 min Scan# 1760
Delta R.T. -0.000 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21




Instrument :
BNA_P
ClientSampleId :
SSTD080621


Tgt Ion:216 Resp: 1655819
Ion Ratio Lower Upper
216 100
214 79.7 62.6 93.8
218 49.2 37.4 56.0



#76
Pentachlorobenzene
Concen: 78.831 ng/uL
RT: 14.863 min Scan# 2019
Delta R.T. 0.006 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21

Tgt Ion:250 Resp: 1737406
Ion Ratio Lower Upper
250 100
248 64.0 51.4 77.0
252 64.3 51.5 77.3





#77

Carbazole

Concen: 83.667 ng/ul

RT: 17.710 min Scan# 2503

Delta R.T. 0.006 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21

Instrument :

BNA_P

ClientSampleId :

SSTD080621





Tgt Ion:167 Resp: 5858969

Ion Ratio Lower Upper

167 100

166 22.3 17.1 25.7

139 13.2 10.1 15.1



#78

Di-n-butylphthalate

Concen: 89.521 ng/ul

RT: 18.257 min Scan# 2596

Delta R.T. 0.006 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21




Tgt Ion:149 Resp: 7115749


Ion Ratio Lower Upper

149 100

150 9.7 7.5 11.3

104 4.5 3.6 5.4





#80

Fluoranthene

Concen: 76.635 ng/ul

RT: 19.310 min Scan# 21

Delta R.T. 0.006 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21

Instrument :

BNA_P

ClientSampleId :

SSTD080621





Tgt Ion:202 Resp: 7204309

Ion Ratio Lower Upper

202 100

101 10.8 9.8 14.6

100 8.0 7.4 11.0



#82

Pyrene

Concen: 75.268 ng/ul

RT: 19.663 min Scan# 2835

Delta R.T. 0.006 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21




Tgt Ion:202 Resp: 7299257


Ion Ratio Lower Upper

202 100

101 12.9 11.6 17.4

100 10.2 9.4 14.0





#83

Butylbenzylphthalate

Concen: 111.277 ng/ul

RT: 20.533 min Scan# 2983

Delta R.T. -0.000 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21

Instrument :

BNA_P

ClientSampleId :

SSTD080621





Tgt Ion:149 Resp: 3498847

Ion Ratio Lower Upper

149 100

91 59.8 50.2 75.4

206 22.9 16.9 25.3



#84

3,3'-Dichlorobenzidine

Concen: 104.189 ng/ul

RT: 21.304 min Scan# 3114

Delta R.T. -0.000 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21




Tgt Ion:252 Resp: 2776167


Ion Ratio Lower Upper

252 100

254 63.5 51.4 77.0

126 11.0 8.9 13.3









#85
Benzo(a)anthracene
Concen: 80.623 ng/ul
RT: 21.374 min Scan# 3125
Delta R.T. 0.006 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21




Instrument :
BNA_P
ClientSampleId :
SSTD080621


Tgt Ion:228 Resp: 7474428
Ion Ratio Lower Upper
228 100
229 20.5 15.8 23.6
226 29.9 22.0 33.0



#86
Bis(2-ethylhexyl)phthalate
Concen: 95.257 ng/ul
RT: 21.292 min Scan# 3112
Delta R.T. 0.006 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21

Tgt Ion:149 Resp: 4778000
Ion Ratio Lower Upper
149 100
167 29.8 21.2 31.8
279 5.5 2.9 4.3#





#87

Chrysene

Concen: 77.225 ng/ul

RT: 21.427 min Scan# 3134

Delta R.T. 0.006 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21

Instrument :

BNA_P

ClientSampleId :

SSTD080621





Tgt Ion:228 Resp: 6913572

Ion Ratio Lower Upper

228 100

226 32.8 25.3 37.9

229 20.5 16.2 24.2



#89

Di-n-octyl phthalate

Concen: 92.377 ng/ul




RT: 22.227 min Scan# 3271


Delta R.T. -0.000 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21

Tgt Ion:149 Resp: 8889977









#90
Benzo(b)fluoranthene
Concen: 78.958 ng/ul
RT: 23.086 min Scan# 3415
Delta R.T. 0.012 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21




Instrument :
BNA_P
ClientSampleId :
SSTD080621


Tgt Ion:252 Resp: 8640935
Ion Ratio Lower Upper
252 100
253 23.0 17.8 26.8
125 10.4 9.2 13.8



#91
Benzo(k)fluoranthene
Concen: 75.765 ng/ul
RT: 23.133 min Scan# 3425
Delta R.T. 0.012 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21

Tgt Ion:252 Resp: 7937187
Ion Ratio Lower Upper
252 100
253 23.2 18.0 27.0
125 10.5 9.2 13.8









#93
Benzo(a)pyrene
Concen: 72.013 ng/ul
RT: 23.727 min Scan# 31
Delta R.T. 0.012 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21




Instrument :
BNA_P
ClientSampleId :
SSTD080621


Tgt Ion:252 Resp: 7639491
Ion Ratio Lower Upper
252 100
253 22.7 17.7 26.5
125 11.6 9.8 14.8



#94
Indeno(1,2,3-cd)pyrene
Concen: 81.308 ng/ul
RT: 26.386 min Scan# 3978
Delta R.T. 0.023 min
Lab File: BP011848.D
Acq: 30 Sep 2022 19:21

Tgt Ion:276 Resp: 9954995
Ion Ratio Lower Upper
276 100
138 26.3 21.4 32.0
277 25.0 19.9 29.9





#95

Dibenzo(a,h)anthracene

Concen: 81.067 ng/ul

RT: 26.409 min Scan# 3977

Delta R.T. 0.029 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21

Instrument :

BNA_P

ClientSampleId :

SSTD080621





Tgt Ion:278 Resp: 8557517

Ion Ratio Lower Upper

278 100

139 17.0 15.0 22.6

279 24.5 19.0 28.6



#96

Benzo(g,h,i)perylene

Concen: 87.829 ng/ul

RT: 27.180 min Scan# 4113

Delta R.T. 0.035 min

Lab File: BP011848.D

Acq: 30 Sep 2022 19:21

Tgt Ion:276 Resp: 8970479

Ion Ratio Lower Upper

276 100

138 24.0 19.8 29.6

277 24.3 18.6 27.8

