
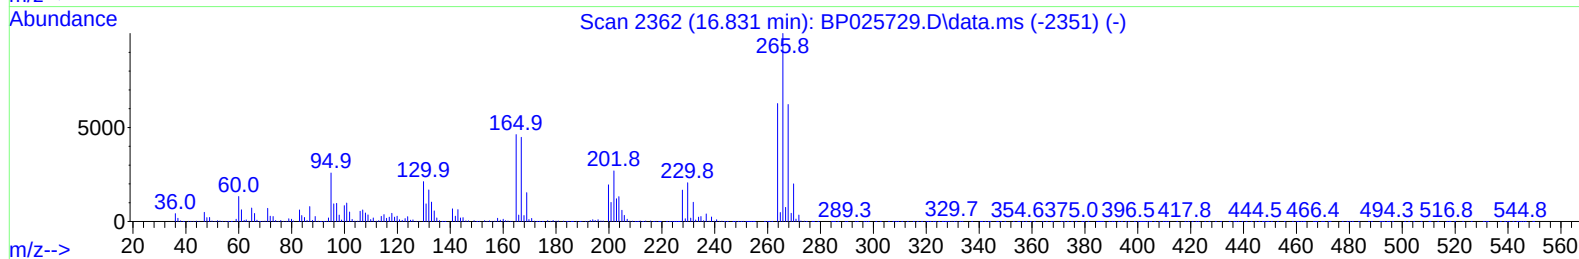
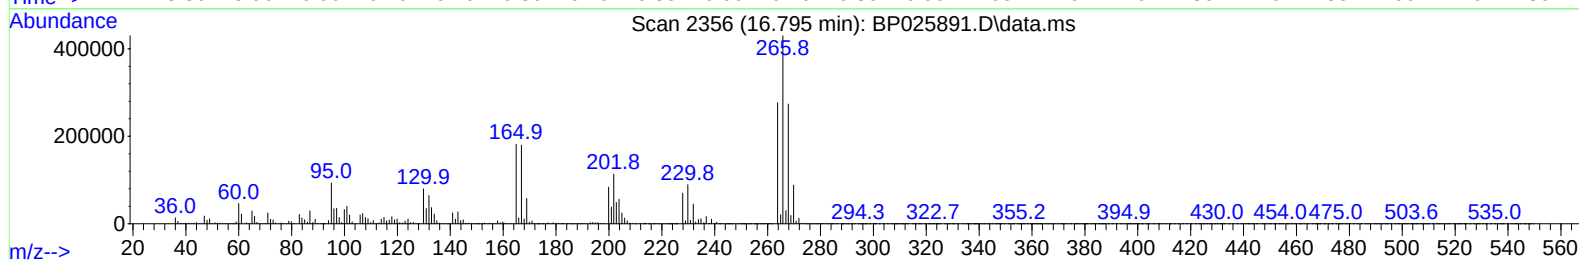


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093025\
Data File : BP025891.D
Acq On : 30 Sep 2025 14:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 15:07:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

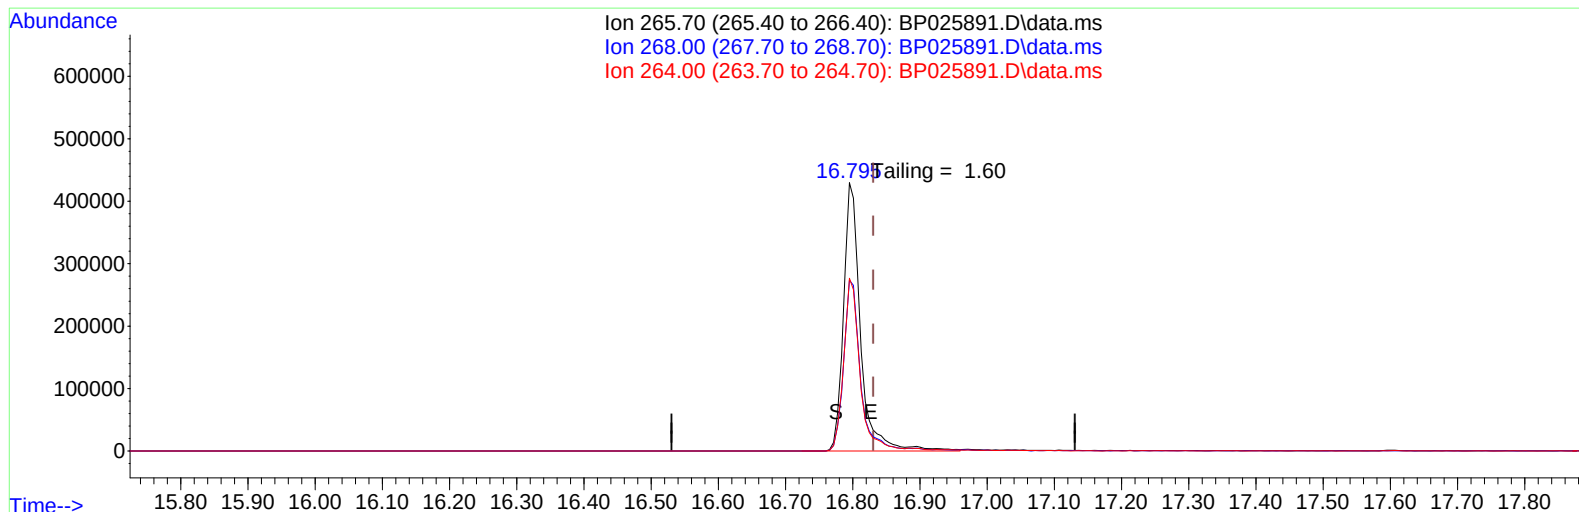

TIC: BP025891.D\data.ms

(70) Pentachlorophenol (C)




16.795min (-0.036) 1604261.33 ng

response 739379

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.70
264.00	62.70	64.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP093025\
Data File : BP025891.D
Acq On : 30 Sep 2025 14:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 15:07:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

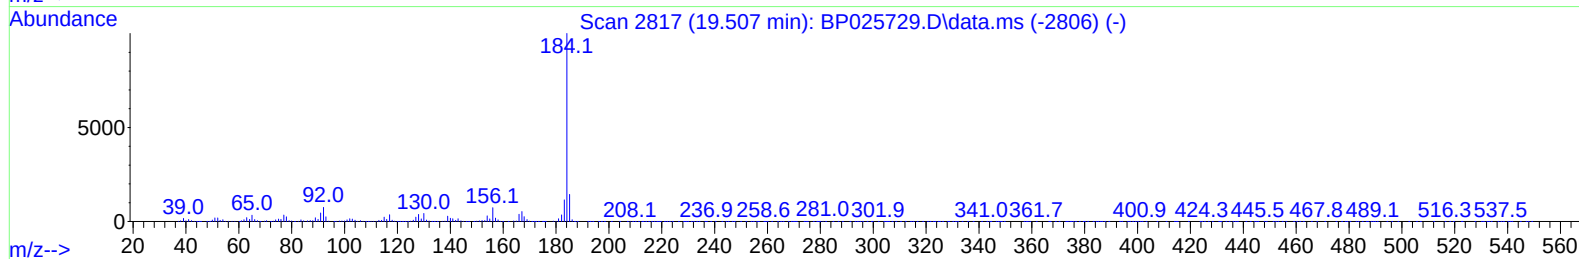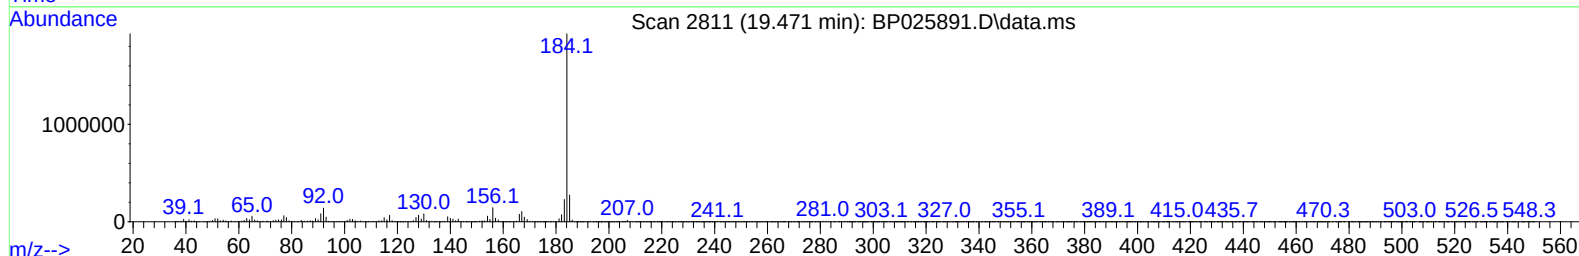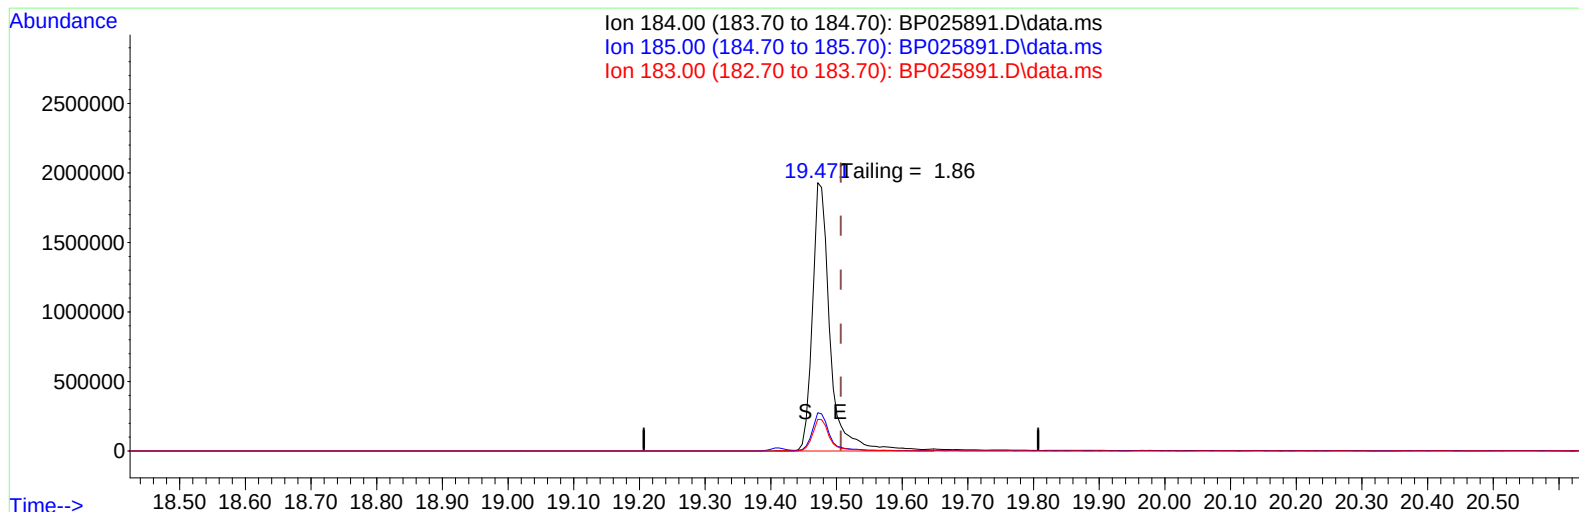

TIC: BP025891.D\data.ms

(77) Benzidine

19.471min (-0.036) 176773.01 ng

response 3574590

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.25
183.00	11.50	11.80
0.00	0.00	0.00