


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100119\
Data File : BP000477.D
Acq On : 01 Oct 2019 11:09
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 01 18:03:42 2019

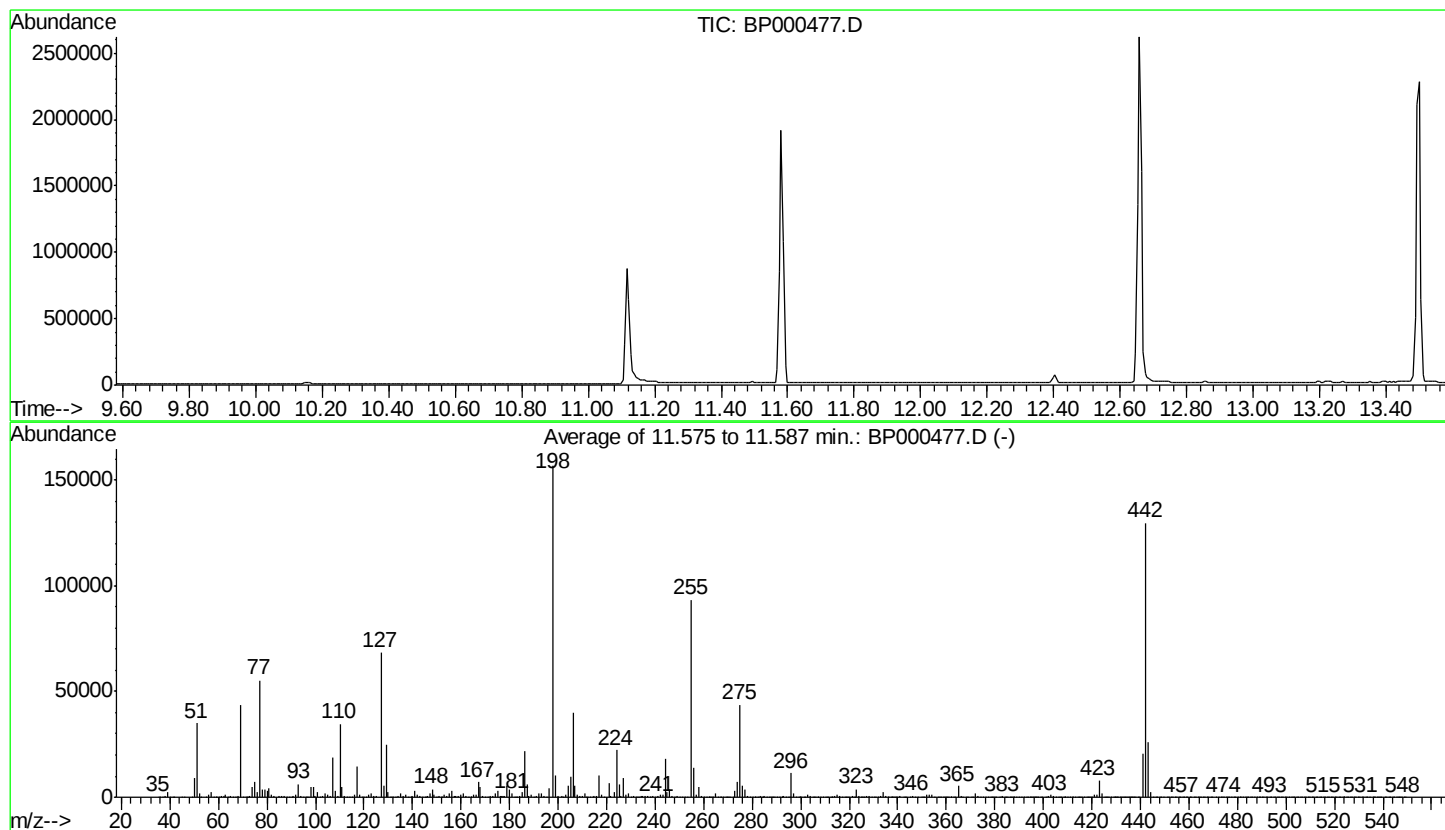

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.3	35032	PASS
68	69	0.00	2	1.8	796	PASS
69	198	0.00	100	27.9	43786	PASS
70	69	0.00	2	0.6	247	PASS
127	198	10	80	43.5	68191	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	156849	PASS
199	198	5	9	6.7	10458	PASS
275	198	10	60	27.9	43733	PASS
365	198	1	100	3.4	5299	PASS
441	198	0.01	100	13.1	20570	PASS
442	198	50	100	82.7	129688	PASS
443	442	15	24	19.9	25814	PASS