
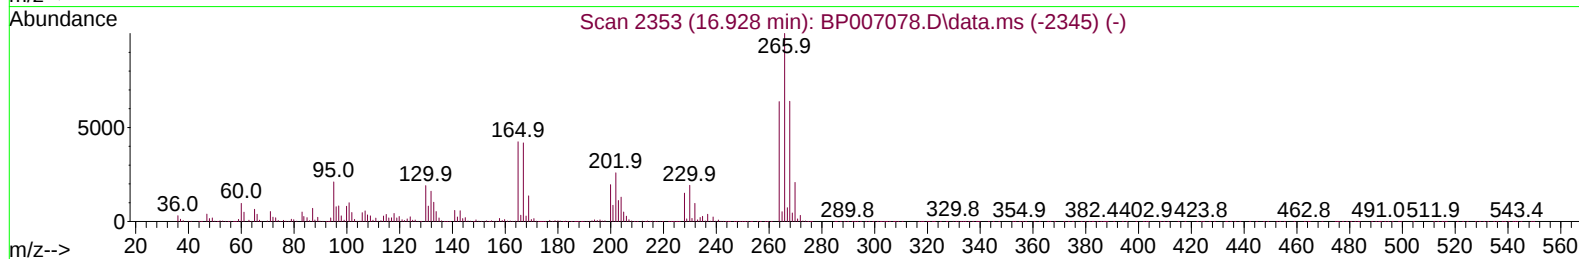
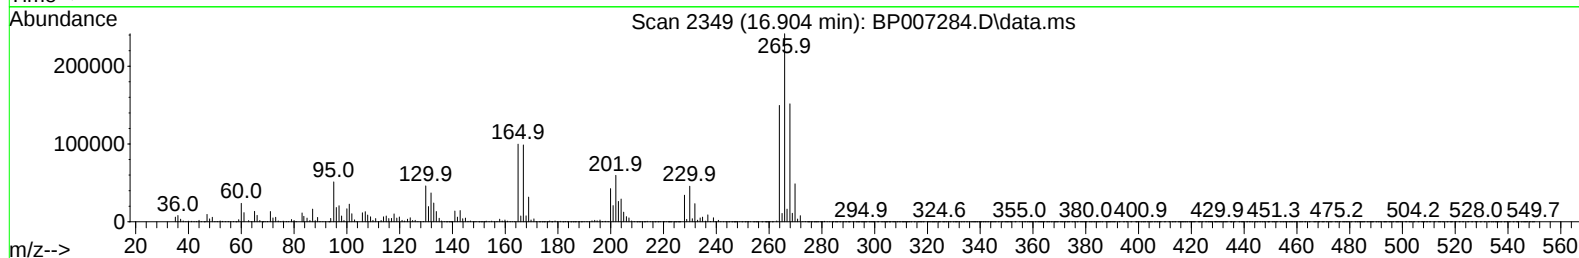


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100121\
 Data File : BP007284.D
 Acq On : 01 Oct 2021 10:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 01 12:42:35 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 29 14:45:49 2021
 Response via : Initial Calibration



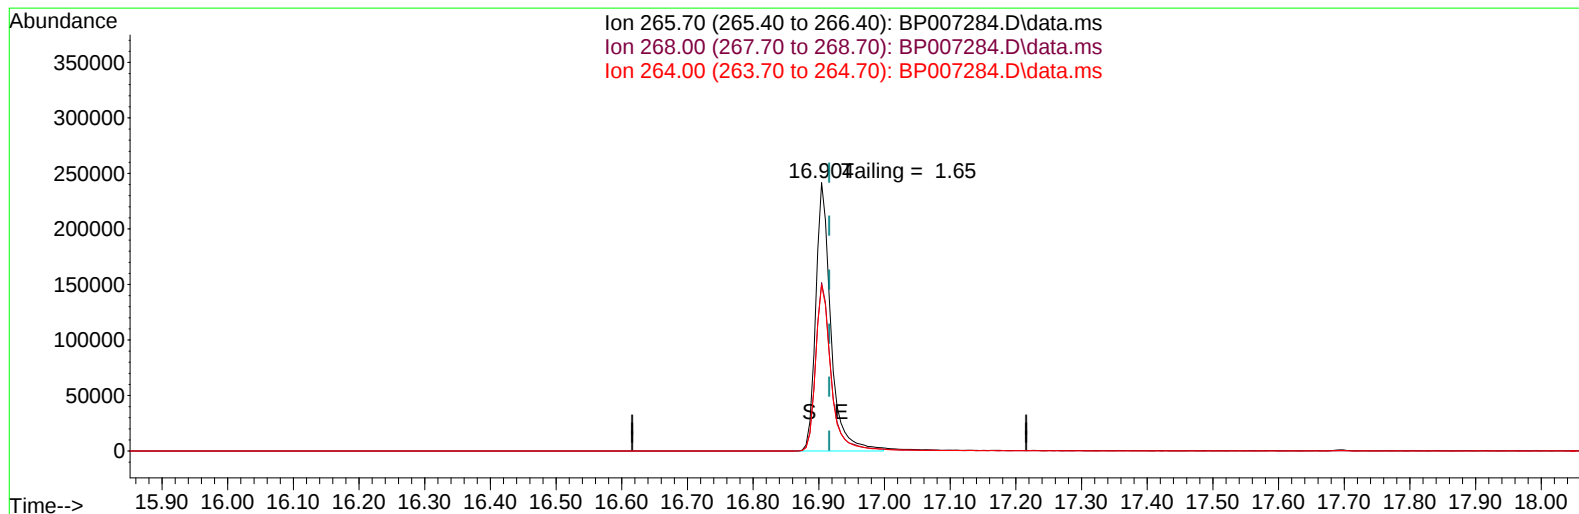


TIC: BP007284.D\data.ms

(70) Pentachlorophenol (C)**16.904min (-0.012) 4019333.10 ng****response 393052**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.72
264.00	62.90	61.90
0.00	0.00	0.00

Quant Time: Oct 01 12:42:35 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 29 14:45:49 2021
Response via : Initial Calibration

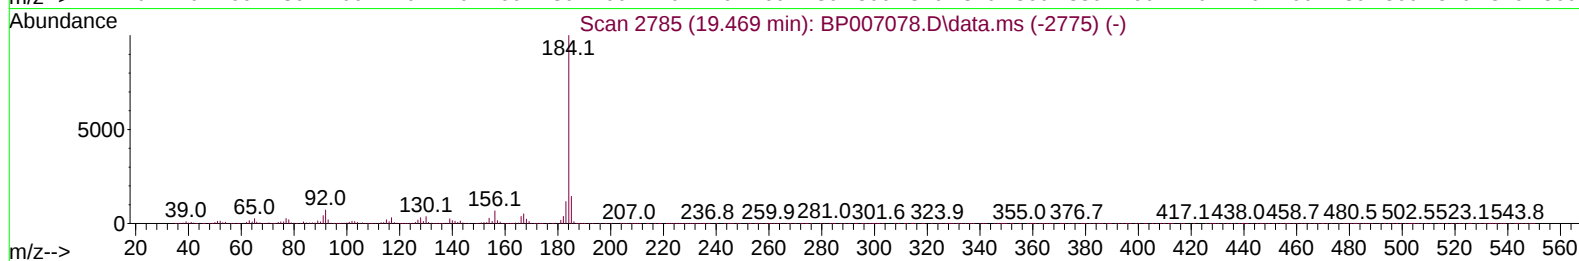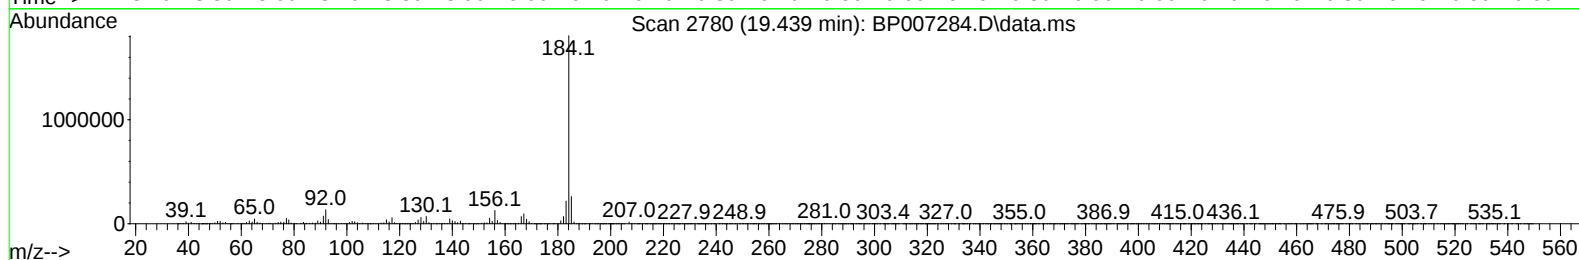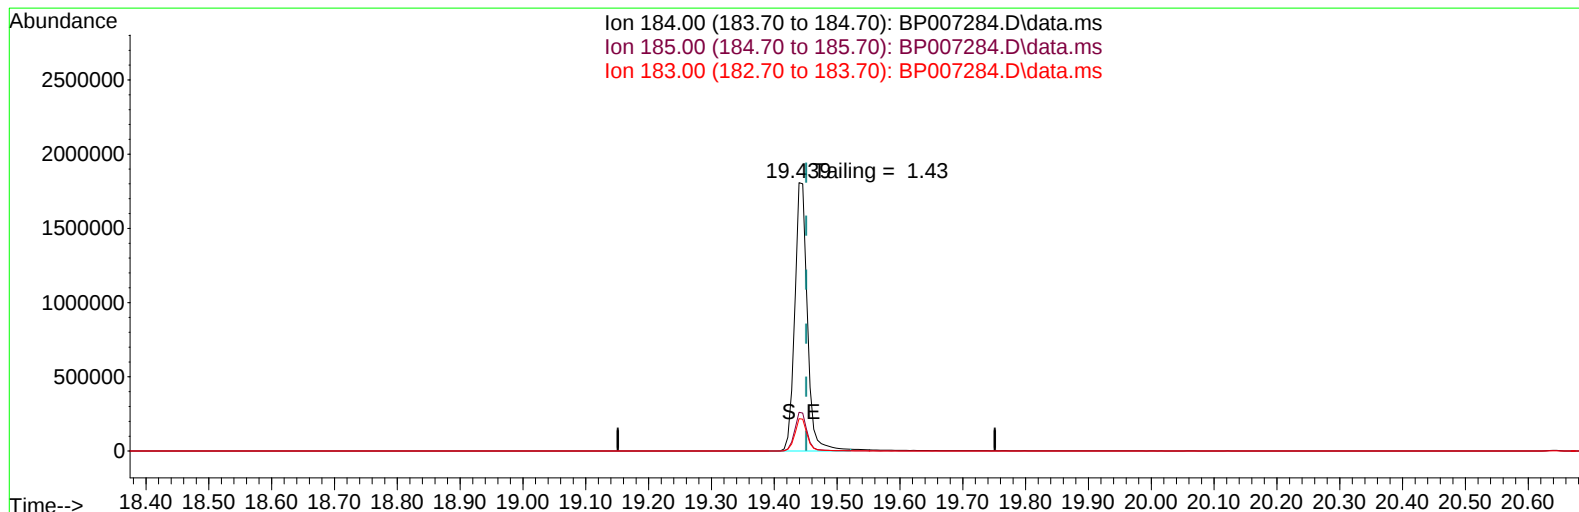

TIC: BP007284.D\data.ms

(77) Benzidine

19.439min (-0.012) 317549.46 ng

response **2576321**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.47
183.00	11.90	12.07
0.00	0.00	0.00