

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100121\
 Data File : BP007286.D
 Acq On : 01 Oct 2021 12:12
 Operator : CG/JU
 Sample : PB139478BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB139478BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007286.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.446	395	401	417	rBV	2540093	3714836	35.32%	8.843%
2	7.046	666	673	697	rBV	2387013	3918401	37.26%	9.328%
3	7.863	805	812	821	rBV	603044	937304	8.91%	2.231%
4	9.028	1001	1010	1029	rBV	1420469	2440050	23.20%	5.808%
5	10.663	1280	1288	1306	rBV	676117	1273596	12.11%	3.032%
6	13.122	1699	1706	1725	rBV	3777018	6100325	58.01%	14.521%
7	14.504	1933	1941	1955	rBV	1061195	1696980	16.14%	4.040%
8	15.992	2187	2194	2224	rBV	2968590	4656831	44.28%	11.085%
9	17.251	2401	2408	2421	rBV	1257674	2057307	19.56%	4.897%
10	19.810	2838	2843	2856	rBV	8434756	10516619	100.00%	25.034%
11	21.339	3098	3103	3111	rBV	1735672	2345043	22.30%	5.582%
12	23.745	3506	3512	3522	rVB2	1115313	2351756	22.36%	5.598%




Sum of corrected areas: 42009048

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100121\
Data File : BP007286.D
Acq On : 01 Oct 2021 12:12
Operator : CG/JU
Sample : PB139478BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139478BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

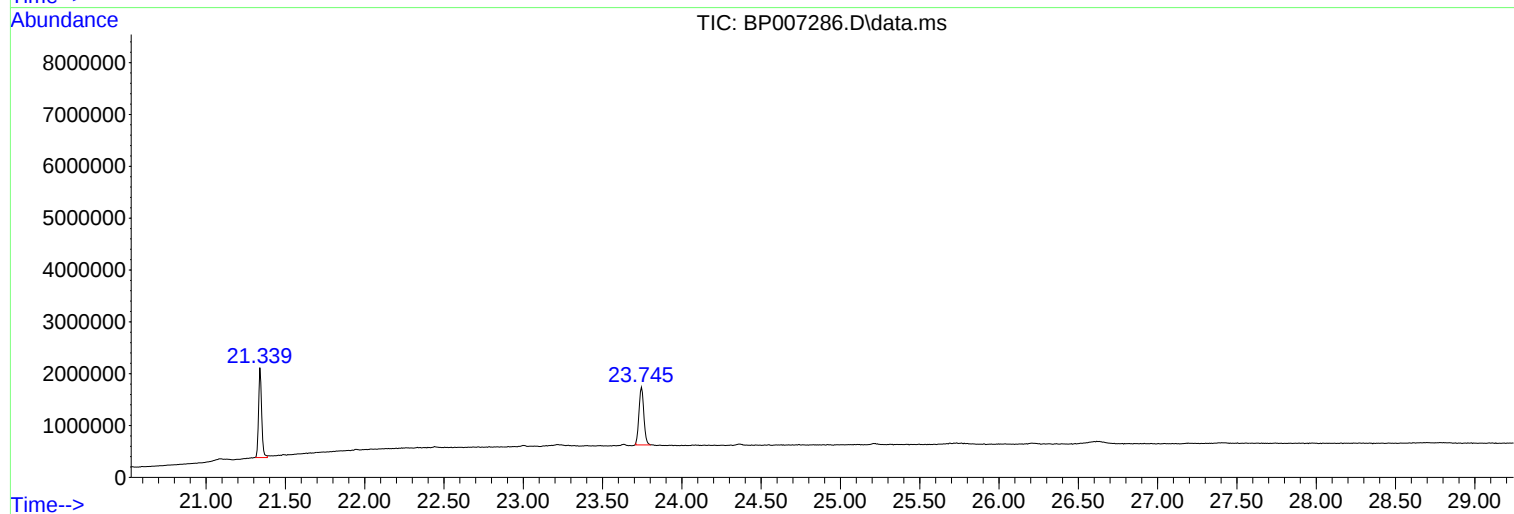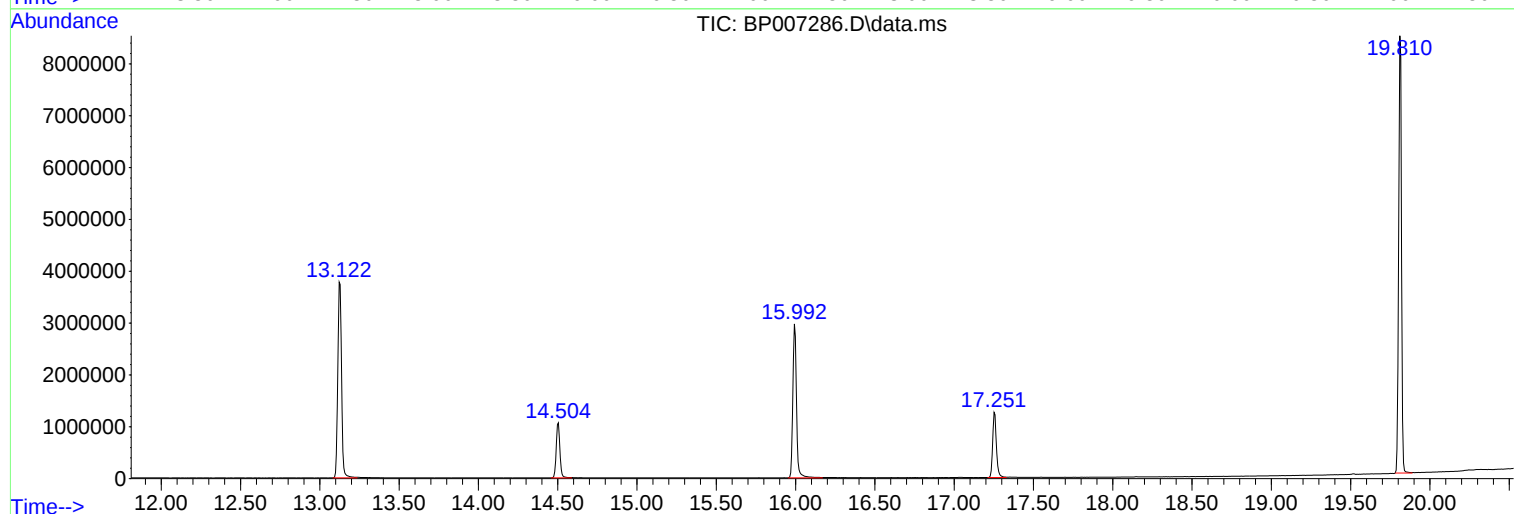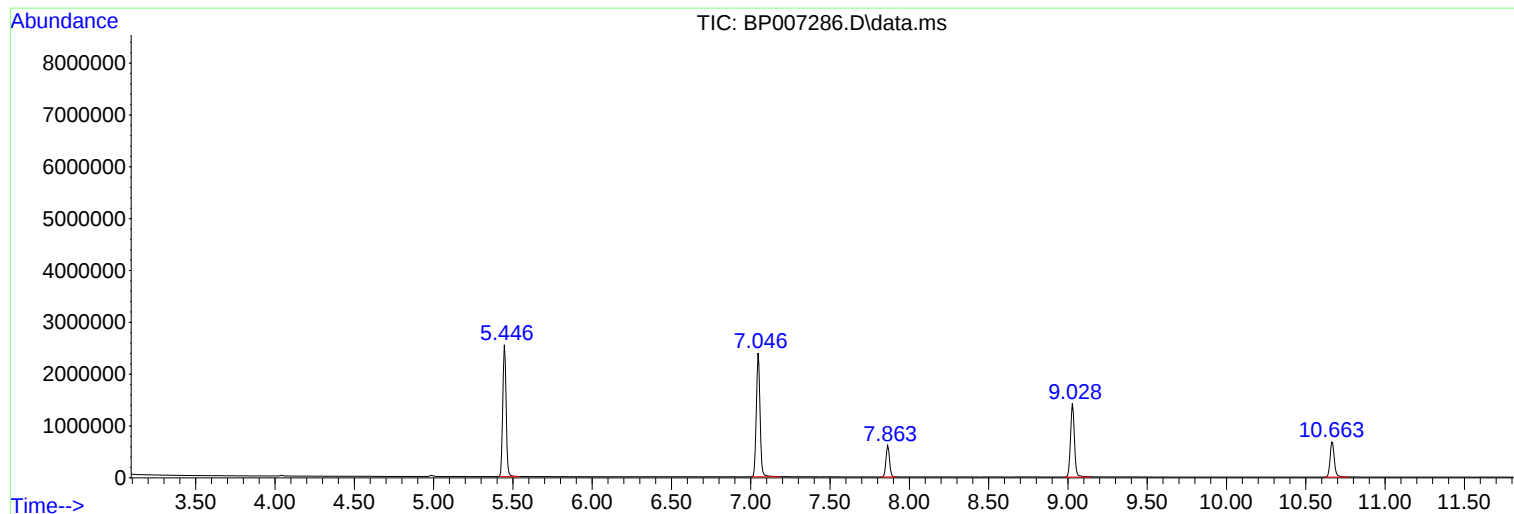

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100121\
Data File : BP007286.D
Acq On : 01 Oct 2021 12:12
Operator : CG/JU
Sample : PB139478BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139478BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100121\
Data File : BP007286.D
Acq On : 01 Oct 2021 12:12
Operator : CG/JU
Sample : PB139478BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB139478BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------