

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100121\
 Data File : BP007292.D
 Acq On : 01 Oct 2021 15:54
 Operator : CG/JU
 Sample : M4005-18 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BU-08-093021

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP007292.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.452	396	402	410	rBV	486292	744501	25.99%	3.785%
2	7.052	664	674	688	rBV	417745	730807	25.51%	3.715%
3	7.869	804	813	822	rBV	775365	1257436	43.90%	6.393%
4	9.034	1004	1011	1019	rBV	247505	444598	15.52%	2.260%
5	10.469	1247	1255	1263	rBV	26307	66962	2.34%	0.340%
6	10.663	1279	1288	1300	rBV	978490	1749294	61.07%	8.893%
7	12.087	1524	1530	1538	rBV2	22418	38038	1.33%	0.193%
8	13.122	1700	1706	1718	rBV	732415	1152129	40.22%	5.857%
9	13.328	1737	1741	1748	rVB	33041	48681	1.70%	0.247%
10	14.398	1914	1923	1929	rBV2	46072	92560	3.23%	0.471%
11	14.498	1932	1940	1955	rBV	1512345	2352681	82.14%	11.961%
12	15.351	2081	2085	2090	rVB	41242	50016	1.75%	0.254%
13	15.992	2189	2194	2208	rBV	540063	802576	28.02%	4.080%
14	16.216	2228	2232	2240	rVB	42486	86098	3.01%	0.438%
15	17.010	2363	2367	2370	rBV	36392	48960	1.71%	0.249%
16	17.251	2402	2408	2420	rBV	1896861	2750021	96.01%	13.981%
17	18.139	2556	2559	2563	rBV2	78238	111370	3.89%	0.566%
18	19.810	2839	2843	2847	rBV	1346201	1570389	54.83%	7.984%
19	21.339	3099	3103	3107	rVB	2254839	2708968	94.58%	13.772%
20	23.751	3508	3513	3519	rVB2	1504002	2864284	100.00%	14.561%




Sum of corrected areas: 19670369

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100121\
Data File : BP007292.D
Acq On : 01 Oct 2021 15:54
Operator : CG/JU
Sample : M4005-18 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BU-08-093021

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

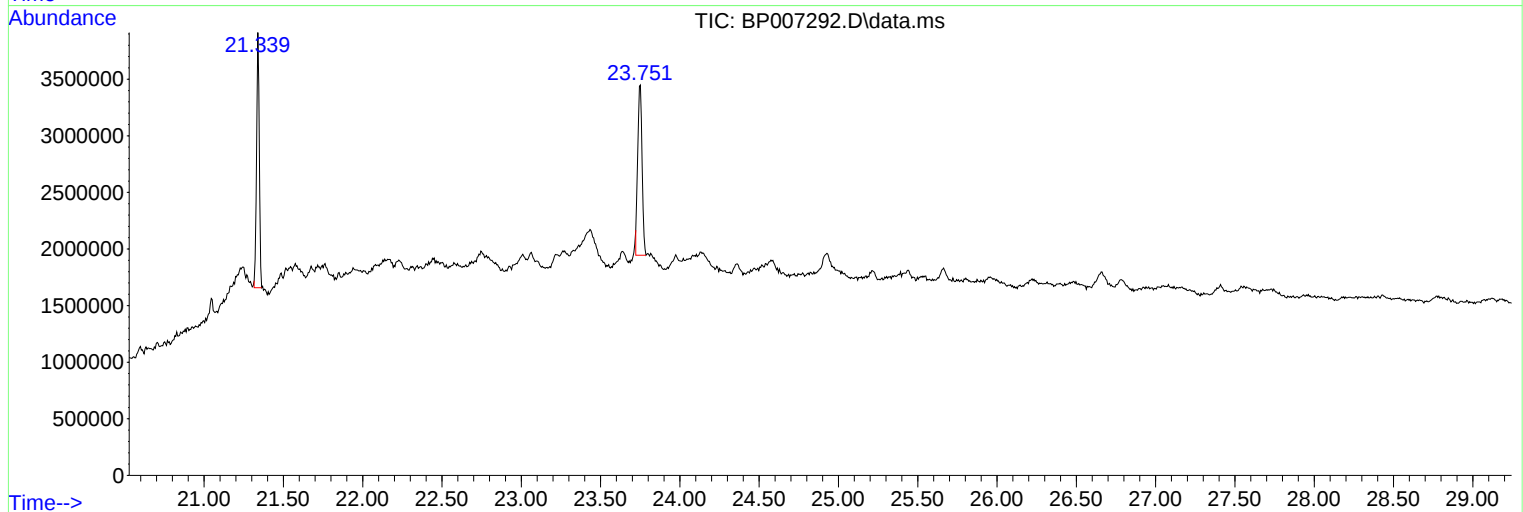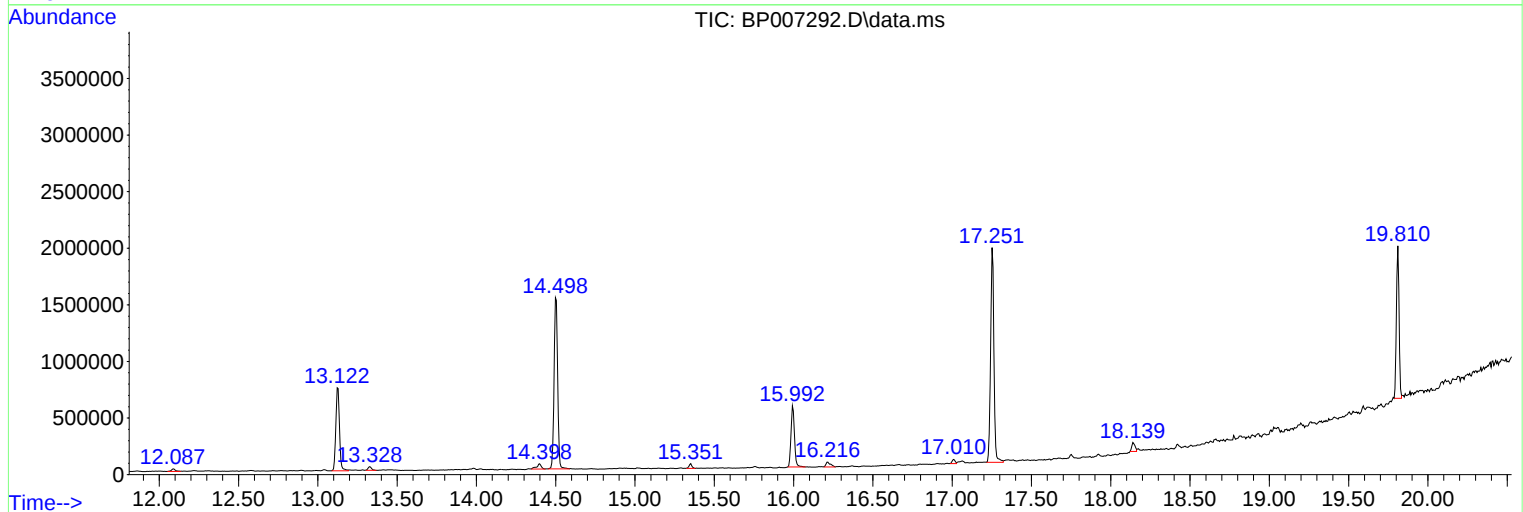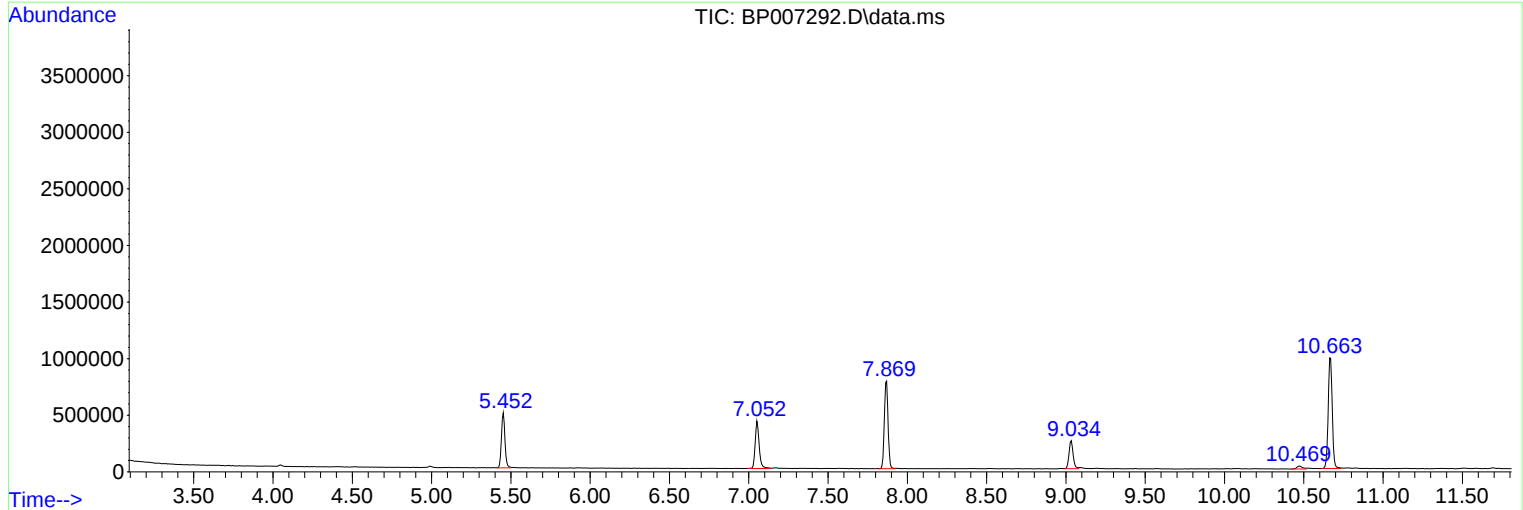

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100121\
Data File : BP007292.D
Acq On : 01 Oct 2021 15:54
Operator : CG/JU
Sample : M4005-18 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BU-08-093021

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100121\
Data File : BP007292.D
Acq On : 01 Oct 2021 15:54
Operator : CG/JU
Sample : M4005-18 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BU-08-093021

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
