
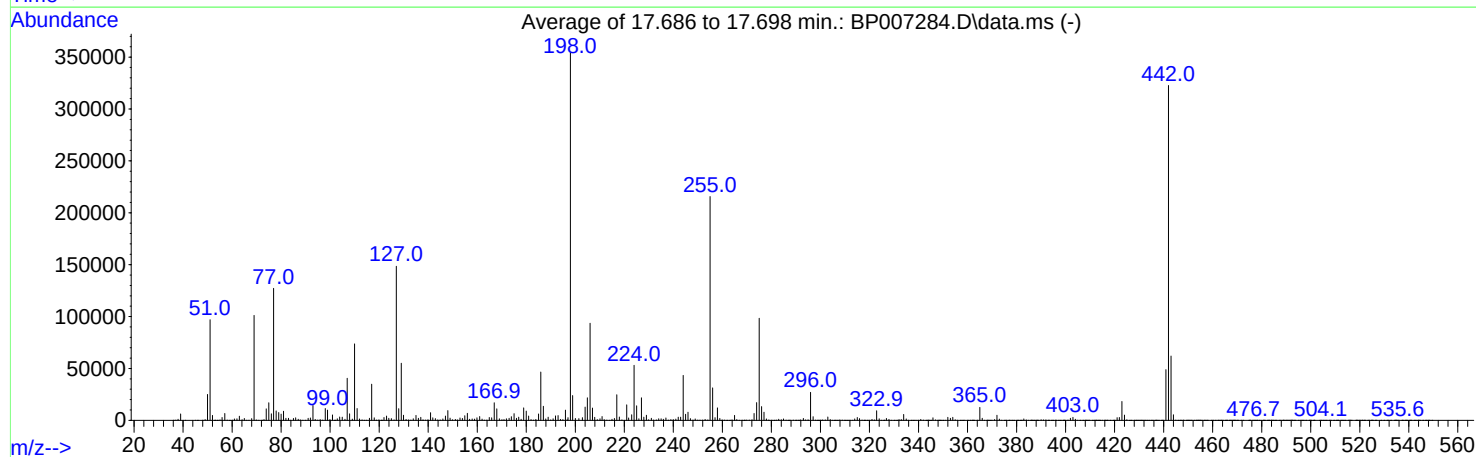


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100121\
 Data File : BP007284.D
 Acq On : 01 Oct 2021 10:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 01 12:49:05 2021

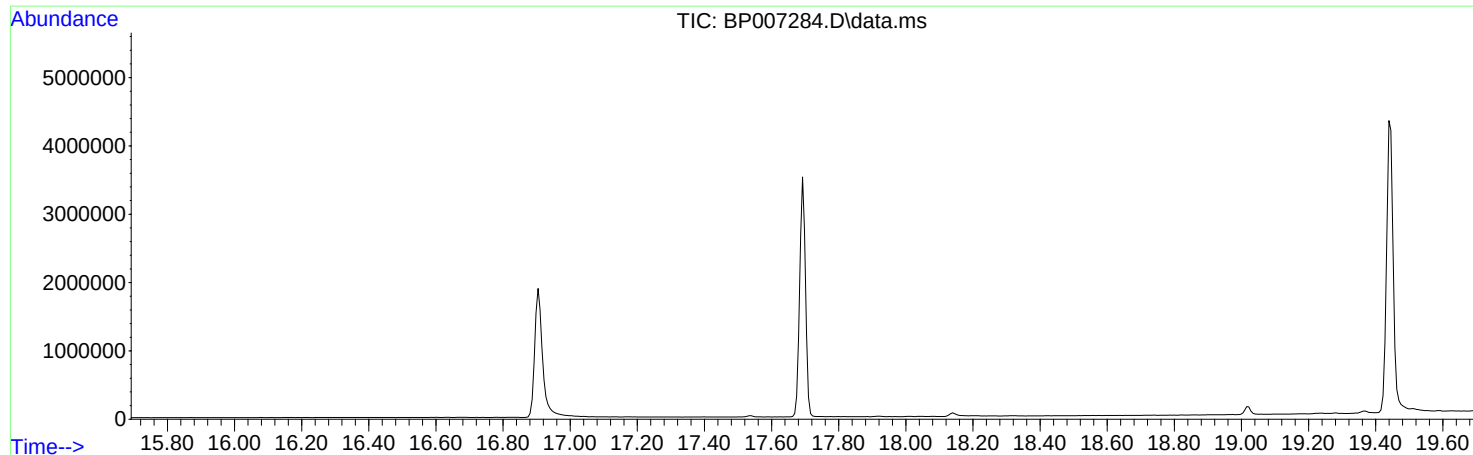




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.3	96915	PASS
68	69	0.00	2	1.7	1696	PASS
69	198	0.00	100	28.5	101066	PASS
70	69	0.00	2	0.5	516	PASS
127	198	10	80	41.9	148528	PASS
197	198	0.00	2	0.7	2618	PASS
198	198	100	100	100.0	354411	PASS
199	198	5	9	6.7	23845	PASS
275	198	10	60	27.8	98381	PASS
365	198	1	100	3.5	12570	PASS
441	198	0.01	100	13.8	48905	PASS
442	442	100	100	100.0	322688	PASS
443	442	15	24	19.2	61955	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100121\
 Data File : BP007284.D
 Acq On : 01 Oct 2021 10:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Oct 01 12:42:35 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 29 14:45:49 2021
 Response via : Initial Calibration

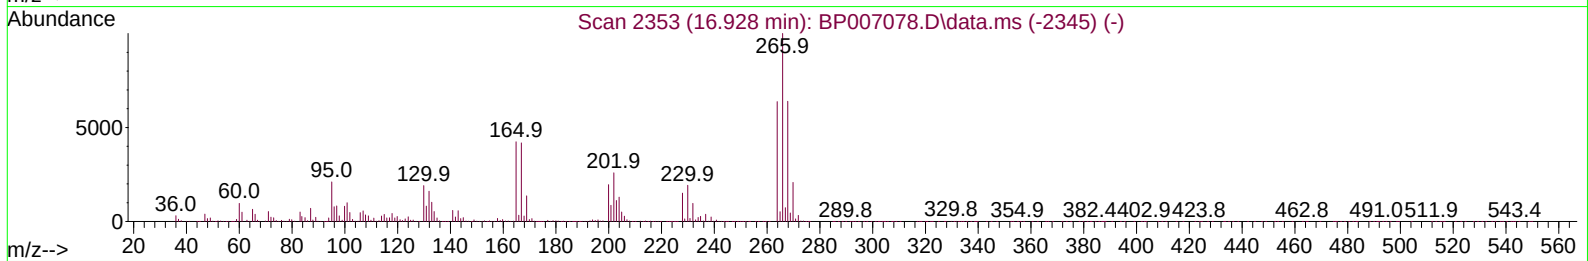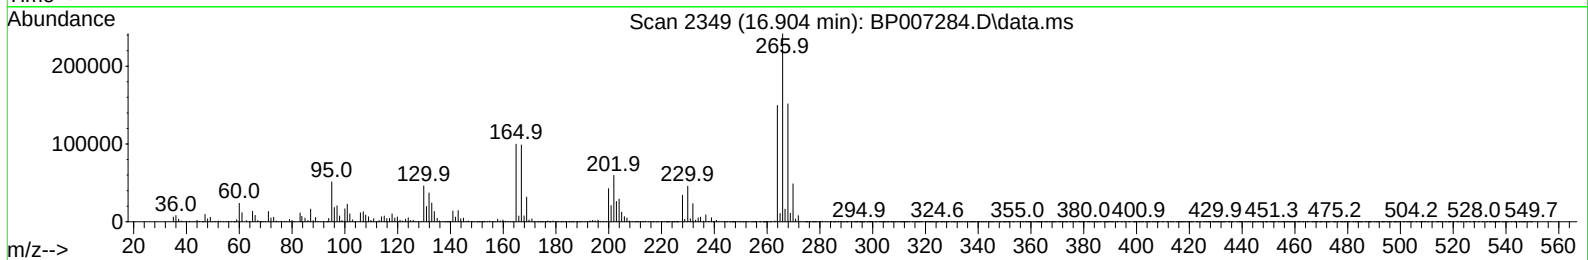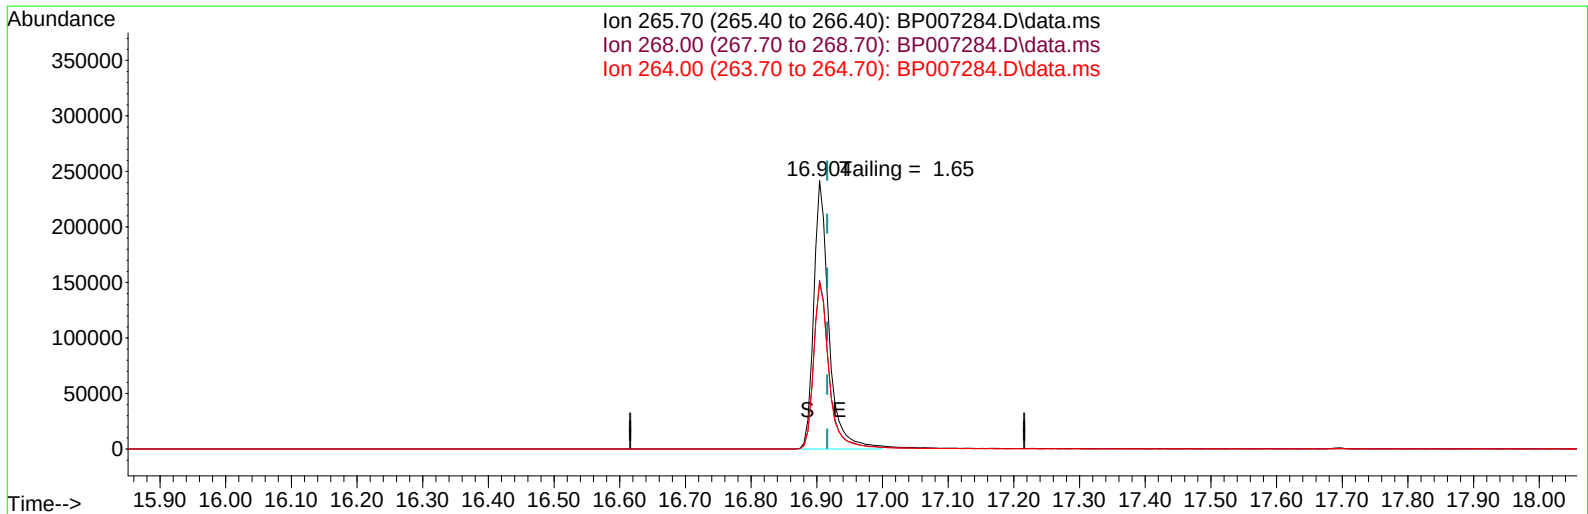

TIC: BP007284.D\data.ms

(70) Pentachlorophenol (C)

16.904min (-0.012) 4019333.10 ng




response 393052

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.72
264.00	62.90	61.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100121\
 Data File : BP007284.D
 Acq On : 01 Oct 2021 10:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Oct 01 12:42:35 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 29 14:45:49 2021
 Response via : Initial Calibration

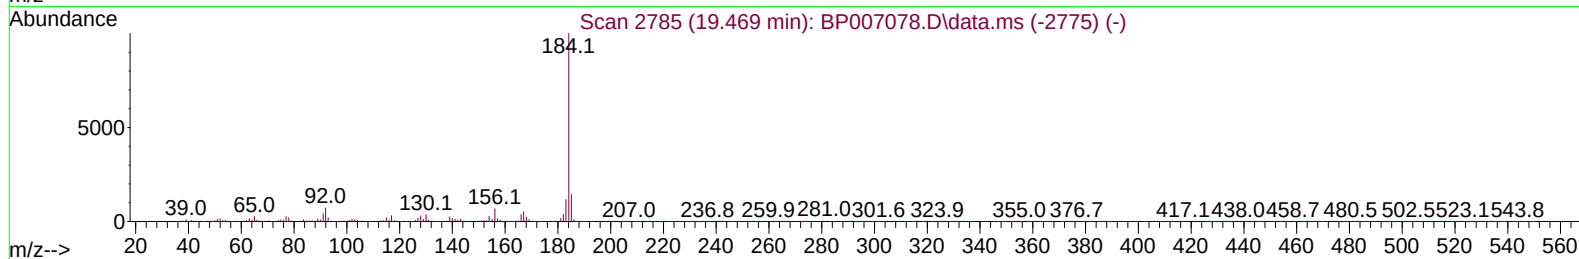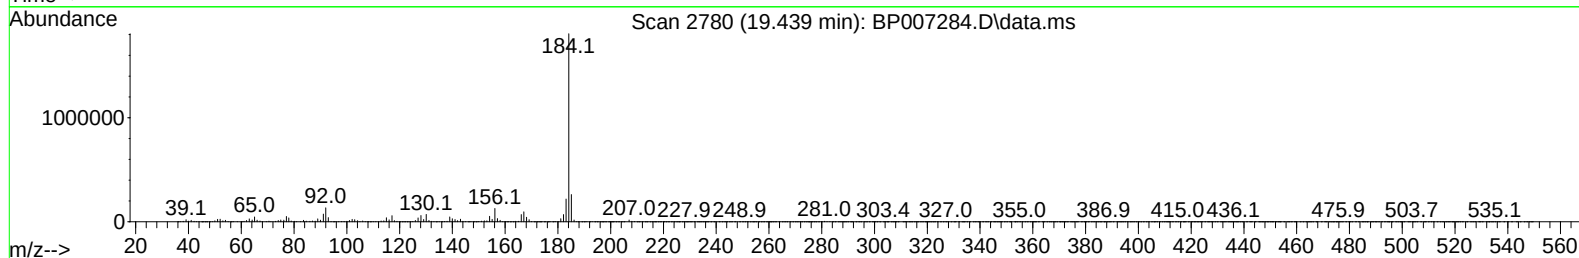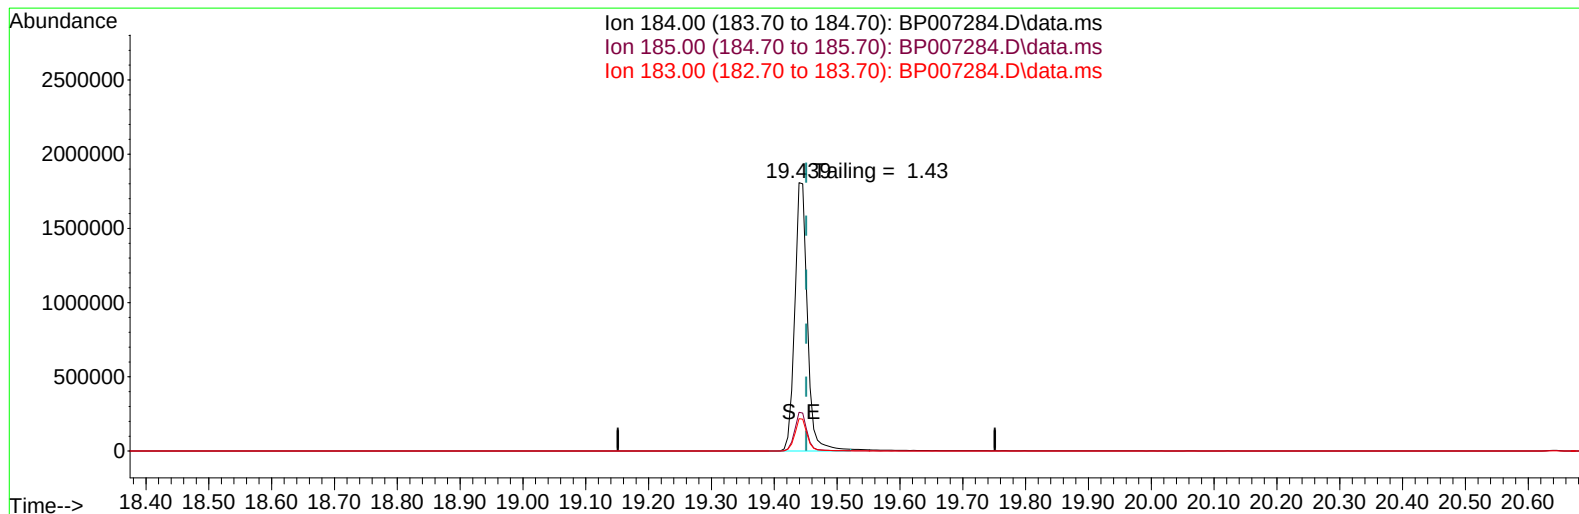

TIC: BP007284.D\data.ms

(77) Benzidine

19.439min (-0.012) 317549.46 ng

response 2576321

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.47
183.00	11.90	12.07
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/1/2021	BNA_P	BP007284.D
Compound Name	Response	Retention Time
DDT	1341105	20.63
DDD	11117	20.21
DDE	2399	19.72
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13516	1354621	1.00