

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100122\
 Data File : BP011859.D
 Acq On : 01 Oct 2022 13:35
 Operator : CG/JU
 Sample : N4824-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8M8

Quant Time: Oct 03 00:59:17 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 01 00:53:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	317707	20.000	ng/u1	0.00
20) Naphthalene-d8	10.704	136	1420211	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.545	164	898947	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.298	188	1838081	20.000	ng/u1	0.00
79) Chrysene-d12	21.386	240	1683477	20.000	ng/u1	0.00
88) Perylene-d12	23.821	264	1416448	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	37149	5.157	ng/uL	0.00
4) Pyridine-d5	3.734	84	241285	11.435	ng/u1	0.00
7) Phenol-d5	7.057	99	335072	12.217	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	455838	29.983	ng/u1	0.00
11) 2-Chlorophenol-d4	7.422	132	622232	28.738	ng/u1	0.00
15) 4-Methylphenol-d8	8.604	113	593408	26.172	ng/u1	0.00
21) Nitrobenzene-d5	9.063	128	369664	34.173	ng/u1	0.00
24) 2-Nitrophenol-d4	9.787	143	406207	35.098	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	752989	35.175	ng/u1	0.00
31) 4-Chloroaniline-d4	10.845	131	859962	26.350	ng/u1	0.00
46) Dimethylphthalate-d6	13.957	166	2403613	37.390	ng/u1	0.00
49) Acenaphthylene-d8	14.234	160	2761373	37.680	ng/u1	0.00
54) 4-Nitrophenol-d4	14.757	143	123645	9.288	ng/u1	0.02
60) Fluorene-d10	15.539	176	2061208	36.921	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.657	200	360214	32.378	ng/u1	0.00
73) Anthracene-d10	17.398	188	3166480	37.818	ng/u1	0.00
81) Pyrene-d10	19.633	212	3538404	41.502	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.668	264	2727974	38.473	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.340	88	16087	2.068	ng/uL#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100122\
Data File : BP011859.D
Acq On : 01 Oct 2022 13:35
Operator : CG/JU
Sample : N4824-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8M8

Quant Time: Oct 03 00:59:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 01 00:53:59 2022
Response via : Initial Calibration

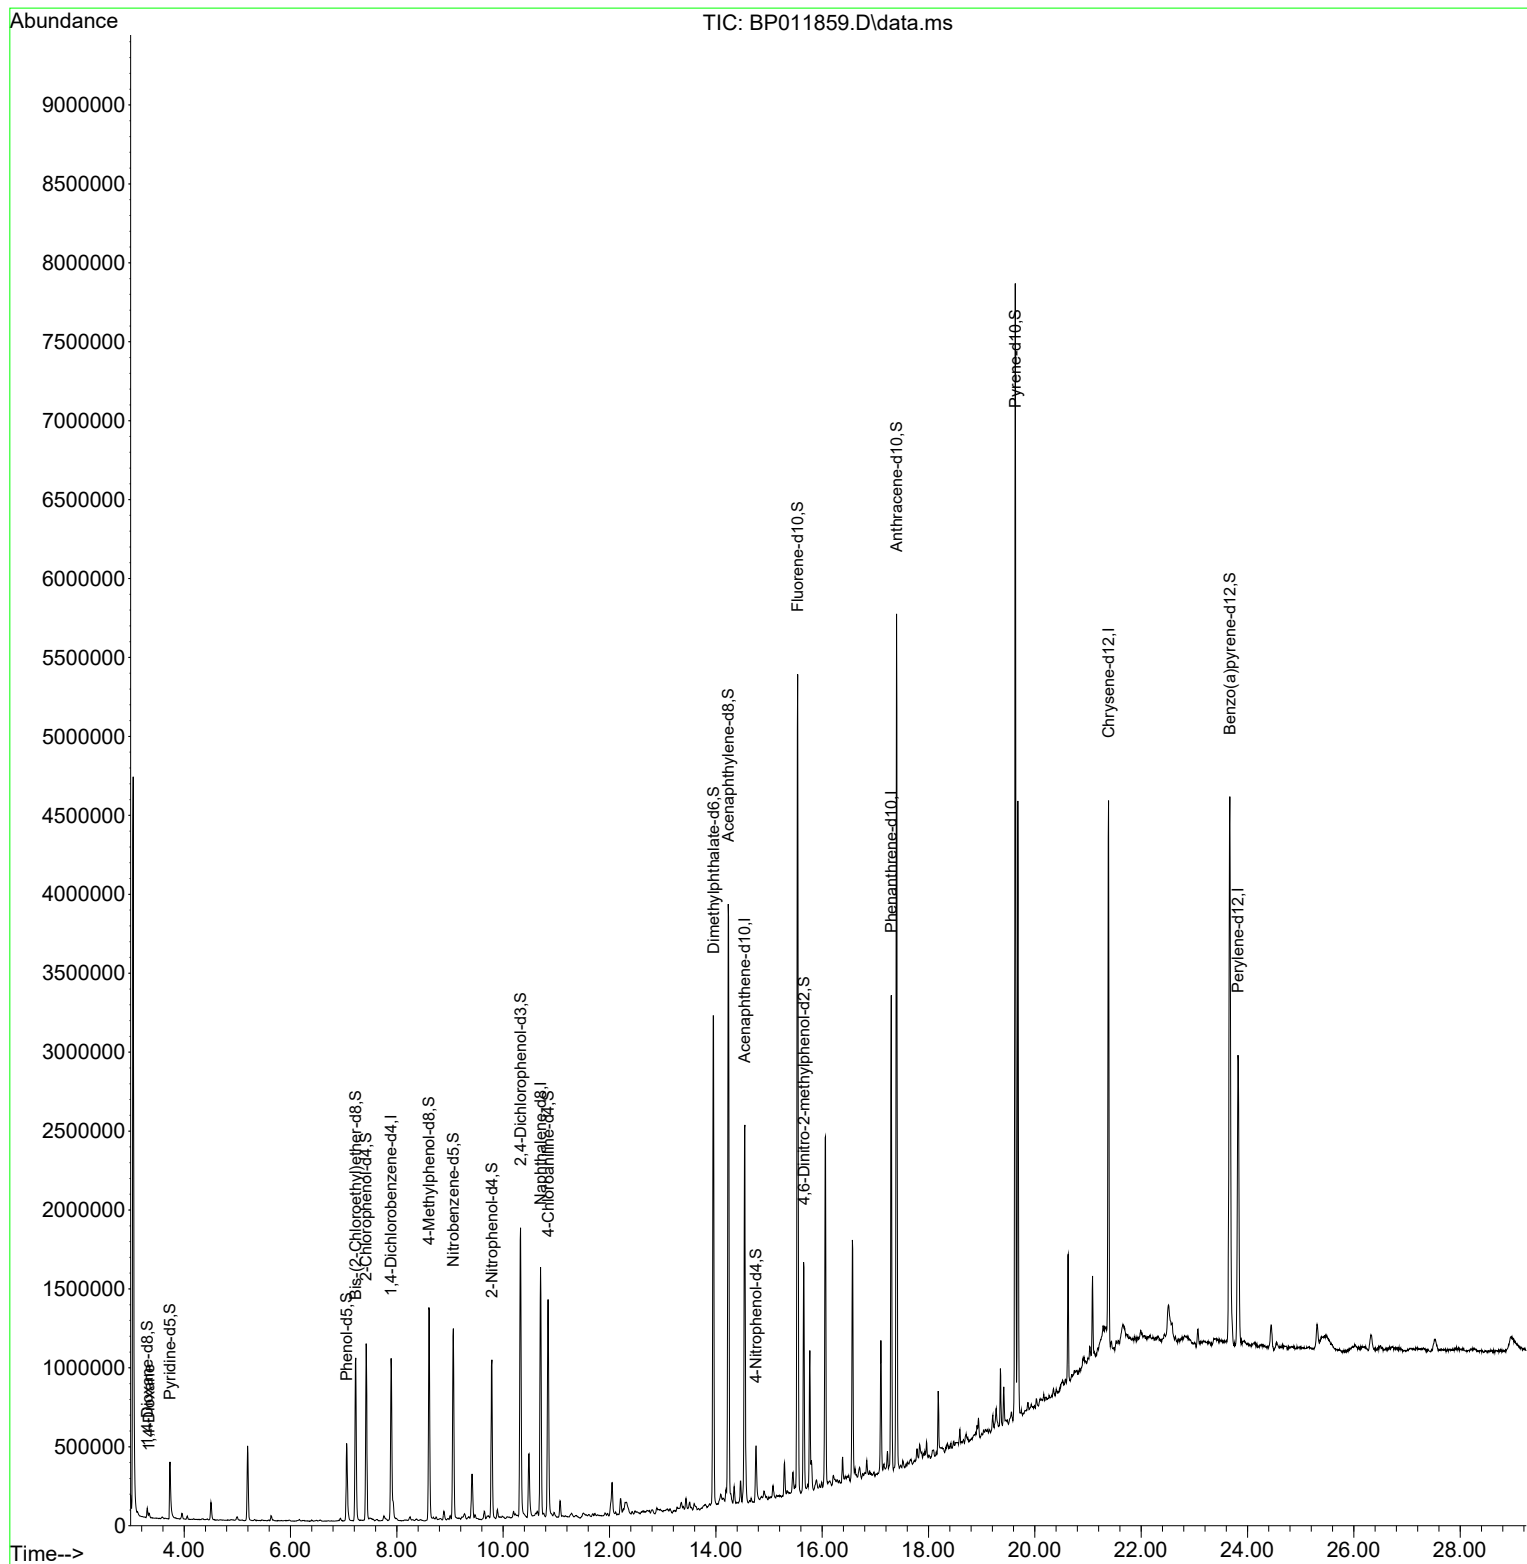

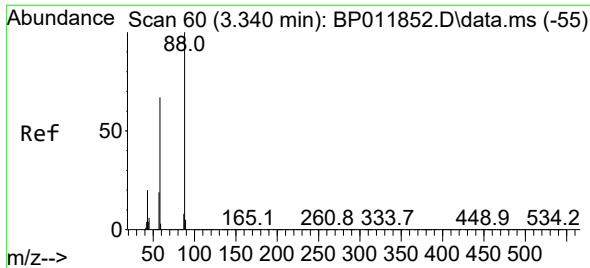

#2
 1,4-Dioxane
 Concen: 2.068 ng/uL
 RT: 3.340 min Scan# 60
 Delta R.T. 0.000 min
 Lab File: BP011859.D
 Acq: 01 Oct 2022 13:35

Instrument :
 BNA_P
 ClientSampleId :
 CB8M8

Tgt Ion: 88 Resp: 16087
 Ion Ratio Lower Upper
 88 100
 43 27.7 15.6 23.4#
 58 67.8 48.6 72.8

