

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100122\
 Data File : BP011857.D
 Acq On : 01 Oct 2022 12:26
 Operator : CG/JU
 Sample : N4824-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8N0

Quant Time: Oct 03 00:58:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 01 00:53:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	288233	20.000	ng/u1	0.00
20) Naphthalene-d8	10.704	136	1330817	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.539	164	841533	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.298	188	1774619	20.000	ng/u1	0.00
79) Chrysene-d12	21.386	240	1475794	20.000	ng/u1	0.00
88) Perylene-d12	23.827	264	1240632	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	30998	4.743	ng/uL	0.00
4) Pyridine-d5	3.734	84	253366	13.235	ng/u1	0.00
7) Phenol-d5	7.057	99	362522	14.569	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	421511	30.561	ng/u1	0.00
11) 2-Chlorophenol-d4	7.422	132	602607	30.678	ng/u1	0.00
15) 4-Methylphenol-d8	8.604	113	599310	29.136	ng/u1	0.00
21) Nitrobenzene-d5	9.063	128	357425	35.261	ng/u1	0.00
24) 2-Nitrophenol-d4	9.787	143	406625	37.494	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	731496	36.466	ng/u1	0.00
31) 4-Chloroaniline-d4	10.845	131	707083	23.121	ng/u1	0.00
46) Dimethylphthalate-d6	13.951	166	2328254	38.689	ng/u1	0.00
49) Acenaphthylene-d8	14.234	160	2657471	38.737	ng/u1	0.00
54) 4-Nitrophenol-d4	14.751	143	122915	9.863	ng/u1	0.01
60) Fluorene-d10	15.539	176	1977251	37.834	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	380631	35.436	ng/u1	0.00
73) Anthracene-d10	17.398	188	3053434	37.772	ng/u1	0.00
81) Pyrene-d10	19.633	212	3277932	43.857	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.668	264	2447187	39.404	ng/u1	0.00


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.346	88	19883	2.817	ng/uL#	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100122\
Data File : BP011857.D
Acq On : 01 Oct 2022 12:26
Operator : CG/JU
Sample : N4824-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8N0


Quant Time: Oct 03 00:58:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 01 00:53:59 2022
Response via : Initial Calibration

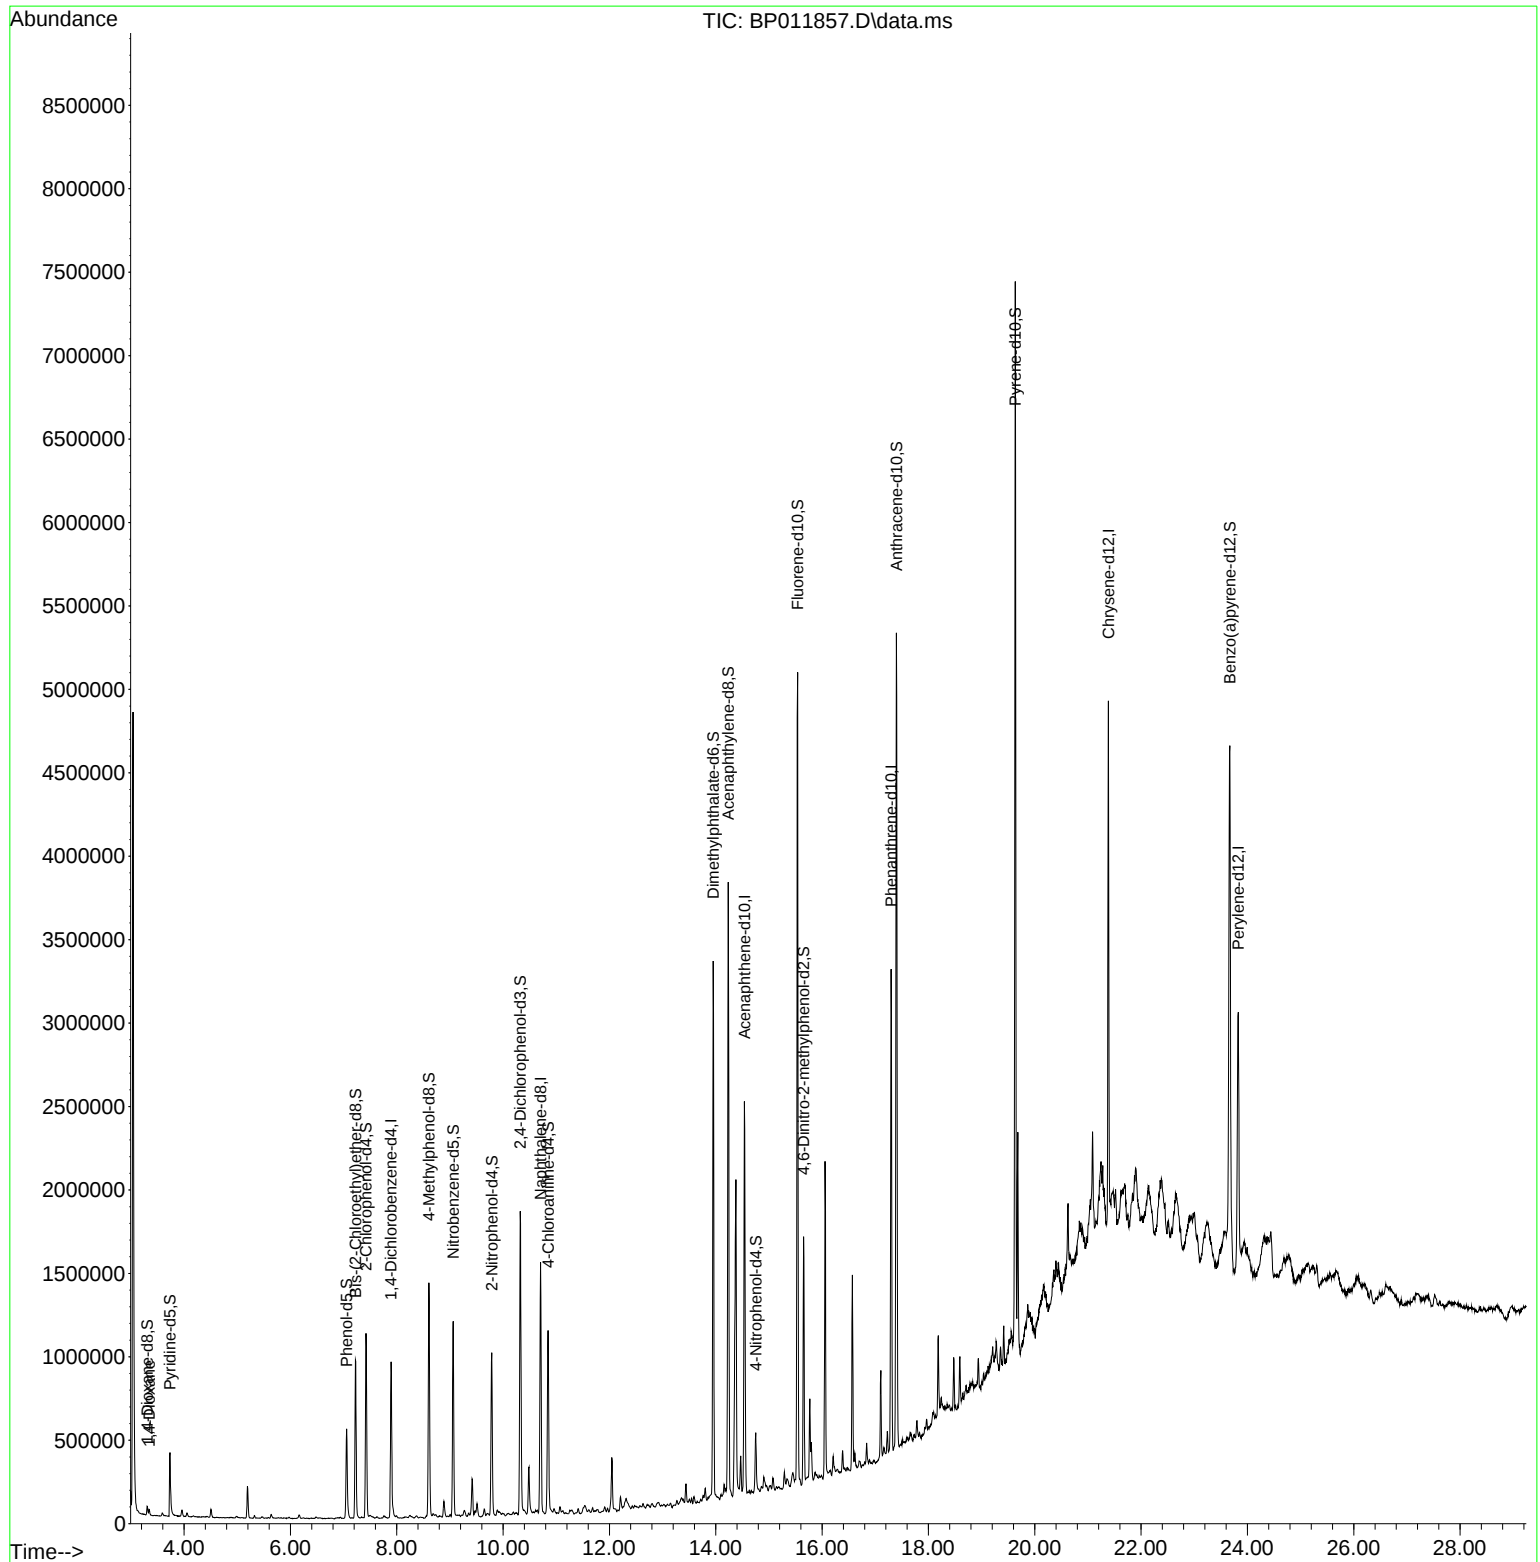

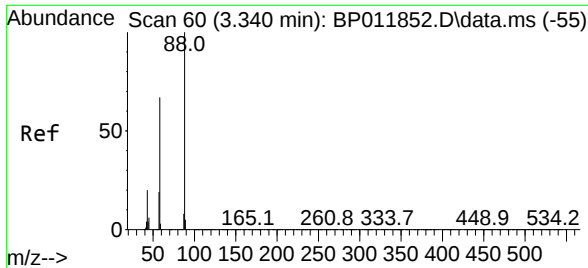

#2
 1,4-Dioxane
 Concen: 2.817 ng/uL
 RT: 3.346 min Scan# 61
 Delta R.T. 0.006 min
 Lab File: BP011857.D
 Acq: 01 Oct 2022 12:26

Instrument :
 BNA_P
 ClientSampleId :
 CB8N0

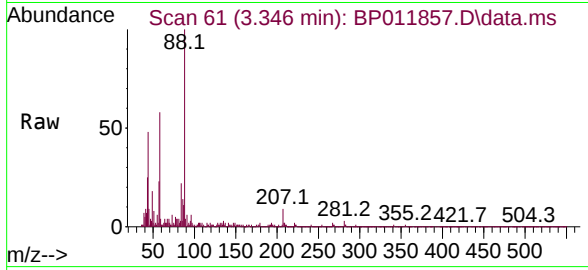

Tgt Ion: 88 Resp: 19883
 Ion Ratio Lower Upper
 88 100
 43 25.0 15.6 23.4#
 58 58.2 48.6 72.8

