

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100122\
 Data File : BP011860.D
 Acq On : 01 Oct 2022 14:09
 Operator : CG/JU
 Sample : N4824-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8N2

Quant Time: Oct 03 00:59:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 01 00:53:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	323210	20.000	ng/u1	0.00
20) Naphthalene-d8	10.705	136	1477565	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.540	164	940359	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.298	188	1979012	20.000	ng/u1	0.00
79) Chrysene-d12	21.386	240	1802412	20.000	ng/u1	0.00
88) Perylene-d12	23.821	264	1458419	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	30561	4.170	ng/uL	0.00
4) Pyridine-d5	3.734	84	99592	4.639	ng/u1	0.00
7) Phenol-d5	7.058	99	326380	11.697	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	474879	30.704	ng/u1	0.00
11) 2-Chlorophenol-d4	7.422	132	617545	28.036	ng/u1	0.00
15) 4-Methylphenol-d8	8.605	113	578881	25.097	ng/u1	0.00
21) Nitrobenzene-d5	9.063	128	375008	33.321	ng/u1	0.00
24) 2-Nitrophenol-d4	9.787	143	414121	34.393	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	745762	33.485	ng/u1	0.00
31) 4-Chloroaniline-d4	10.846	131	676513	19.925	ng/u1	0.00
46) Dimethylphthalate-d6	13.951	166	2499346	37.167	ng/u1	0.00
49) Acenaphthylene-d8	14.234	160	2807708	36.625	ng/u1	0.00
54) 4-Nitrophenol-d4	14.746	143	129393	9.292	ng/u1	0.00
60) Fluorene-d10	15.540	176	2165029	37.073	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.657	200	399679	33.367	ng/u1	0.00
73) Anthracene-d10	17.398	188	3448547	38.254	ng/u1	0.00
81) Pyrene-d10	19.633	212	3856145	42.244	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.669	264	2914079	39.915	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.340	88	33746	4.263	ng/uL	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100122\
Data File : BP011860.D
Acq On : 01 Oct 2022 14:09
Operator : CG/JU
Sample : N4824-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8N2


Quant Time: Oct 03 00:59:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 01 00:53:59 2022
Response via : Initial Calibration

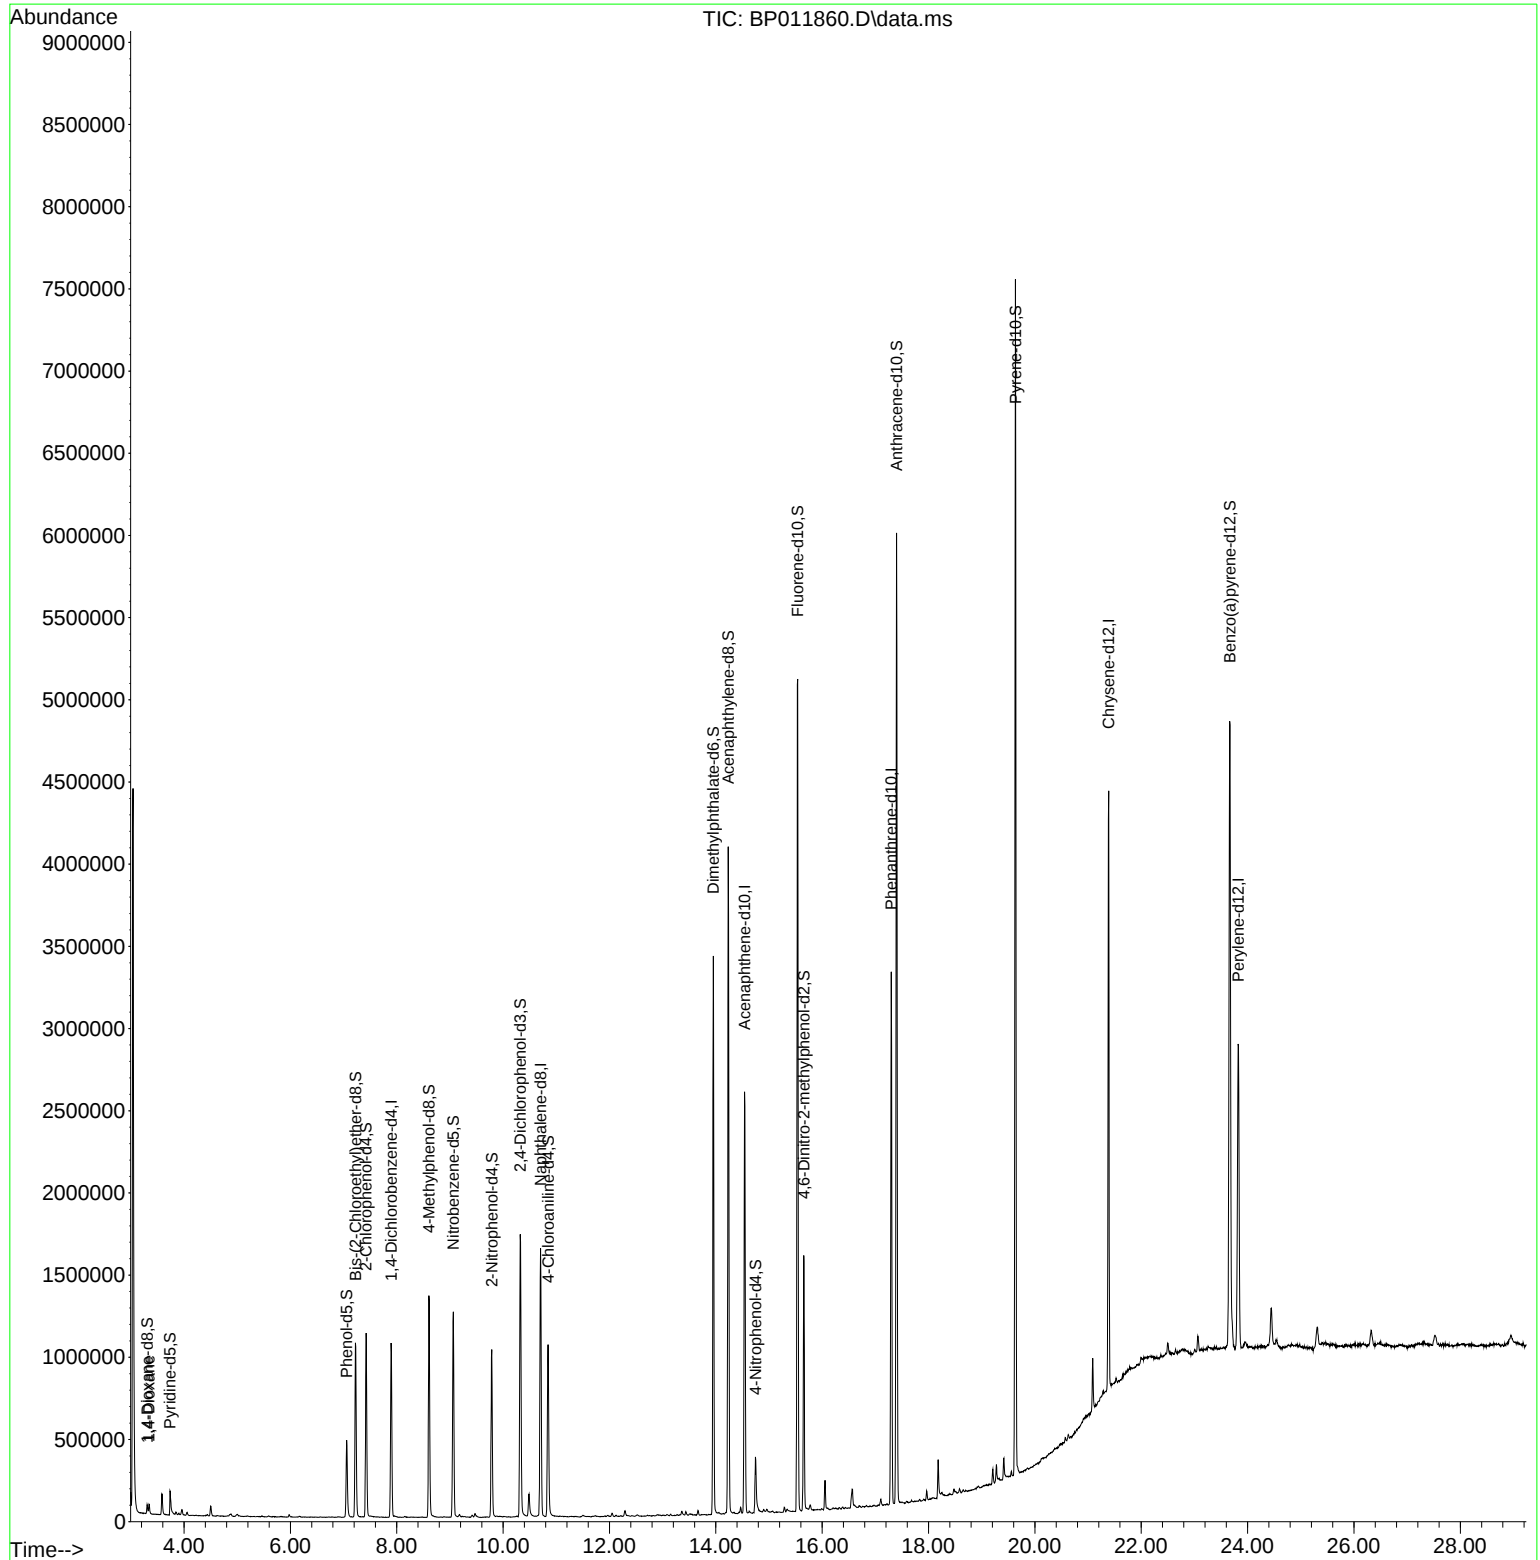

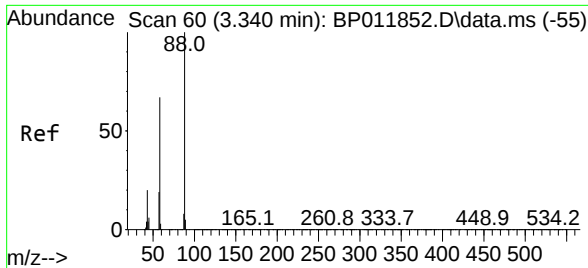

#2
 1,4-Dioxane
 Concen: 4.263 ng/uL
 RT: 3.340 min Scan# 60
 Delta R.T. 0.000 min
 Lab File: BP011860.D
 Acq: 01 Oct 2022 14:09

Instrument :
 BNA_P
 ClientSampleId :
 CB8N2

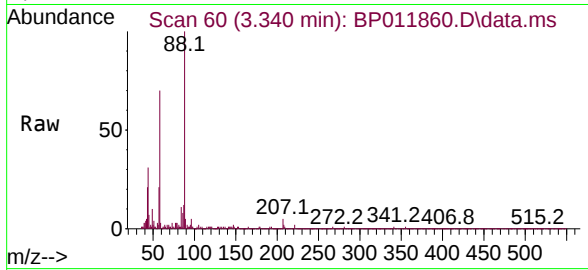

Tgt Ion:	88	Resp:	33746
Ion	Ratio	Lower	Upper
88	100		
43	21.1	15.6	23.4
58	69.7	48.6	72.8

