
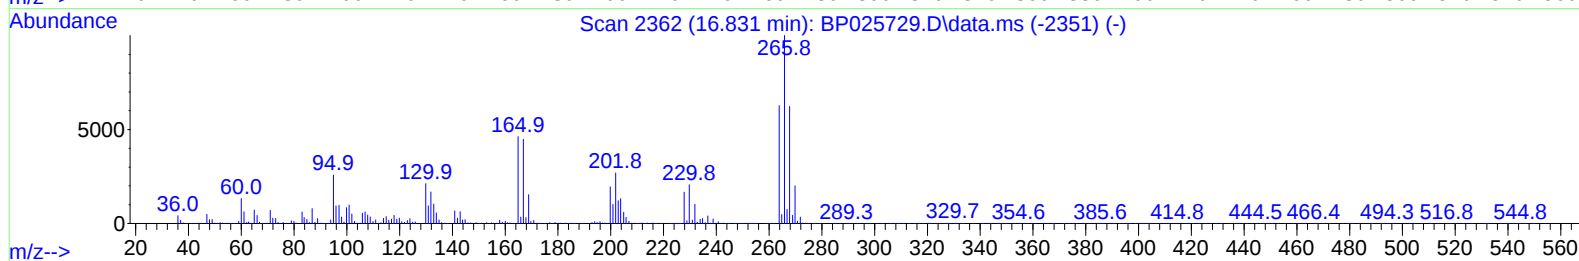
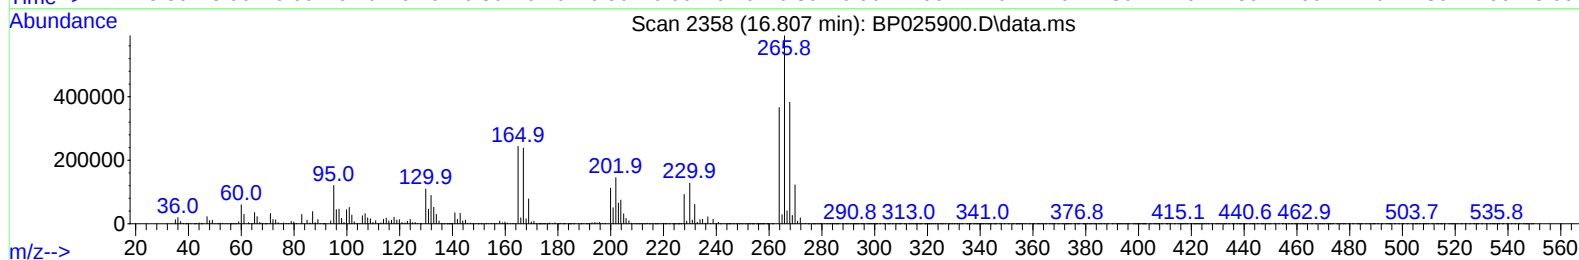


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100125\
Data File : BP025900.D
Acq On : 01 Oct 2025 14:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 01 14:49:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

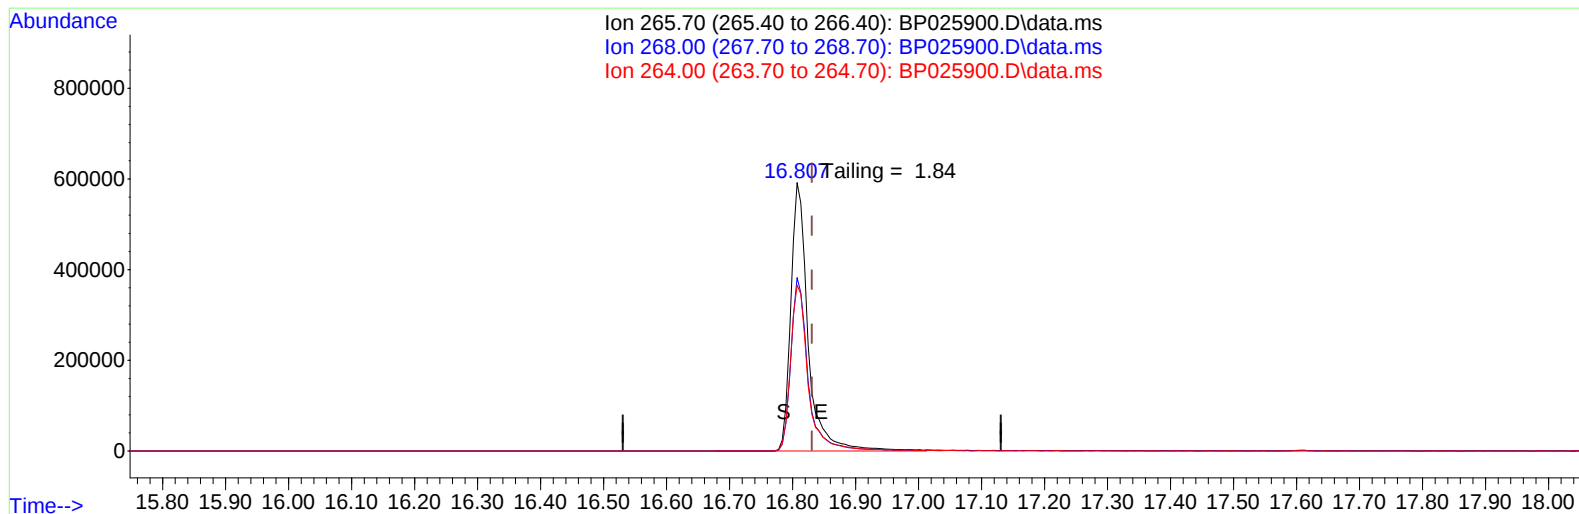

TIC: BP025900.D\data.ms

(70) Pentachlorophenol (C)




16.807min (-0.024) 6411668.82 ng

response 1140541

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.61
264.00	62.70	61.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100125\
Data File : BP025900.D
Acq On : 01 Oct 2025 14:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 01 14:49:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP091225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 16:45:04 2025
Response via : Initial Calibration

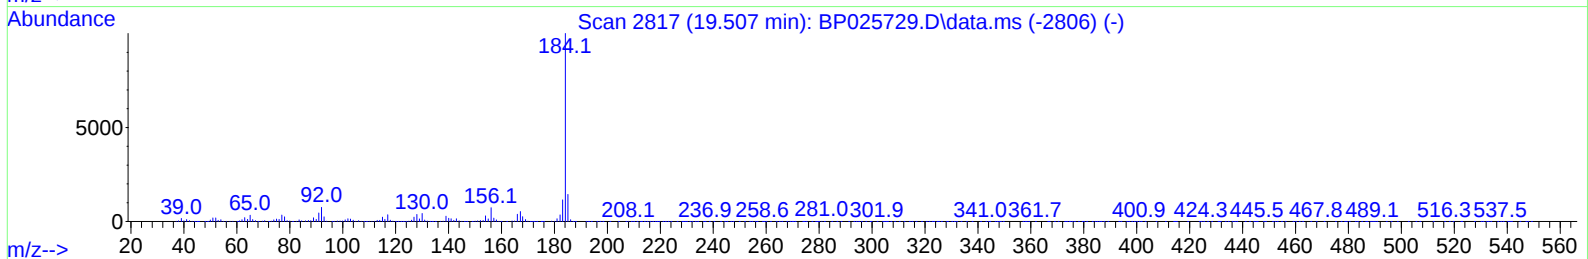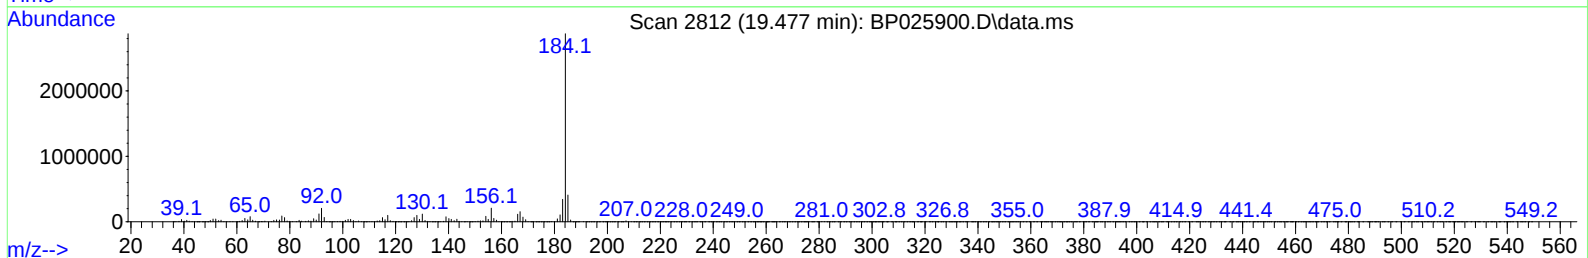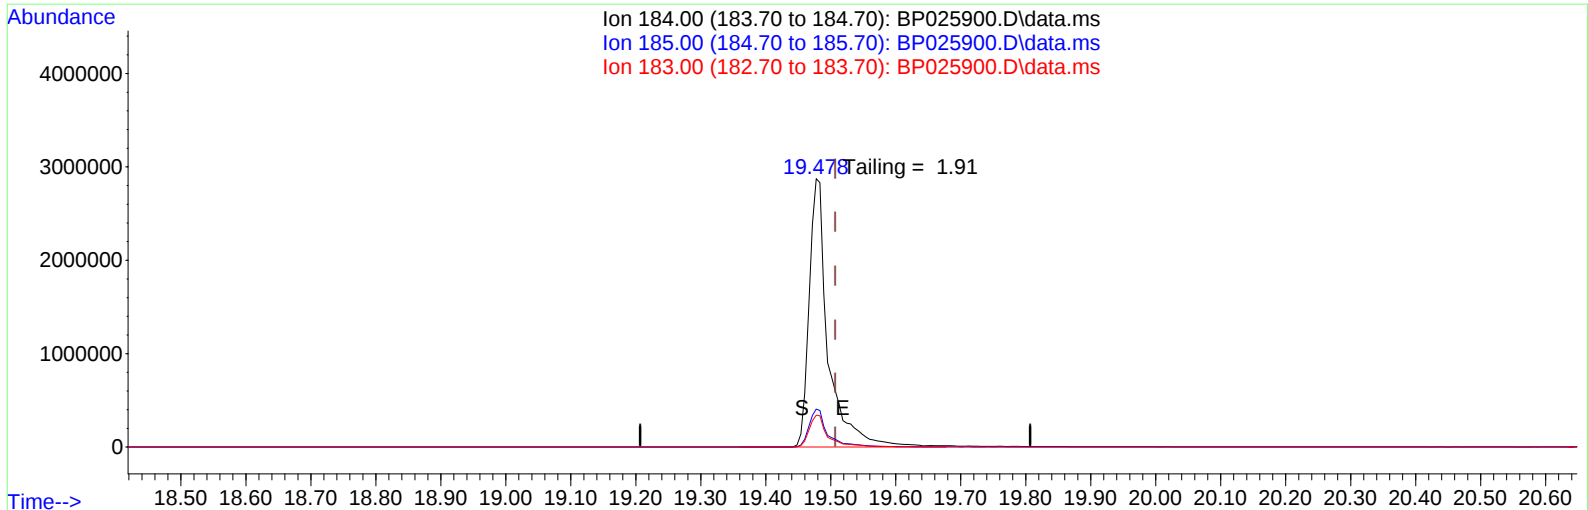

TIC: BP025900.D\data.ms

(77) Benzidine**19.477min (-0.029) 106666.91 ng****response 5893204**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.17
183.00	11.50	11.89
0.00	0.00	0.00