

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
 Data File : BP017484.D
 Acq On : 02 Oct 2023 19:07
 Operator : MA/JU
 Sample : 04571-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBK87

Quant Time: Oct 02 23:15:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 30 04:02:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	113151	20.000	ng/ul	0.00
20) Naphthalene-d8	10.787	136	451367	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.640	164	263943	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.428	188	569455	20.000	ng/ul	0.00
79) Chrysene-d12	21.557	240	540163	20.000	ng/ul	0.00
88) Perylene-d12	24.127	264	602338	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	15328	5.564	ng/uL	0.00
4) Pyridine-d5	3.734	84	121220	15.740	ng/ul	0.00
7) Phenol-d5	7.099	99	87162	9.379	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	254137	45.314	ng/ul	0.00
11) 2-Chlorophenol-d4	7.463	132	257392	34.921	ng/ul	0.00
15) 4-Methylphenol-d8	8.669	113	158139	21.888	ng/ul	0.00
21) Nitrobenzene-d5	9.157	128	162794	49.889	ng/ul	0.00
24) 2-Nitrophenol-d4	9.869	143	164394	46.398	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.399	165	282890	42.260	ng/ul	0.00
31) 4-Chloroaniline-d4	10.951	131	365785	37.722	ng/ul	0.00
46) Dimethylphthalate-d6	14.057	166	932557	49.321	ng/ul	0.00
49) Acenaphthylene-d8	14.340	160	1052546	48.400	ng/ul	0.00
54) 4-Nitrophenol-d4	14.881	143	15578	4.729	ng/ul	0.00
60) Fluorene-d10	15.645	176	814339	50.027	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.781	200	111751	34.818	ng/ul	0.00
73) Anthracene-d10	17.528	188	1377971	54.561	ng/ul	0.00
81) Pyrene-d10	19.780	212	1671296	57.215	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.963	264	1582794	54.578	ng/ul	0.00
Target Compounds						
					Qvalue	
34) Caprolactam	11.793	113	27472	14.406	ng/ul	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017484.D
Acq On : 02 Oct 2023 19:07
Operator : MA/JU
Sample : 04571-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBK87

Quant Time: Oct 02 23:15:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 30 04:02:20 2023
Response via : Initial Calibration

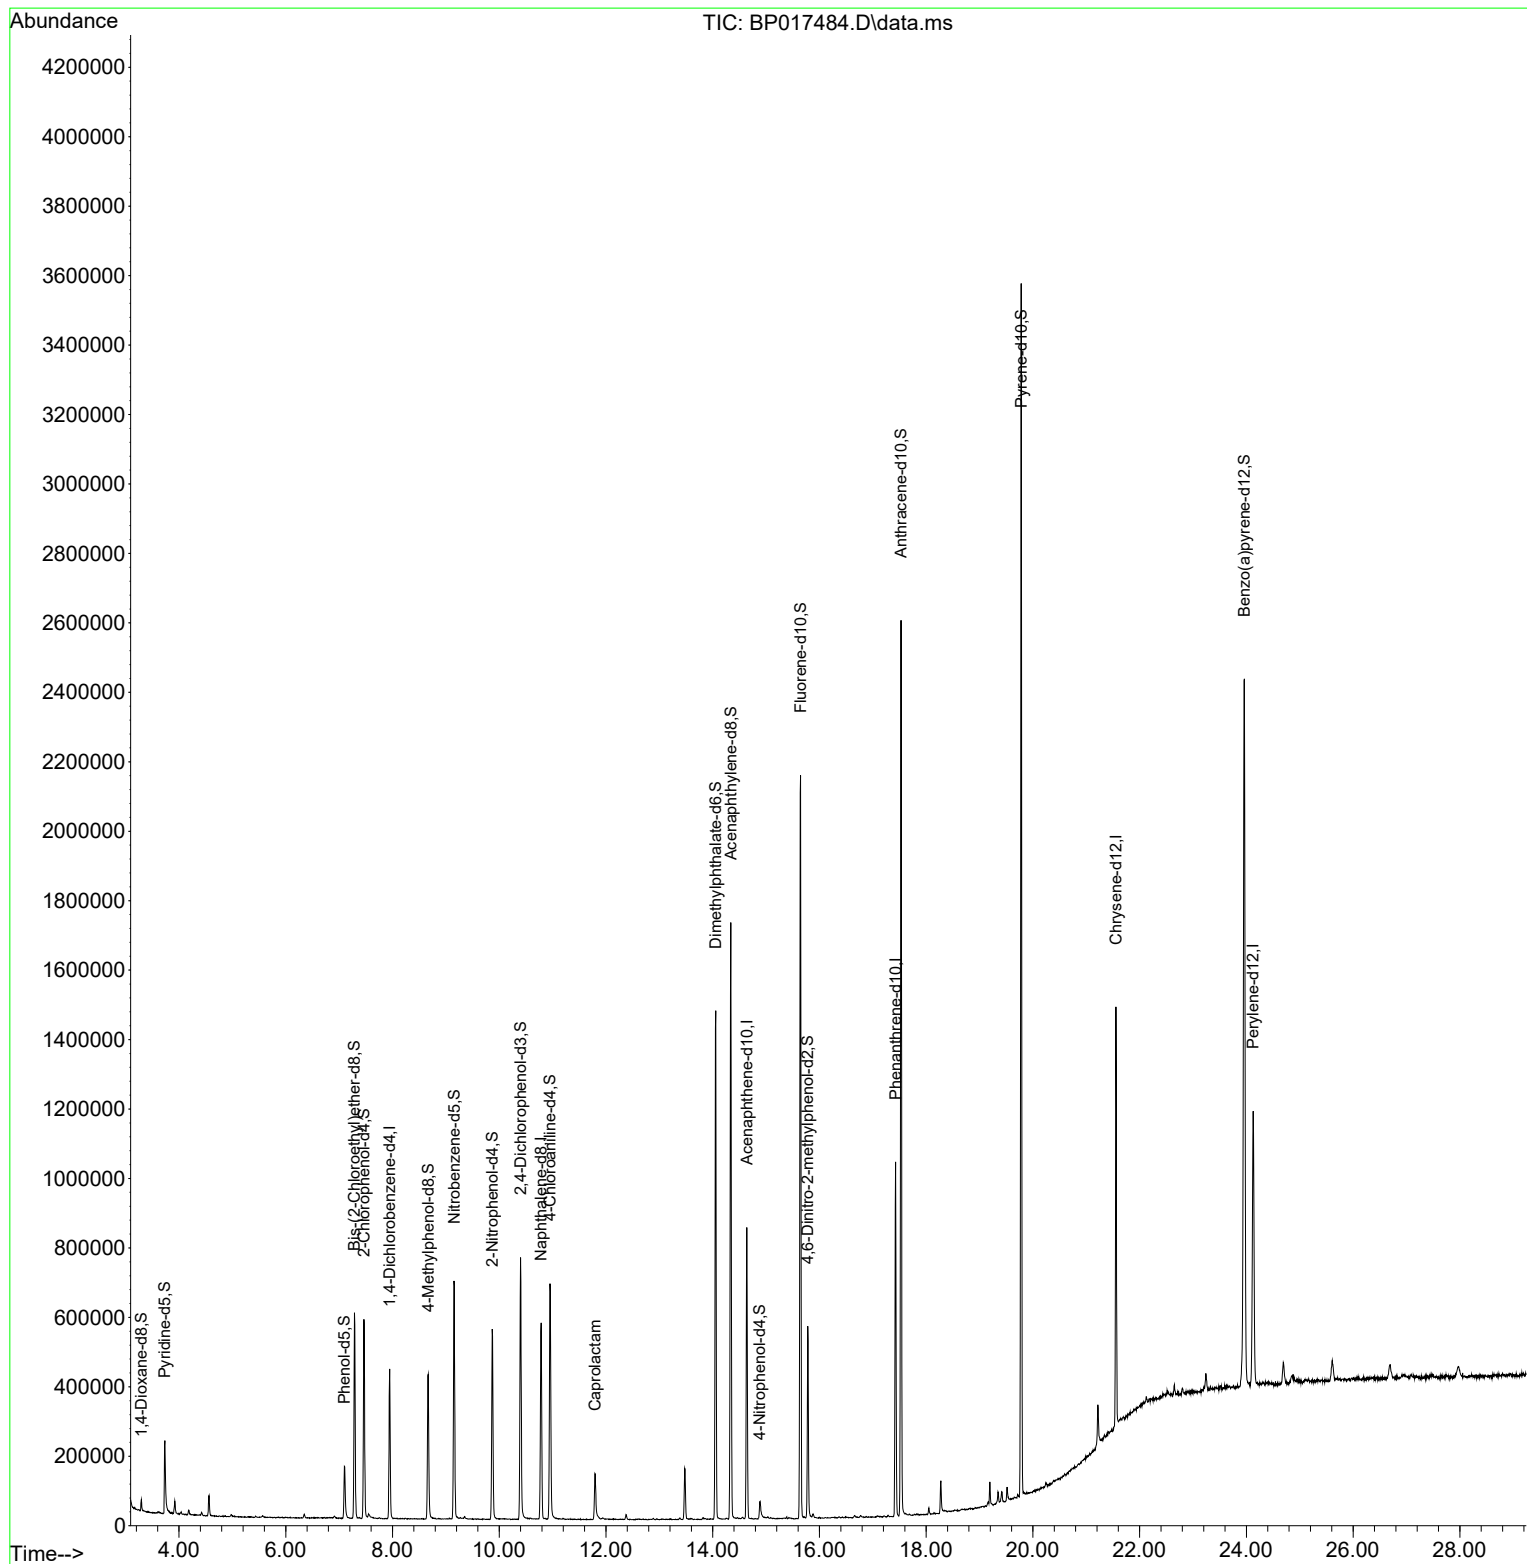

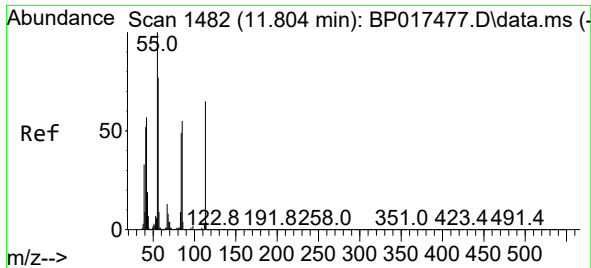

#34
 Caprolactam
 Concen: 14.406 ng/ul
 RT: 11.793 min Scan# 14
 Delta R.T. -0.018 min
 Lab File: BP017484.D
 Acq: 02 Oct 2023 19:07

Instrument :
 BNA_P
 ClientSampleId :
 BBK87

Tgt Ion:113 Resp: 27472
 Ion Ratio Lower Upper
 113 100
 55 143.0 127.4 191.0
 56 111.9 94.5 141.7

