

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
 Data File : BP017524.D
 Acq On : 03 Oct 2023 19:14
 Operator : MA/JU
 Sample : 04679-26
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PMW-7D(20230928)

Quant Time: Oct 03 23:29:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 03 22:59:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	97993	20.000	ng/ul	0.00
20) Naphthalene-d8	10.775	136	391837	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.628	164	230969	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.421	188	505494	20.000	ng/ul	0.00
79) Chrysene-d12	21.557	240	501198	20.000	ng/ul	0.00
88) Perylene-d12	24.139	264	555245	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	10415	4.366	ng/uL	0.00
4) Pyridine-d5	3.722	84	95426	14.308	ng/ul	0.00
7) Phenol-d5	7.093	99	66836	8.305	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	208952	43.021	ng/ul	0.00
11) 2-Chlorophenol-d4	7.457	132	212987	33.367	ng/ul	0.00
15) 4-Methylphenol-d8	8.657	113	133098	21.272	ng/ul	0.00
21) Nitrobenzene-d5	9.140	128	137256	48.453	ng/ul	0.00
24) 2-Nitrophenol-d4	9.857	143	142320	46.270	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.392	165	250753	43.150	ng/ul	0.00
31) 4-Chloroaniline-d4	10.945	131	271842	32.293	ng/ul	0.00
46) Dimethylphthalate-d6	14.045	166	884526	53.459	ng/ul	0.00
49) Acenaphthylene-d8	14.328	160	970452	50.996	ng/ul	0.00
54) 4-Nitrophenol-d4	14.898	143	17131	5.943	ng/ul	0.02
60) Fluorene-d10	15.633	176	766817	53.832	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.775	200	80196	28.148	ng/ul	0.00
73) Anthracene-d10	17.521	188	1283505	57.251	ng/ul	0.00
81) Pyrene-d10	19.774	212	1549712	57.178	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.968	264	1521546	56.916	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.316	88	28708	11.750	ng/uL#	96
32) 4-Chloroaniline	10.969	127	16991	2.106	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017524.D
Acq On : 03 Oct 2023 19:14
Operator : MA/JU
Sample : 04679-26
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PMW-7D(20230928)

Quant Time: Oct 03 23:29:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 03 22:59:42 2023
Response via : Initial Calibration




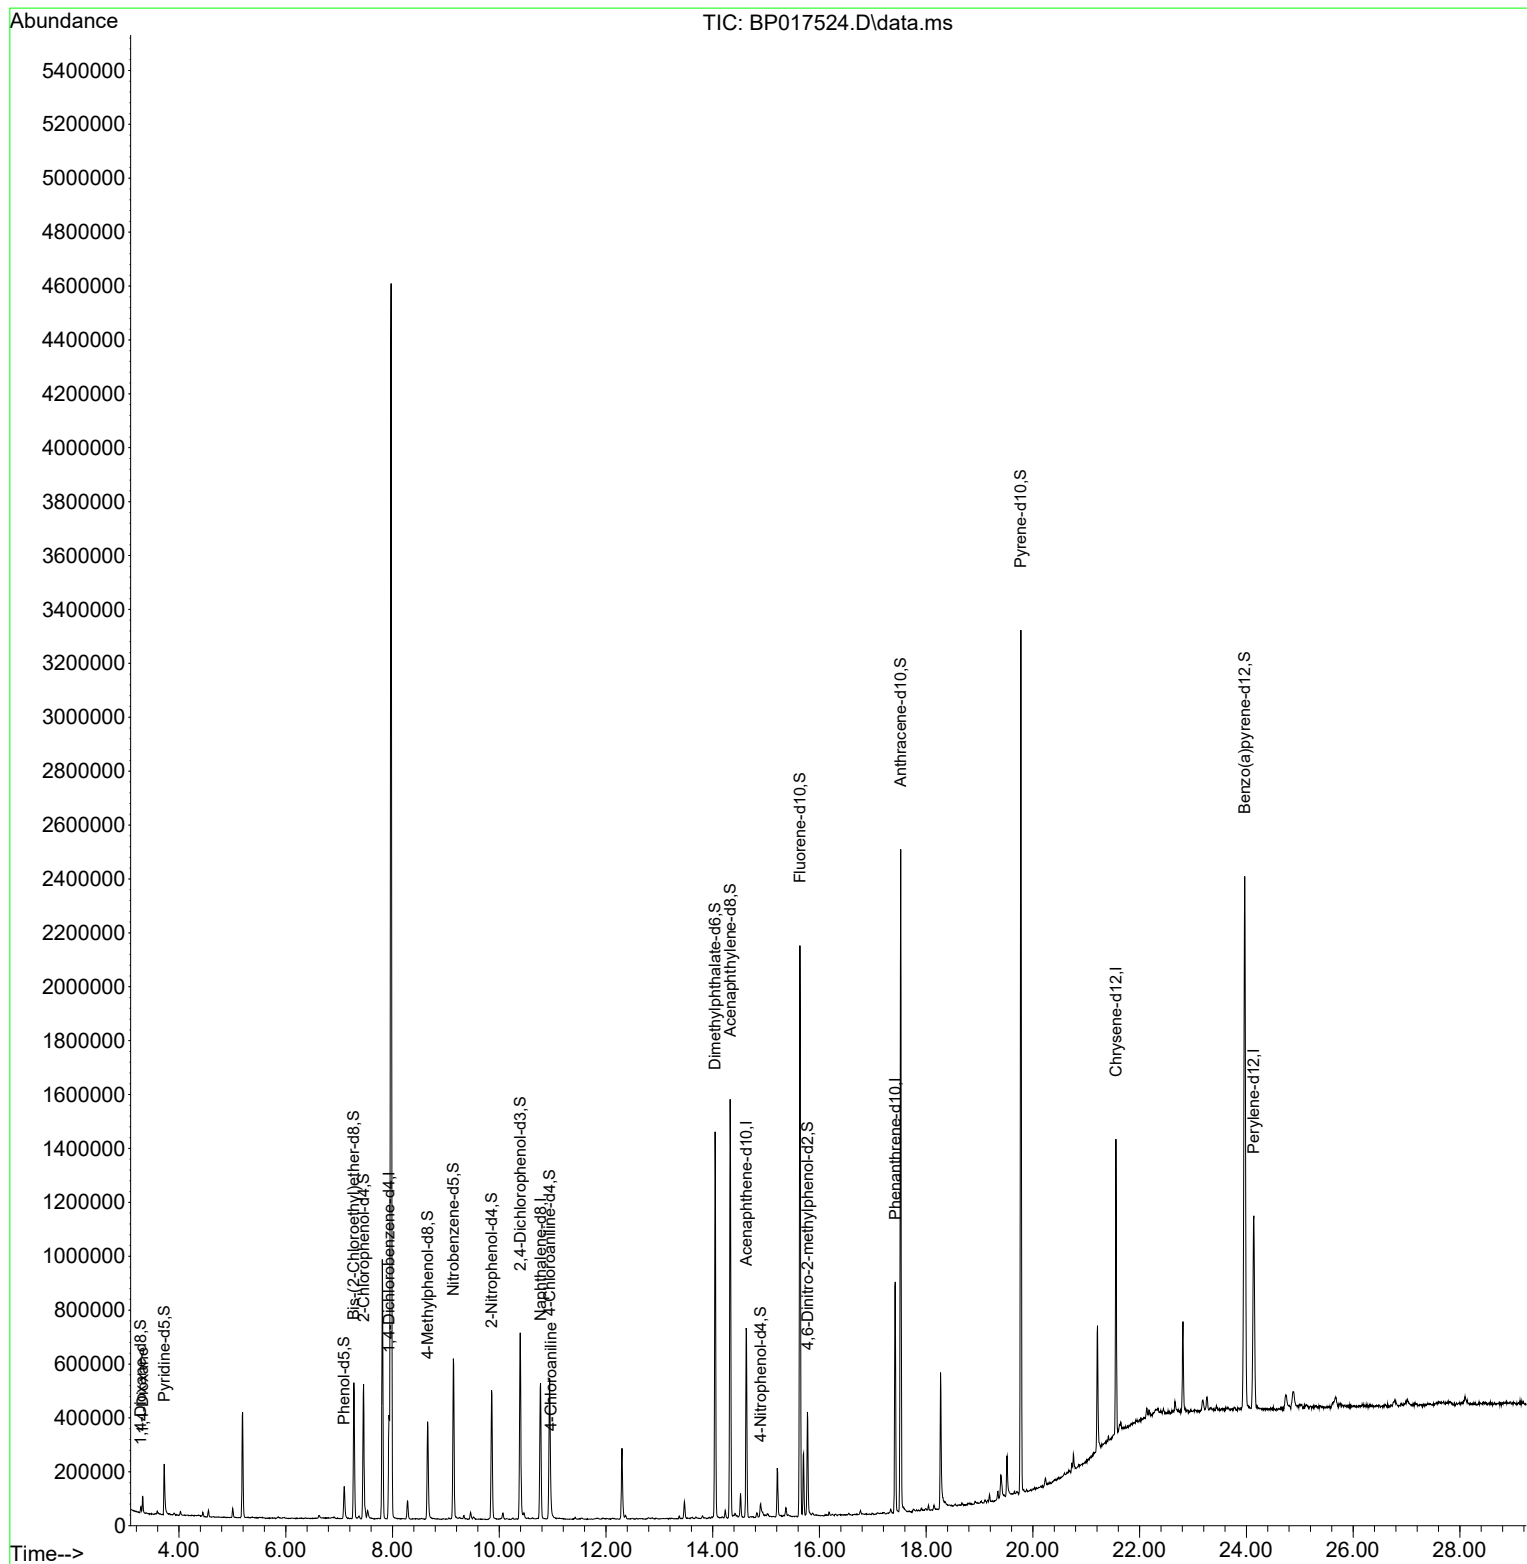


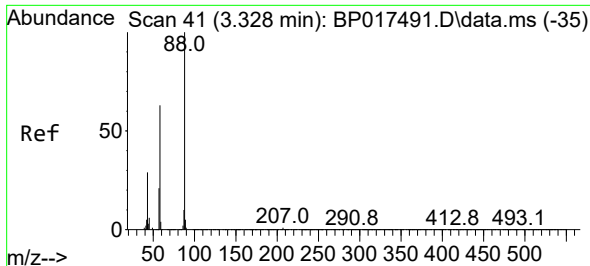

#2
1,4-Dioxane
Concen: 11.750 ng/uL
RT: 3.316 min Scan# 31
Delta R.T. -0.000 min
Lab File: BP017524.D
Acq: 03 Oct 2023 19:14

Instrument :
BNA_P
ClientSampleId :
PMW-7D(20230928)

Tgt Ion: 88 Resp: 28708
Ion Ratio Lower Upper
88 100
43 38.1 25.0 37.4#
58 71.4 56.6 84.8

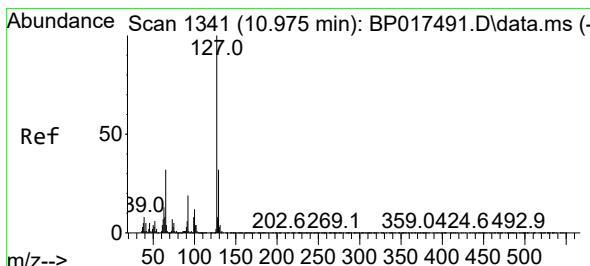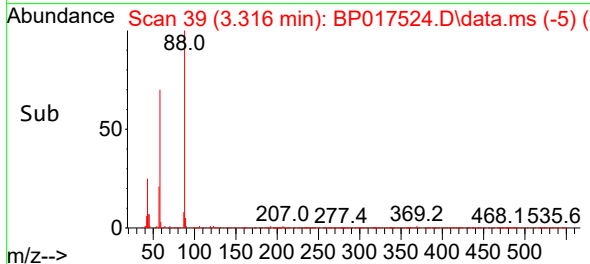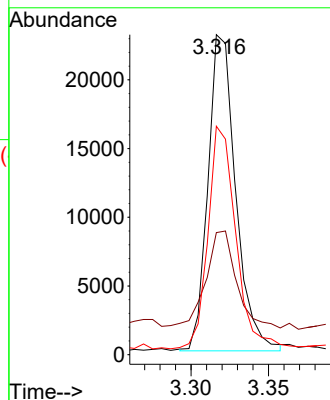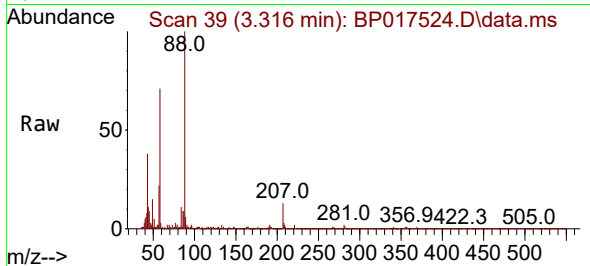

#32
4-Chloroaniline
Concen: 2.106 ng/uL
RT: 10.969 min Scan# 1340
Delta R.T. -0.000 min
Lab File: BP017524.D
Acq: 03 Oct 2023 19:14

Tgt Ion: 127 Resp: 16991
Ion Ratio Lower Upper
127 100
129 30.6 25.1 37.7

