

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
 Data File : BP017483.D
 Acq On : 02 Oct 2023 18:33
 Operator : MA/JU
 Sample : 04571-11
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBK62

Quant Time: Oct 02 23:15:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 30 04:02:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	120457	20.000	ng/u1	0.00
20) Naphthalene-d8	10.787	136	478987	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.640	164	272903	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.428	188	588921	20.000	ng/u1	0.00
79) Chrysene-d12	21.557	240	567607	20.000	ng/u1	0.00
88) Perylene-d12	24.127	264	637372	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	16480	5.619	ng/uL	0.00
4) Pyridine-d5	3.734	84	116084	14.159	ng/u1	0.00
7) Phenol-d5	7.099	99	105588	10.673	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	271948	45.549	ng/u1	0.00
11) 2-Chlorophenol-d4	7.464	132	287389	36.626	ng/u1	0.00
15) 4-Methylphenol-d8	8.664	113	186991	24.312	ng/u1	0.00
21) Nitrobenzene-d5	9.152	128	172338	49.769	ng/u1	0.00
24) 2-Nitrophenol-d4	9.869	143	178023	47.347	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.399	165	309074	43.509	ng/u1	0.00
31) 4-Chloroaniline-d4	10.952	131	329303	32.002	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	985325	50.400	ng/u1	0.00
49) Acenaphthylene-d8	14.340	160	1087477	48.365	ng/u1	0.00
54) 4-Nitrophenol-d4	14.887	143	18929	5.558	ng/u1	0.01
60) Fluorene-d10	15.646	176	843872	50.139	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.787	200	120996	36.452	ng/u1	0.00
73) Anthracene-d10	17.528	188	1335736	51.140	ng/u1	0.00
81) Pyrene-d10	19.781	212	1662736	54.170	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.957	264	1551041	50.543	ng/u1	0.00
Target Compounds						
					Qvalue	
34) Caprolactam	11.799	113	34027	16.814	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017483.D
Acq On : 02 Oct 2023 18:33
Operator : MA/JU
Sample : 04571-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBK62

Quant Time: Oct 02 23:15:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 30 04:02:20 2023
Response via : Initial Calibration

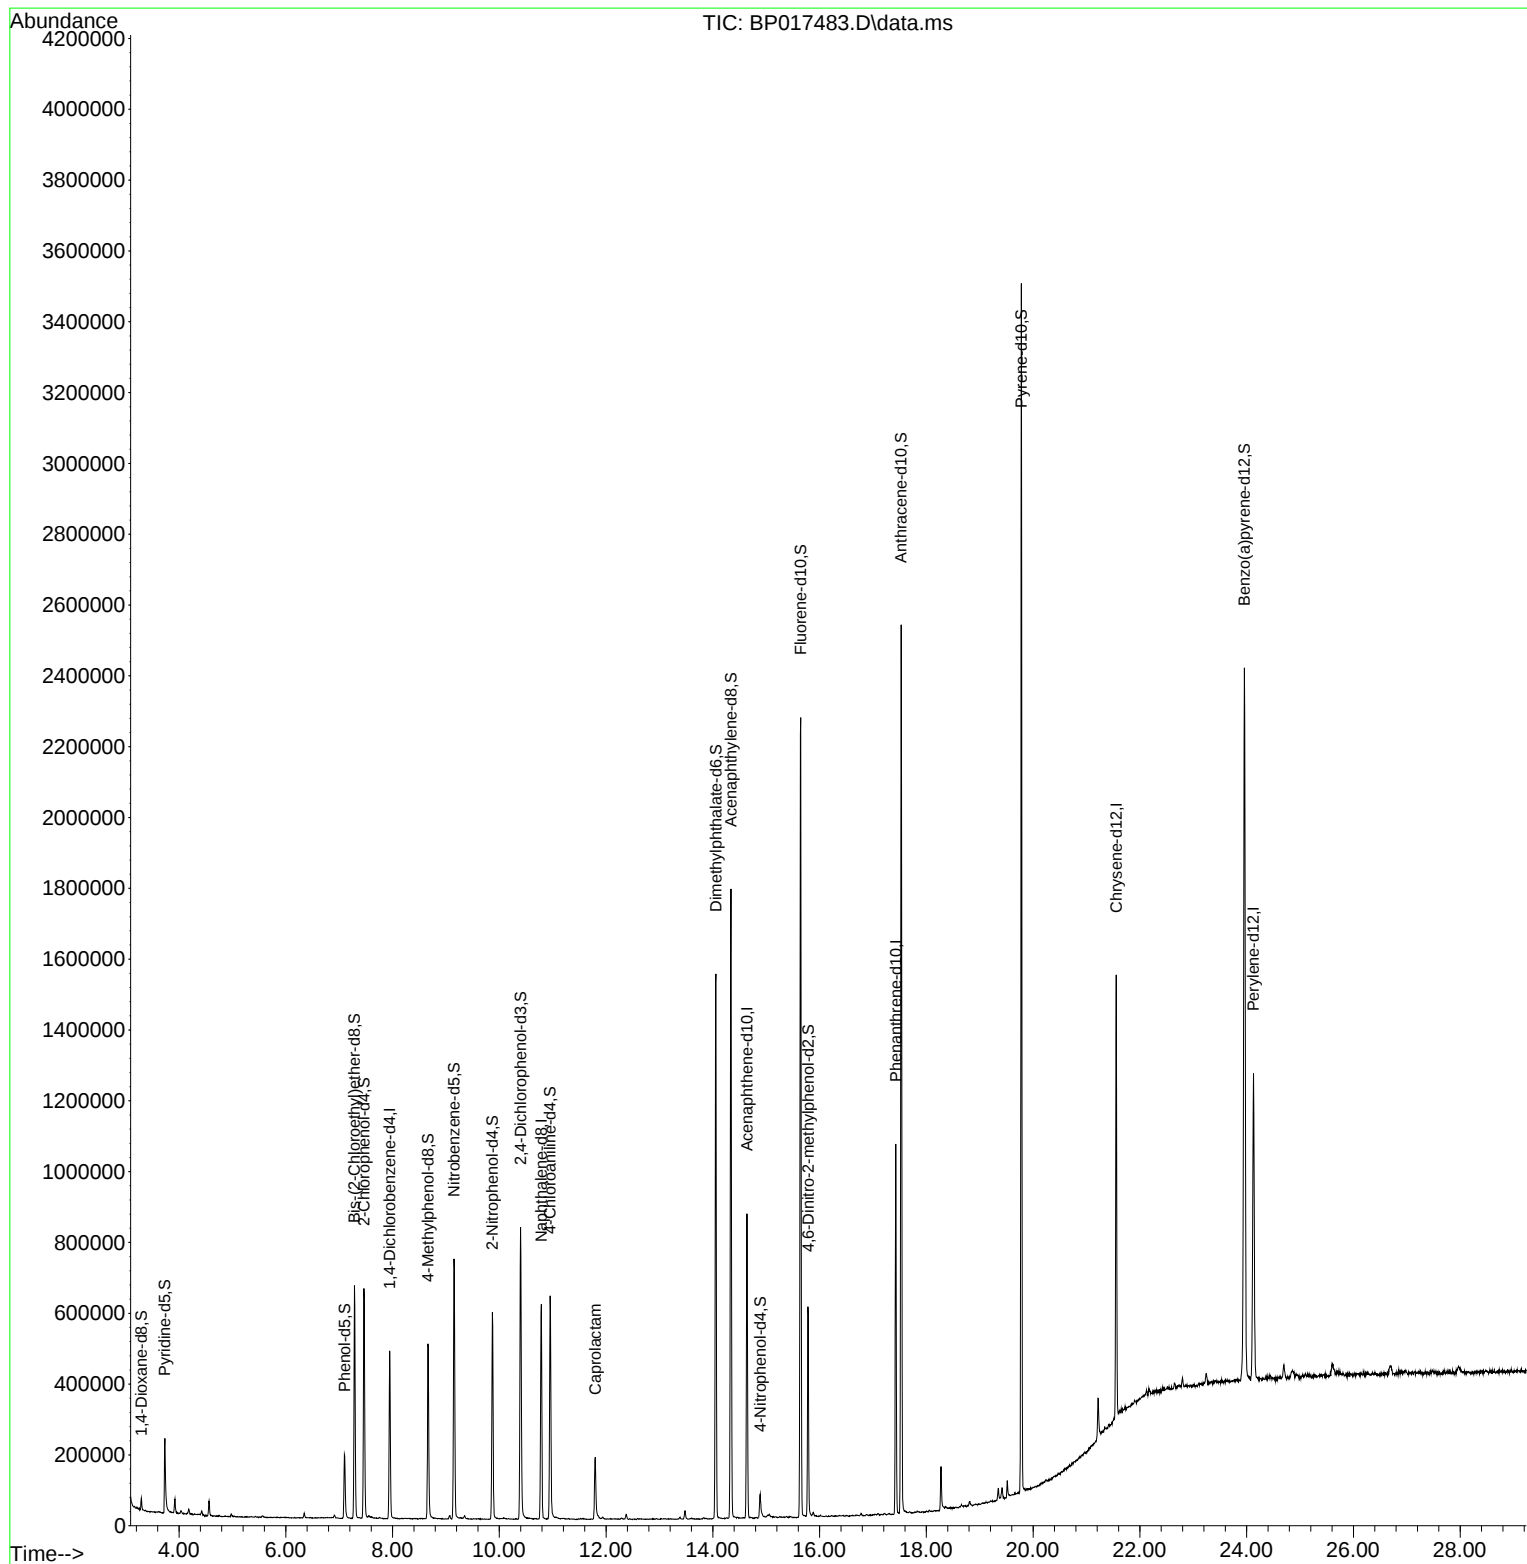

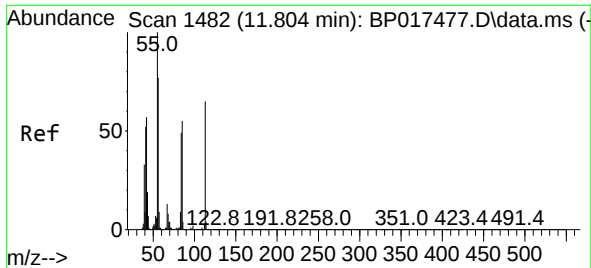

#34
Caprolactam
Concen: 16.814 ng/ul
RT: 11.799 min Scan# 14
Delta R.T. -0.012 min
Lab File: BP017483.D
Acq: 02 Oct 2023 18:33

Instrument :
BNA_P
ClientSampleId :
BBK62

Tgt Ion:113 Resp: 34027
Ion Ratio Lower Upper
113 100
55 159.7 127.4 191.0
56 123.2 94.5 141.7

