

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
 Data File : BP017478.D
 Acq On : 02 Oct 2023 15:41
 Operator : MA/JU
 Sample : PB155899BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK899

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017478.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	40	rBV	33620	42224	1.55%	0.158%
2	3.728	106	109	127	rBV	394834	624860	22.99%	2.338%
3	4.040	159	162	167	rVB4	7379	10718	0.39%	0.040%
4	4.893	304	307	310	rBV5	2422	3212	0.12%	0.012%
5	7.104	676	683	692	rBV	465559	771012	28.37%	2.884%
6	7.293	707	715	726	rVB	387440	606924	22.33%	2.271%
7	7.469	738	745	760	rBV	491070	804131	29.59%	3.008%
8	7.946	819	826	835	rBV	357630	569335	20.95%	2.130%
9	8.669	941	949	963	rBV	550779	942620	34.69%	3.526%
10	9.157	1024	1032	1042	rBV	455390	747104	27.49%	2.795%
11	9.287	1051	1054	1056	rBV4	2701	3052	0.11%	0.011%
12	9.869	1145	1153	1165	rBV	357029	601033	22.12%	2.249%
13	9.957	1167	1168	1173	rVB5	3502	3906	0.14%	0.015%
14	10.398	1235	1243	1264	rBV	549684	980459	36.08%	3.668%
15	10.787	1300	1309	1319	rBV	477783	795057	29.26%	2.974%
16	10.951	1331	1337	1351	rBV	535286	955377	35.16%	3.574%
17	11.845	1479	1489	1491	rBV	3550	9715	0.36%	0.036%
18	12.028	1517	1520	1523	rBV5	1757	2920	0.11%	0.011%
19	12.381	1572	1580	1587	rBV4	9343	19234	0.71%	0.072%
20	12.469	1592	1595	1598	rVB5	2167	2856	0.11%	0.011%
21	12.622	1618	1621	1624	rBV4	2307	3129	0.12%	0.012%
22	13.169	1709	1714	1716	rVB6	2210	3038	0.11%	0.011%
23	13.233	1722	1725	1729	rVB5	2531	3663	0.13%	0.014%
24	13.481	1760	1767	1771	rVV6	7239	11378	0.42%	0.043%
25	13.604	1782	1788	1791	rVB8	1989	3172	0.12%	0.012%
26	14.057	1857	1865	1877	rBV	969399	1352178	49.76%	5.059%
27	14.339	1903	1913	1928	rBV	1109881	1625813	59.83%	6.082%
28	14.639	1957	1964	1976	rBV	699499	1000906	36.83%	3.744%
29	14.880	1998	2005	2025	rBV	195352	420558	15.48%	1.573%
30	15.645	2128	2135	2149	rBV	1448263	2045327	75.27%	7.652%
31	15.786	2153	2159	2169	rBV	266874	387101	14.24%	1.448%
32	15.880	2172	2175	2179	rVB4	6541	8216	0.30%	0.031%
33	16.980	2356	2362	2364	rBV7	1908	3167	0.12%	0.012%
34	17.086	2376	2380	2382	rBV5	2234	3045	0.11%	0.011%
35	17.216	2398	2402	2406	rBV7	2364	3448	0.13%	0.013%
36	17.427	2431	2438	2448	rBV	861362	1212827	44.63%	4.537%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017478.D
Acq On : 02 Oct 2023 15:41
Operator : MA/JU
Sample : PB155899BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK899

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Title : SVOA CALIBRATION

37	17.527	2448	2455	2470	rBV2	1594235	2269572	83.52%	8.491%
38	19.351	2761	2765	2770	rBV3	21150	29125	1.07%	0.109%
39	19.415	2774	2776	2785	rVB	17047	25041	0.92%	0.094%
40	19.780	2832	2838	2848	rBV	2118188	2717464	100.00%	10.166%
41	21.557	3135	3140	3147	rBV	960868	1313624	48.34%	4.914%
42	23.956	3542	3548	3563	rVB2	1224588	2491421	91.68%	9.321%
43	24.127	3572	3577	3588	rVB	636532	1301184	47.88%	4.868%



Sum of corrected areas: 26730146

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017478.D
Acq On : 02 Oct 2023 15:41
Operator : MA/JU
Sample : PB155899BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK899

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

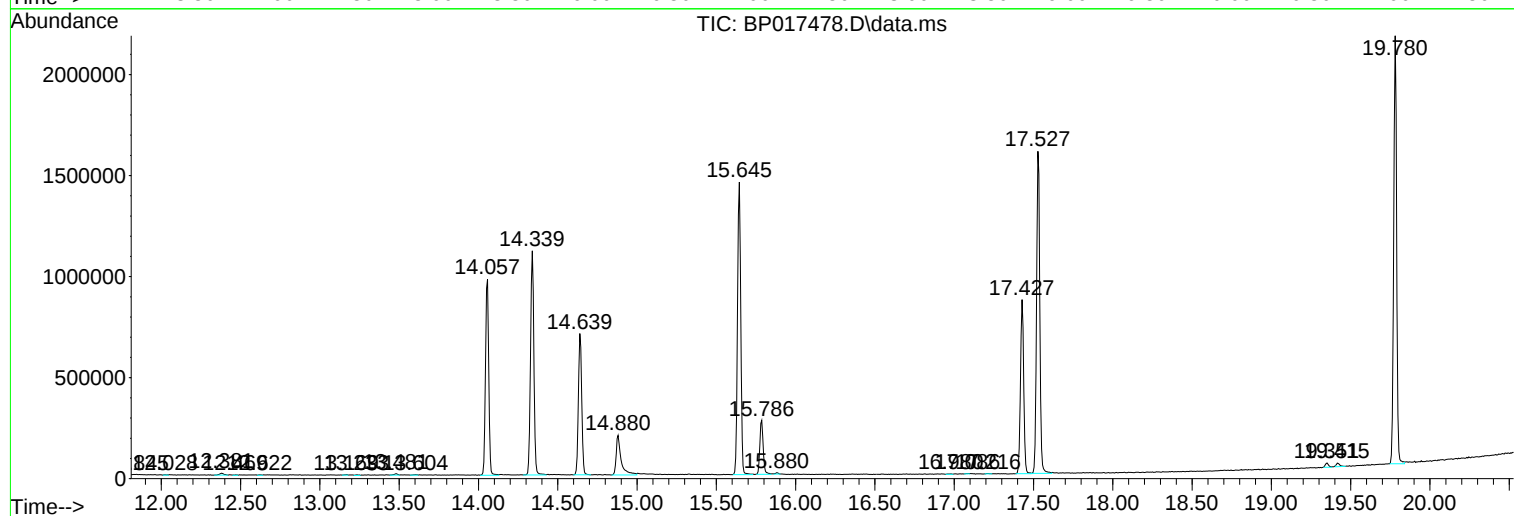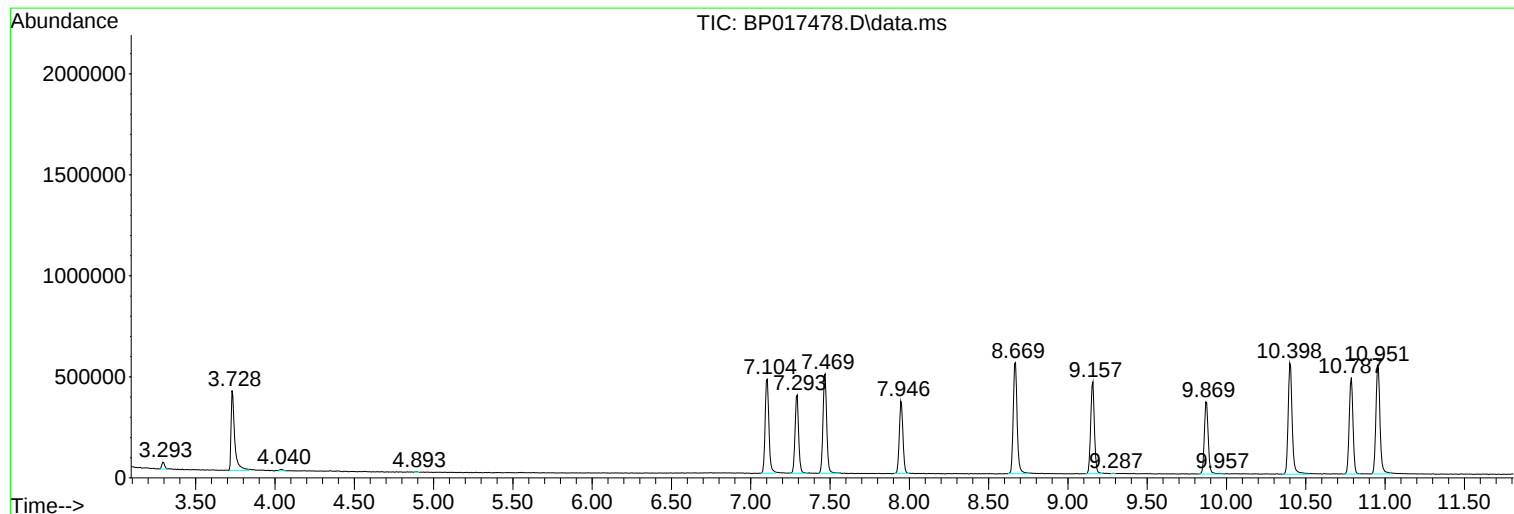

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017478.D
Acq On : 02 Oct 2023 15:41
Operator : MA/JU
Sample : PB155899BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK899

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017478.D
Acq On : 02 Oct 2023 15:41
Operator : MA/JU
Sample : PB155899BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK899

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------