

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
 Data File : BP017480.D
 Acq On : 02 Oct 2023 16:50
 Operator : MA/JU
 Sample : 04562-09 50X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCJL9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017480.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.040	158	162	165	rBV5	5858	9072	0.67%	0.129%
2	4.805	290	292	294	rBV3	1830	2359	0.17%	0.034%
3	5.005	324	326	328	rBV3	2064	1592	0.12%	0.023%
4	5.569	420	422	426	rVB5	1778	2668	0.20%	0.038%
5	6.064	503	506	507	rBV2	3126	2058	0.15%	0.029%
6	6.152	518	521	523	rBV4	1801	2338	0.17%	0.033%
7	6.711	613	616	618	rVB4	1728	1861	0.14%	0.026%
8	6.852	638	640	644	rVB5	1927	1915	0.14%	0.027%
9	7.040	670	672	675	rVB4	2148	2313	0.17%	0.033%
10	7.093	679	681	683	rBV3	2285	2541	0.19%	0.036%
11	7.116	683	685	688	rVB3	1778	2246	0.17%	0.032%
12	7.293	710	715	721	rBV4	7063	11388	0.84%	0.162%
13	7.475	741	746	752	rVB6	6116	12534	0.92%	0.178%
14	7.563	759	761	766	rVB6	2001	1815	0.13%	0.026%
15	7.681	778	781	782	rBV2	2300	2262	0.17%	0.032%
16	7.946	820	826	844	rBV	380011	613566	45.24%	8.715%
17	8.293	882	885	887	rBV4	1557	1749	0.13%	0.025%
18	8.452	911	912	915	rVB3	1665	1466	0.11%	0.021%
19	8.516	921	923	928	rVB6	1481	1835	0.14%	0.026%
20	8.687	949	952	955	rVV4	3391	3724	0.27%	0.053%
21	8.716	955	957	962	rVB6	1986	2060	0.15%	0.029%
22	9.163	1028	1033	1039	rVB4	6177	12187	0.90%	0.173%
23	9.210	1039	1041	1044	rBV4	1596	1478	0.11%	0.021%
24	9.387	1070	1071	1074	rVB3	2358	1915	0.14%	0.027%
25	9.493	1086	1089	1092	rVB5	1474	1766	0.13%	0.025%
26	9.546	1096	1098	1102	rVB5	1391	1884	0.14%	0.027%
27	9.599	1104	1107	1108	rBV3	1584	1521	0.11%	0.022%
28	9.816	1143	1144	1147	rVB3	1942	1770	0.13%	0.025%
29	9.846	1147	1149	1150	rBV2	1693	1533	0.11%	0.022%
30	9.881	1150	1155	1160	rVV9	3934	8623	0.64%	0.122%
31	9.975	1170	1171	1175	rVB4	1854	1851	0.14%	0.026%
32	10.140	1194	1199	1202	rBV7	1796	2704	0.20%	0.038%
33	10.175	1202	1205	1207	rBV4	1556	1963	0.14%	0.028%
34	10.422	1241	1247	1248	rBV6	4052	5930	0.44%	0.084%
35	10.499	1257	1260	1264	rVB6	1288	1743	0.13%	0.025%
36	10.681	1289	1291	1296	rVB5	2007	2972	0.22%	0.042%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
 Data File : BP017480.D
 Acq On : 02 Oct 2023 16:50
 Operator : MA/JU
 Sample : 04562-09 50X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCJL9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

37	10.787	1301	1309	1320	rBV	499750	842303	62.11%	11.964%
38	10.975	1338	1341	1344	rBV5	1844	3043	0.22%	0.043%
39	11.334	1398	1402	1404	rVB5	1790	2418	0.18%	0.034%
40	11.757	1470	1474	1476	rBV5	1315	1689	0.12%	0.024%
41	11.863	1488	1492	1496	rVB7	1774	2229	0.16%	0.032%
42	12.128	1534	1537	1539	rVB3	1573	1911	0.14%	0.027%
43	12.163	1539	1543	1545	rBV5	1483	1582	0.12%	0.022%
44	12.222	1549	1553	1556	rBV6	1668	2568	0.19%	0.036%
45	12.393	1579	1582	1584	rVB4	1605	1607	0.12%	0.023%
46	12.410	1584	1585	1588	rVV3	2088	1992	0.15%	0.028%
47	12.446	1590	1591	1595	rVB3	1641	1759	0.13%	0.025%
48	12.540	1604	1607	1610	rBV4	1367	1796	0.13%	0.026%
49	12.687	1628	1632	1633	rBV4	1136	1524	0.11%	0.022%
50	12.975	1678	1681	1684	rBV5	1551	2243	0.17%	0.032%
51	13.216	1719	1722	1723	rBV3	1853	1908	0.14%	0.027%
52	13.357	1745	1746	1749	rBV3	1349	1503	0.11%	0.021%
53	13.463	1758	1764	1765	rBV6	1224	2119	0.16%	0.030%
54	13.575	1780	1783	1786	rBV5	2893	3411	0.25%	0.048%
55	13.693	1800	1803	1804	rBV3	1337	1611	0.12%	0.023%
56	13.863	1830	1832	1835	rVB4	2273	1950	0.14%	0.028%
57	13.993	1850	1854	1856	rBV5	1419	1456	0.11%	0.021%
58	14.057	1860	1865	1876	rVB2	19499	32847	2.42%	0.467%
59	14.145	1879	1880	1883	rVB3	2219	1514	0.11%	0.022%
60	14.181	1883	1886	1889	rBV4	1693	1781	0.13%	0.025%
61	14.240	1893	1896	1897	rBV3	1788	1486	0.11%	0.021%
62	14.340	1908	1913	1919	rBV2	22191	35063	2.59%	0.498%
63	14.422	1922	1927	1928	rBV5	1376	1771	0.13%	0.025%
64	14.492	1935	1939	1942	rVB6	1744	2036	0.15%	0.029%
65	14.551	1942	1949	1957	rBV2	8870	24651	1.82%	0.350%
66	14.640	1957	1964	1978	rVB	739118	1065204	78.55%	15.130%
67	14.863	2001	2002	2008	rVB6	1743	2606	0.19%	0.037%
68	14.975	2018	2021	2025	rBV5	2123	3165	0.23%	0.045%
69	15.245	2063	2067	2068	rBV4	1864	1869	0.14%	0.027%
70	15.322	2079	2080	2083	rVB3	1826	1562	0.12%	0.022%
71	15.369	2086	2088	2091	rVV4	1480	1517	0.11%	0.022%
72	15.434	2096	2099	2101	rVB3	1832	2112	0.16%	0.030%
73	15.498	2109	2110	2114	rVB4	2233	1896	0.14%	0.027%
74	15.539	2114	2117	2119	rBV3	2883	3921	0.29%	0.056%
75	15.557	2119	2120	2123	rVB3	3102	1776	0.13%	0.025%
76	15.645	2125	2135	2141	rBV	30534	53054	3.91%	0.754%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
 Data File : BP017480.D
 Acq On : 02 Oct 2023 16:50
 Operator : MA/JU
 Sample : 04562-09 50X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCJL9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

77	15.751	2151	2153	2156	rBV4	2568	3024	0.22%	0.043%
78	15.792	2156	2160	2163	rVB4	5194	7676	0.57%	0.109%
79	15.822	2163	2165	2169	rBV5	1678	2460	0.18%	0.035%
80	15.898	2174	2178	2187	rVB7	4671	8634	0.64%	0.123%
81	16.110	2209	2214	2219	rVB2	5167	6899	0.51%	0.098%
82	16.169	2221	2224	2229	rVB7	2149	3448	0.25%	0.049%
83	16.363	2253	2257	2265	rBV2	10480	25959	1.91%	0.369%
84	16.445	2268	2271	2275	rVB	4772	6167	0.45%	0.088%
85	16.592	2291	2296	2299	rBV5	3859	6133	0.45%	0.087%
86	16.634	2299	2303	2307	rVB2	4956	5682	0.42%	0.081%
87	16.745	2321	2322	2325	rVB3	4895	3623	0.27%	0.051%
88	16.804	2330	2332	2335	rVB4	2641	2754	0.20%	0.039%
89	16.845	2335	2339	2341	rBV5	1550	1922	0.14%	0.027%
90	16.945	2352	2356	2362	rBV5	4546	5729	0.42%	0.081%
91	17.175	2394	2395	2398	rBV3	1583	1610	0.12%	0.023%
92	17.204	2398	2400	2407	rVV8	2647	4802	0.35%	0.068%
93	17.275	2408	2412	2415	rVB2	5103	6505	0.48%	0.092%
94	17.428	2432	2438	2450	rBV	910354	1278554	94.28%	18.161%
95	17.528	2450	2455	2463	rVV2	30426	51094	3.77%	0.726%
96	17.681	2479	2481	2484	rBV4	1888	2496	0.18%	0.035%
97	18.110	2552	2554	2555	rBV2	3190	2350	0.17%	0.033%
98	19.780	2834	2838	2843	rBV2	47000	62709	4.62%	0.891%
99	21.557	3135	3140	3145	rBV	1064936	1328191	97.94%	18.866%
100	24.127	3571	3577	3586	rVB	680740	1356130	100.00%	19.263%




Sum of corrected areas: 7040206

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017480.D
Acq On : 02 Oct 2023 16:50
Operator : MA/JU
Sample : 04562-09 50X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCJL9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

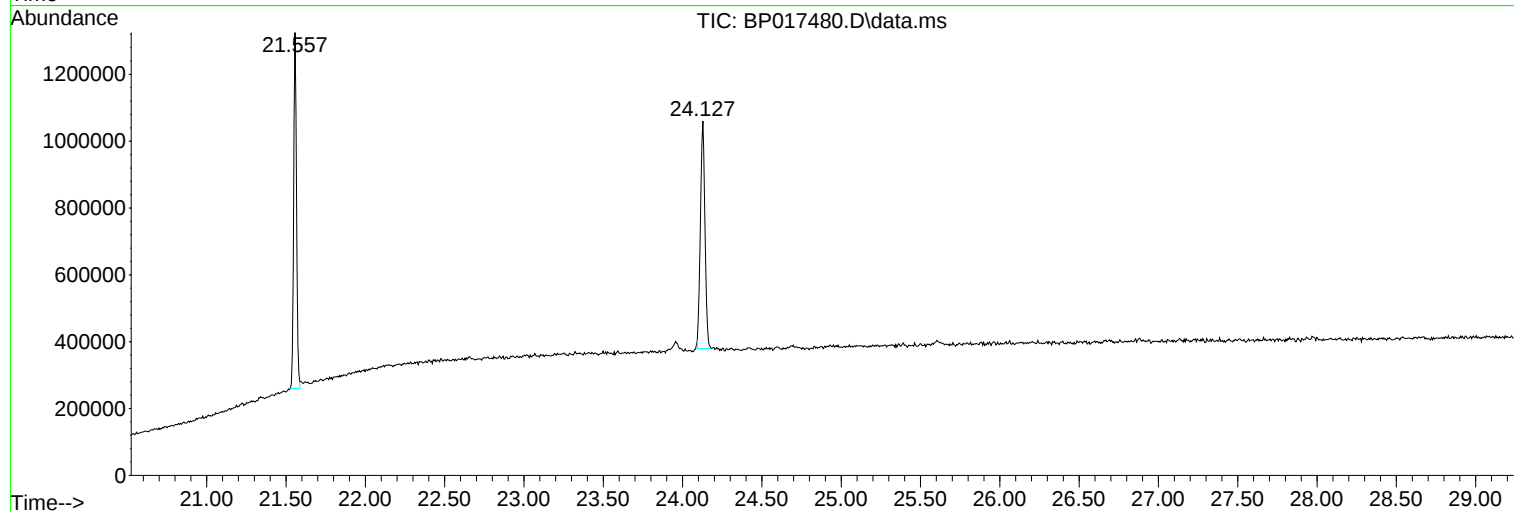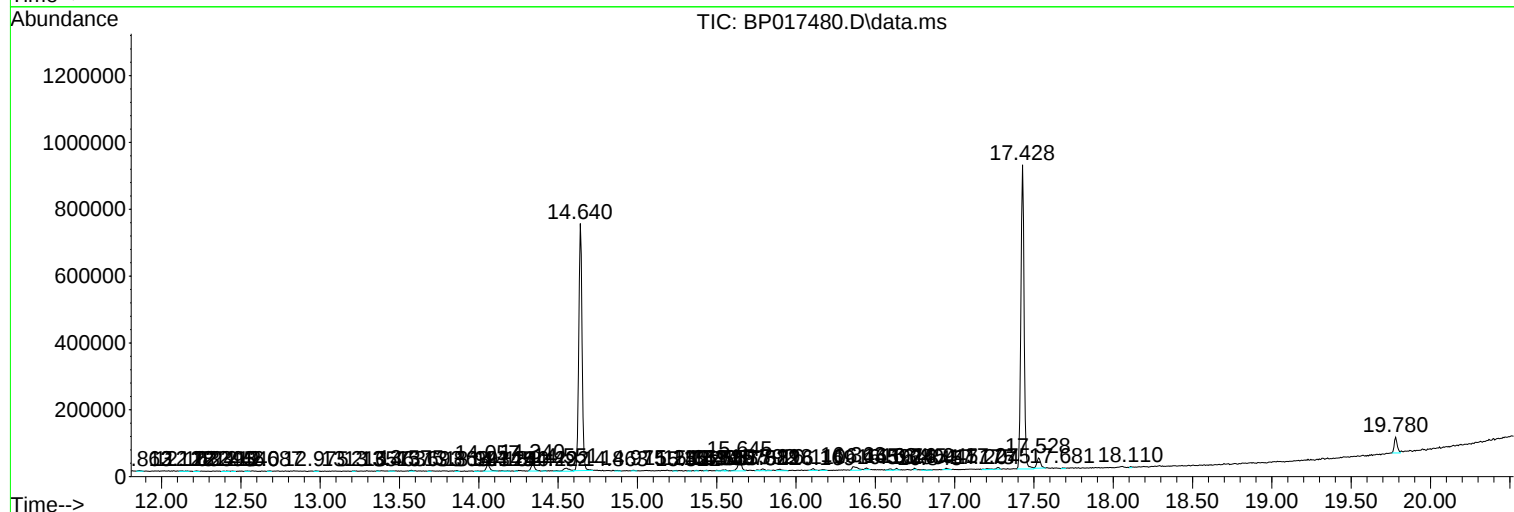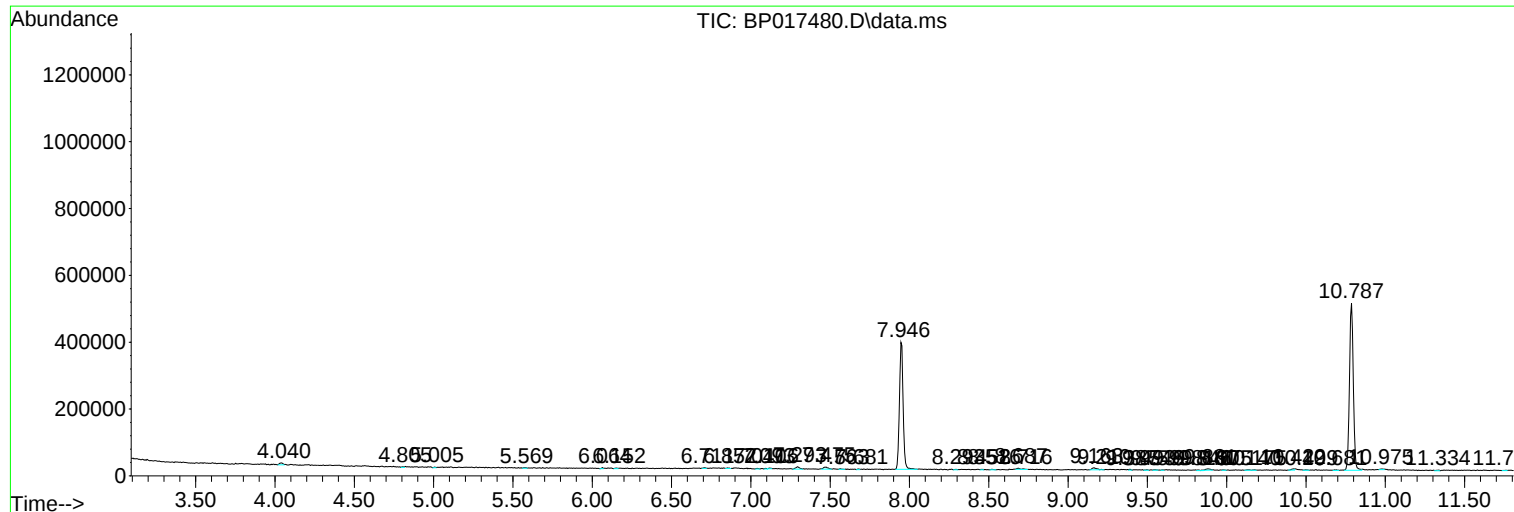

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017480.D
Acq On : 02 Oct 2023 16:50
Operator : MA/JU
Sample : 04562-09 50X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCJL9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017480.D
Acq On : 02 Oct 2023 16:50
Operator : MA/JU
Sample : 04562-09 50X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCJL9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc