

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
 Data File : BP017488.D
 Acq On : 02 Oct 2023 21:24
 Operator : MA/JU
 Sample : 04588-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJ04

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017488.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	44	rVB	32753	42917	0.92%	0.107%
2	3.734	106	110	123	rBV	187486	294508	6.28%	0.735%
3	3.917	139	141	149	rVB2	8008	11585	0.25%	0.029%
4	4.040	158	162	167	rVB2	9535	12697	0.27%	0.032%
5	4.564	245	251	259	rBV	223227	333513	7.11%	0.833%
6	5.517	409	413	421	rVB	11372	21723	0.46%	0.054%
7	5.893	473	477	481	rVB6	4050	7109	0.15%	0.018%
8	6.987	658	663	667	rBV3	3863	5878	0.13%	0.015%
9	7.099	676	682	694	rBV	122466	209163	4.46%	0.522%
10	7.287	708	714	723	rBV	603454	913784	19.49%	2.282%
11	7.463	736	744	755	rBV	563989	898087	19.16%	2.243%
12	7.558	755	760	769	rVB2	13542	29342	0.63%	0.073%
13	7.946	818	826	836	rBV	520491	805288	17.18%	2.011%
14	8.034	837	841	846	rVB5	3967	6801	0.15%	0.017%
15	8.663	940	948	966	rBV	370031	636141	13.57%	1.588%
16	9.034	1007	1011	1015	rVB7	3182	5189	0.11%	0.013%
17	9.152	1021	1031	1046	rBV	696051	1158346	24.71%	2.892%
18	9.352	1062	1065	1070	rVB7	6131	8516	0.18%	0.021%
19	9.869	1146	1153	1172	rBV	560688	929885	19.84%	2.322%
20	10.152	1195	1201	1206	rVB8	4151	6899	0.15%	0.017%
21	10.399	1236	1243	1254	rBV	783921	1328525	28.34%	3.317%
22	10.781	1301	1308	1316	rBV	666623	1098055	23.43%	2.742%
23	10.952	1330	1337	1355	rBV	722063	1259239	26.86%	3.144%
24	11.804	1476	1482	1488	rBV3	19416	46042	0.98%	0.115%
25	12.375	1574	1579	1585	rBV	14449	21948	0.47%	0.055%
26	12.451	1588	1592	1601	rVB9	6277	10293	0.22%	0.026%
27	13.381	1747	1750	1754	rBV6	3971	5990	0.13%	0.015%
28	13.475	1761	1766	1771	rBV2	23495	36717	0.78%	0.092%
29	14.051	1858	1864	1873	rBV	1566676	2139344	45.64%	5.342%
30	14.340	1905	1913	1924	rBV	1781855	2582104	55.08%	6.448%
31	14.640	1956	1964	1972	rBV	1005435	1425270	30.41%	3.559%
32	14.887	2000	2006	2019	rBV2	46503	115755	2.47%	0.289%
33	15.381	2085	2090	2094	rVB	25290	30372	0.65%	0.076%
34	15.457	2099	2103	2111	rVB	21808	32299	0.69%	0.081%
35	15.640	2128	2134	2142	rBV	2291169	3286956	70.12%	8.208%
36	15.716	2146	2147	2151	rVV3	7529	7453	0.16%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
 Data File : BP017488.D
 Acq On : 02 Oct 2023 21:24
 Operator : MA/JU
 Sample : 04588-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJ04

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

37	15.781	2152	2158	2170	rVV	695473	923914	19.71%	2.307%
38	15.887	2172	2176	2184	rVB5	11782	21997	0.47%	0.055%
39	16.769	2320	2326	2329	rBV7	3660	6747	0.14%	0.017%
40	17.086	2377	2380	2382	rBV4	4351	5274	0.11%	0.013%
41	17.210	2397	2401	2403	rBV5	3679	4921	0.10%	0.012%
42	17.339	2420	2423	2426	rBV5	3372	4753	0.10%	0.012%
43	17.428	2430	2438	2448	rBV	1246682	1771449	37.79%	4.423%
44	17.528	2448	2455	2467	rBV2	2806394	3827384	81.65%	9.557%
45	18.051	2542	2544	2551	rVB8	8013	11118	0.24%	0.028%
46	18.269	2577	2581	2589	rBV2	60719	94924	2.03%	0.237%
47	18.357	2594	2596	2602	rVB2	8568	12728	0.27%	0.032%
48	18.416	2603	2606	2609	rBV5	10013	13708	0.29%	0.034%
49	19.192	2735	2738	2742	rVB5	33136	36735	0.78%	0.092%
50	19.345	2761	2764	2768	rVB	37446	39662	0.85%	0.099%
51	19.416	2773	2776	2780	rVB	32739	39410	0.84%	0.098%
52	19.516	2789	2793	2797	rBV3	46333	62943	1.34%	0.157%
53	19.780	2832	2838	2844	rBV	3651084	4687533	100.00%	11.705%
54	21.557	3135	3140	3147	rBV	1483450	1973232	42.10%	4.927%
55	23.957	3541	3548	3562	rVB2	2272714	4678794	99.81%	11.683%
56	24.127	3570	3577	3586	rVB	1009097	2067034	44.10%	5.161%




Sum of corrected areas: 40047993

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017488.D
Acq On : 02 Oct 2023 21:24
Operator : MA/JU
Sample : 04588-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

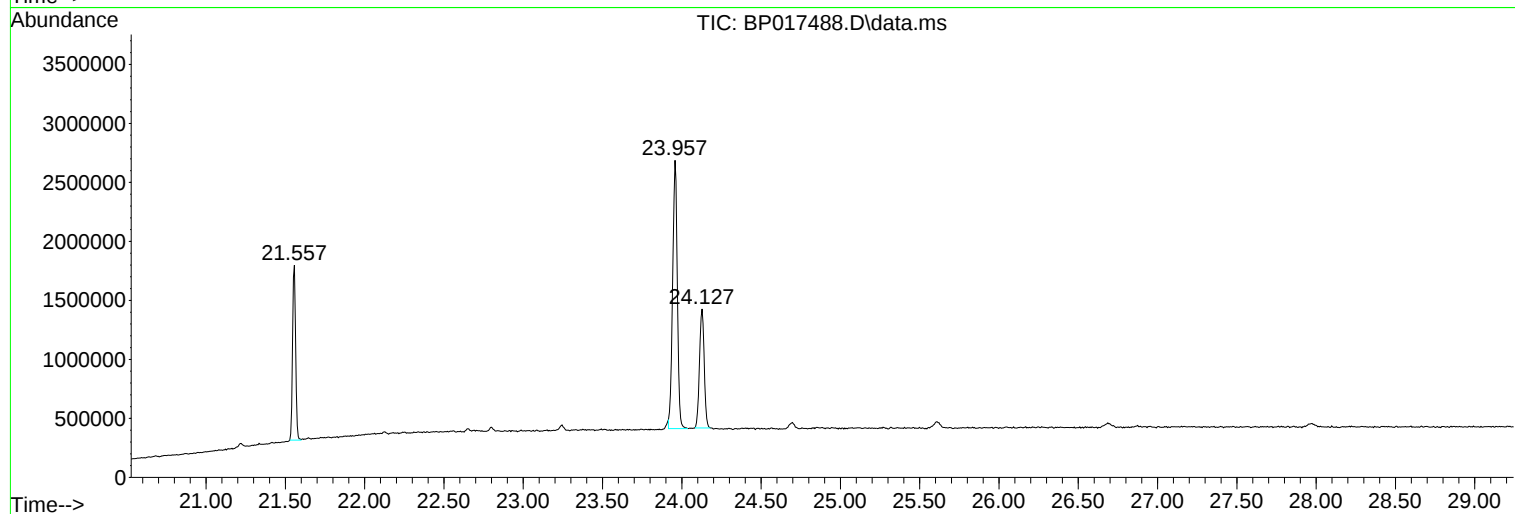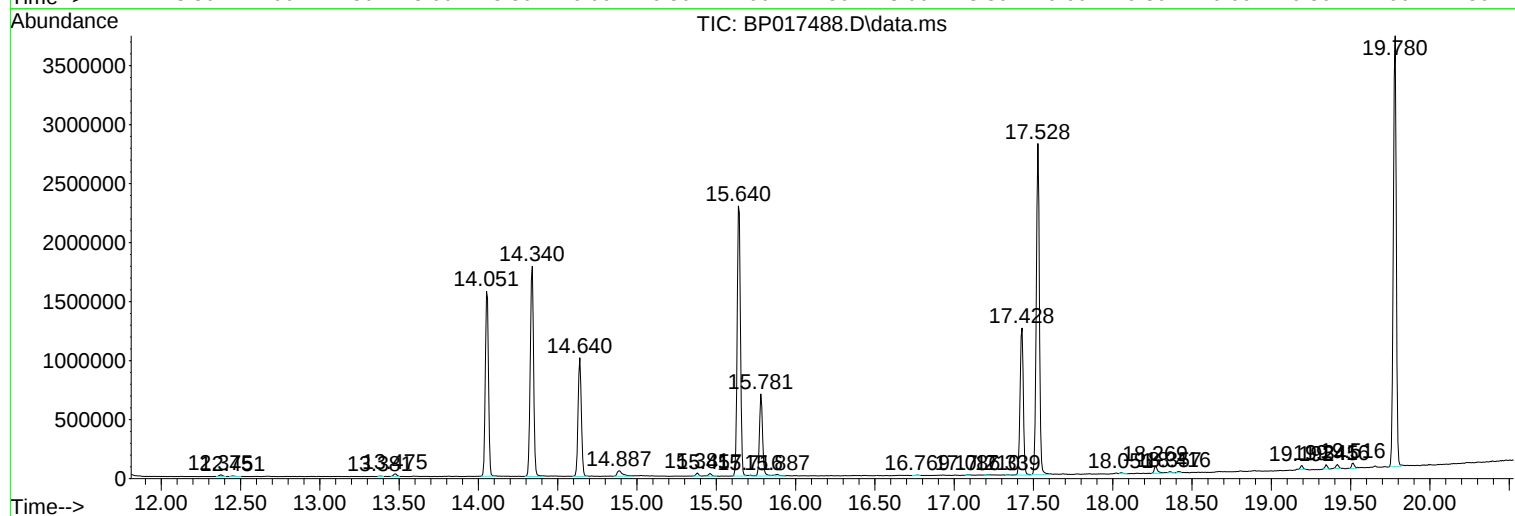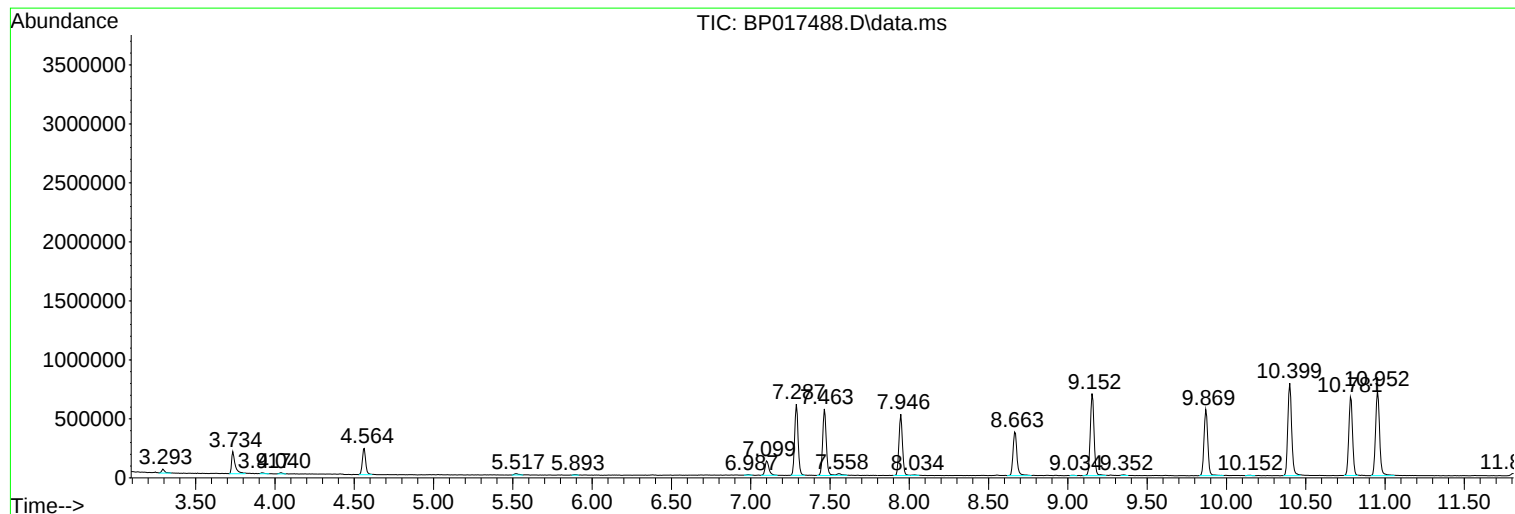

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017488.D
Acq On : 02 Oct 2023 21:24
Operator : MA/JU
Sample : 04588-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ04










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.564	8.28 ng/ul	333513	1,4-Dichlorobenzene-d4	7.946

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	16

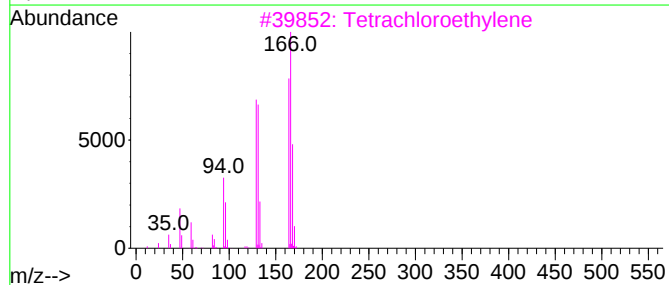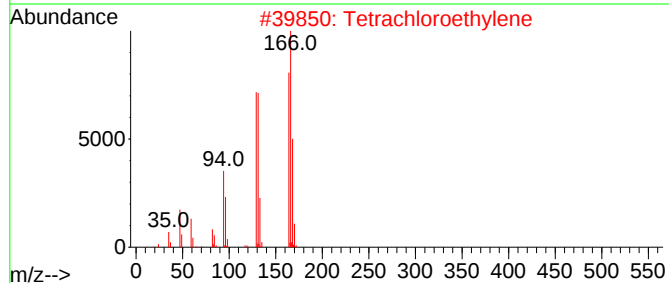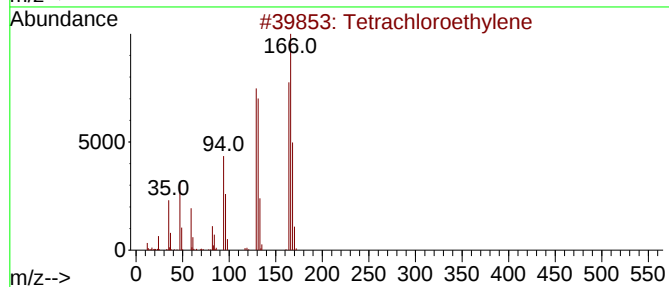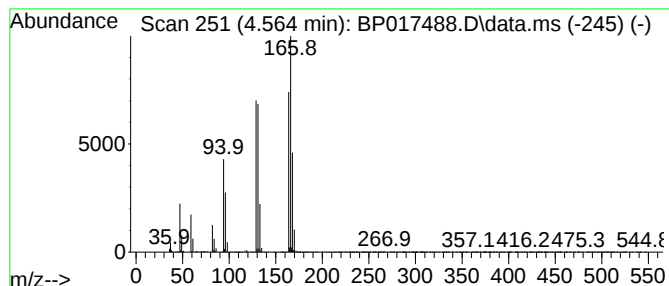

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017488.D
Acq On : 02 Oct 2023 21:24
Operator : MA/JU
Sample : 04588-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.564	8.3	ng/u1	333513	1	7.946	805288	20.0