

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
 Data File : BP017492.D
 Acq On : 03 Oct 2023 00:14
 Operator : MA/JU
 Sample : PB155900BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK900

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017492.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	43	rVB	51743	67361	1.68%	0.163%
2	3.728	105	109	128	rBV	624185	976952	24.43%	2.361%
3	4.034	158	161	165	rVB2	8529	11327	0.28%	0.027%
4	7.099	675	682	693	rBV	787826	1259180	31.49%	3.043%
5	7.287	707	714	724	rVB	653531	994303	24.87%	2.403%
6	7.463	736	744	759	rBV	826052	1312096	32.81%	3.171%
7	7.946	819	826	836	rBV	548338	883885	22.11%	2.136%
8	8.663	941	948	965	rBV	951426	1549866	38.76%	3.745%
9	9.152	1023	1031	1044	rBV	764778	1223346	30.60%	2.956%
10	9.869	1146	1153	1164	rBV	618729	1022845	25.58%	2.472%
11	10.399	1232	1243	1264	rBV	881562	1572002	39.31%	3.799%
12	10.781	1300	1308	1317	rBV	743636	1217819	30.46%	2.943%
13	10.951	1329	1337	1350	rBV	881263	1538854	38.49%	3.719%
14	12.375	1571	1579	1585	rBV2	13660	23882	0.60%	0.058%
15	13.475	1760	1766	1772	rBV8	6604	10913	0.27%	0.026%
16	13.587	1782	1785	1789	rBV5	3150	4388	0.11%	0.011%
17	14.051	1856	1864	1875	rBV	1609215	2077009	51.94%	5.019%
18	14.334	1905	1912	1922	rBV	1803421	2508382	62.73%	6.062%
19	14.634	1957	1963	1974	rBV	1012526	1495080	37.39%	3.613%
20	14.875	1996	2004	2028	rBV	416701	816888	20.43%	1.974%
21	15.639	2125	2134	2142	rBV	2189192	3065091	76.66%	7.407%
22	15.781	2152	2158	2166	rBV	562648	742387	18.57%	1.794%
23	15.881	2170	2175	2181	rVB3	10803	19299	0.48%	0.047%
24	16.357	2247	2256	2258	rBV10	2202	4901	0.12%	0.012%
25	16.433	2266	2269	2273	rVB5	3660	5688	0.14%	0.014%
26	16.686	2307	2312	2316	rBV8	3069	5897	0.15%	0.014%
27	17.204	2396	2400	2405	rBV7	3732	7908	0.20%	0.019%
28	17.422	2431	2437	2447	rBV	1250009	1725318	43.15%	4.169%
29	17.522	2448	2454	2470	rVV2	2382903	3323853	83.13%	8.033%
30	18.275	2578	2582	2587	rBV8	3432	6809	0.17%	0.016%
31	19.345	2760	2764	2768	rBV3	29054	39731	0.99%	0.096%
32	19.416	2773	2776	2782	rVB	22825	31279	0.78%	0.076%
33	19.774	2831	2837	2846	rBV	3088891	3998503	100.00%	9.663%
34	21.551	3134	3139	3147	rBV	1471200	1922803	48.09%	4.647%
35	23.951	3540	3547	3560	rVB2	1914461	3935693	98.43%	9.511%
36	24.121	3569	3576	3586	rVB	979077	1977978	49.47%	4.780%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017492.D
Acq On : 03 Oct 2023 00:14
Operator : MA/JU
Sample : PB155900BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK900

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 41379516

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017492.D
Acq On : 03 Oct 2023 00:14
Operator : MA/JU
Sample : PB155900BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK900

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

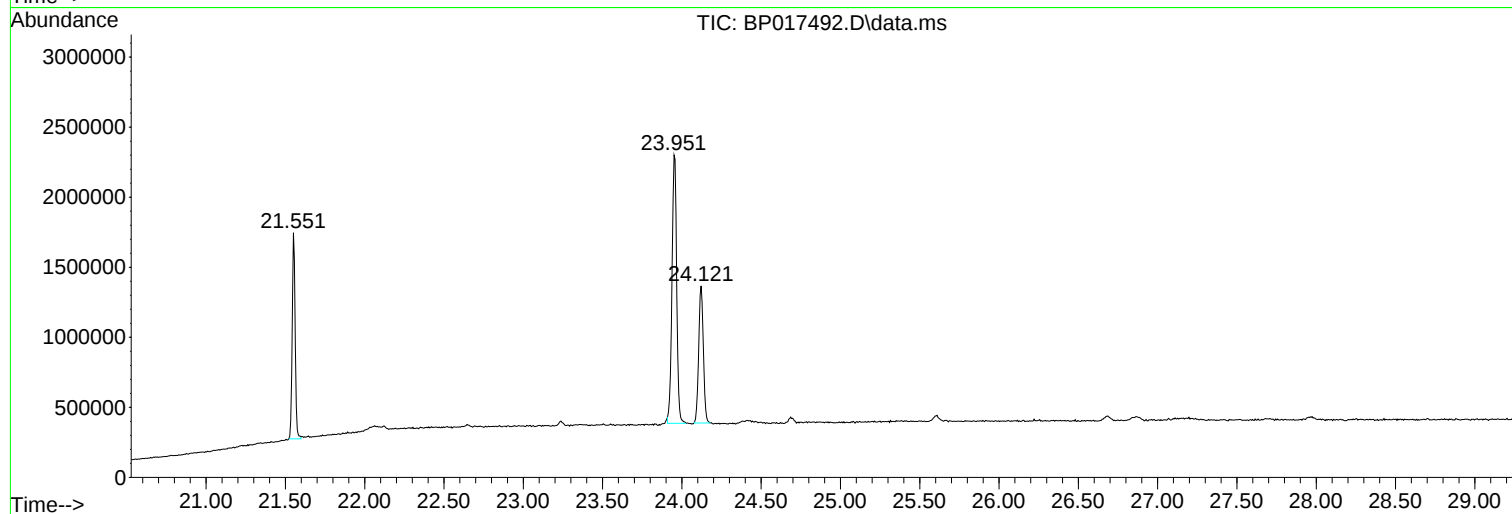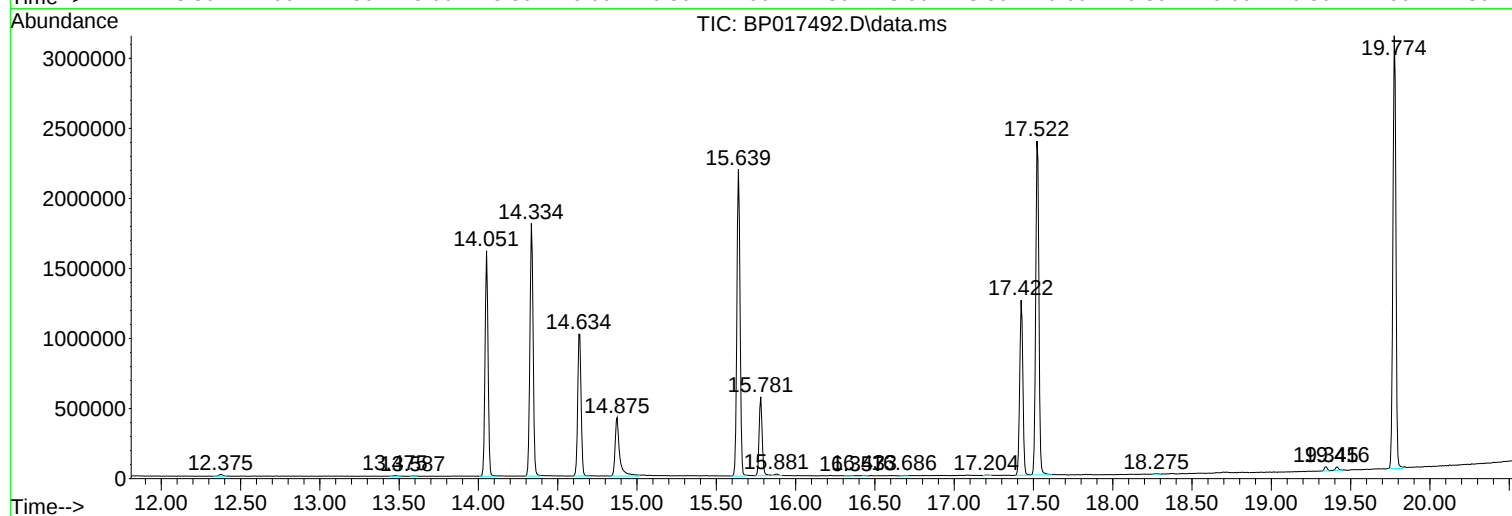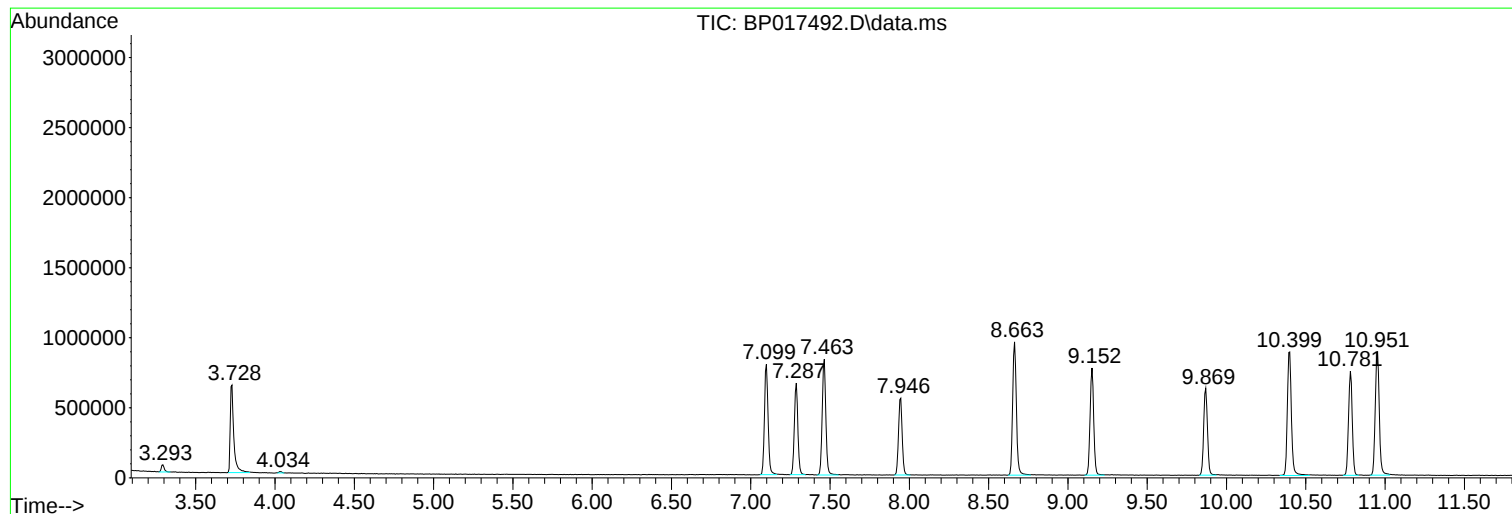

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017492.D
Acq On : 03 Oct 2023 00:14
Operator : MA/JU
Sample : PB155900BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK900

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017492.D
Acq On : 03 Oct 2023 00:14
Operator : MA/JU
Sample : PB155900BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK900

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------