

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
 Data File : BP017493.D
 Acq On : 03 Oct 2023 00:48
 Operator : MA/JU
 Sample : PB155903BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK903

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017493.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	43	rVB	46166	60171	1.55%	0.148%
2	3.728	105	109	126	rBV	540145	848125	21.83%	2.093%
3	4.034	157	161	167	rVB2	10578	16677	0.43%	0.041%
4	7.099	675	682	697	rBV	654267	1067447	27.47%	2.634%
5	7.287	706	714	722	rBV	533515	821149	21.13%	2.026%
6	7.463	736	744	754	rBV	708133	1101061	28.34%	2.717%
7	7.940	818	825	833	rBV	601947	953883	24.55%	2.353%
8	8.663	939	948	968	rBV	811700	1317502	33.91%	3.251%
9	9.069	1015	1017	1023	rBV7	1828	4092	0.11%	0.010%
10	9.152	1023	1031	1042	rBV	634797	1030767	26.53%	2.543%
11	9.869	1143	1153	1166	rBV	527939	878709	22.61%	2.168%
12	10.399	1235	1243	1259	rBV	771518	1356754	34.92%	3.347%
13	10.781	1298	1308	1317	rBV	833959	1344710	34.61%	3.318%
14	10.951	1329	1337	1349	rBV	773125	1344245	34.59%	3.317%
15	12.375	1574	1579	1586	rBV2	11777	19728	0.51%	0.049%
16	13.475	1762	1766	1771	rBV5	6082	10708	0.28%	0.026%
17	13.592	1780	1786	1789	rBV8	3917	6816	0.18%	0.017%
18	14.051	1857	1864	1874	rBV	1444687	1901967	48.95%	4.693%
19	14.334	1905	1912	1929	rBV	1628569	2294340	59.04%	5.661%
20	14.639	1957	1964	1974	rBV	1178895	1736651	44.69%	4.285%
21	14.875	1997	2004	2022	rBV	392668	768032	19.76%	1.895%
22	15.334	2074	2082	2085	rBV10	2735	6671	0.17%	0.016%
23	15.639	2127	2134	2145	rBV	2019678	2883842	74.21%	7.115%
24	15.781	2151	2158	2168	rBV	541916	724581	18.65%	1.788%
25	15.875	2170	2174	2184	rVB3	10449	19540	0.50%	0.048%
26	16.375	2253	2259	2262	rBV7	2544	4581	0.12%	0.011%
27	17.086	2377	2380	2387	rVB8	3379	5840	0.15%	0.014%
28	17.210	2397	2401	2405	rBV6	4345	6261	0.16%	0.015%
29	17.422	2431	2437	2447	rBV	1481703	2119120	54.53%	5.228%
30	17.528	2447	2455	2467	rVV	2285494	3219708	82.86%	7.944%
31	19.345	2760	2764	2768	rBV3	28215	37085	0.95%	0.091%
32	19.416	2772	2776	2780	rVV2	22711	30729	0.79%	0.076%
33	19.774	2832	2837	2845	rBV	3035427	3885847	100.00%	9.587%
34	21.551	3134	3139	3148	rBV	1866012	2389795	61.50%	5.896%
35	23.951	3540	3547	3559	rVB2	1851983	3826251	98.47%	9.440%
36	24.121	3569	3576	3590	rVB	1188988	2487338	64.01%	6.137%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017493.D
Acq On : 03 Oct 2023 00:48
Operator : MA/JU
Sample : PB155903BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK903

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 40530723

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017493.D
Acq On : 03 Oct 2023 00:48
Operator : MA/JU
Sample : PB155903BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK903

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

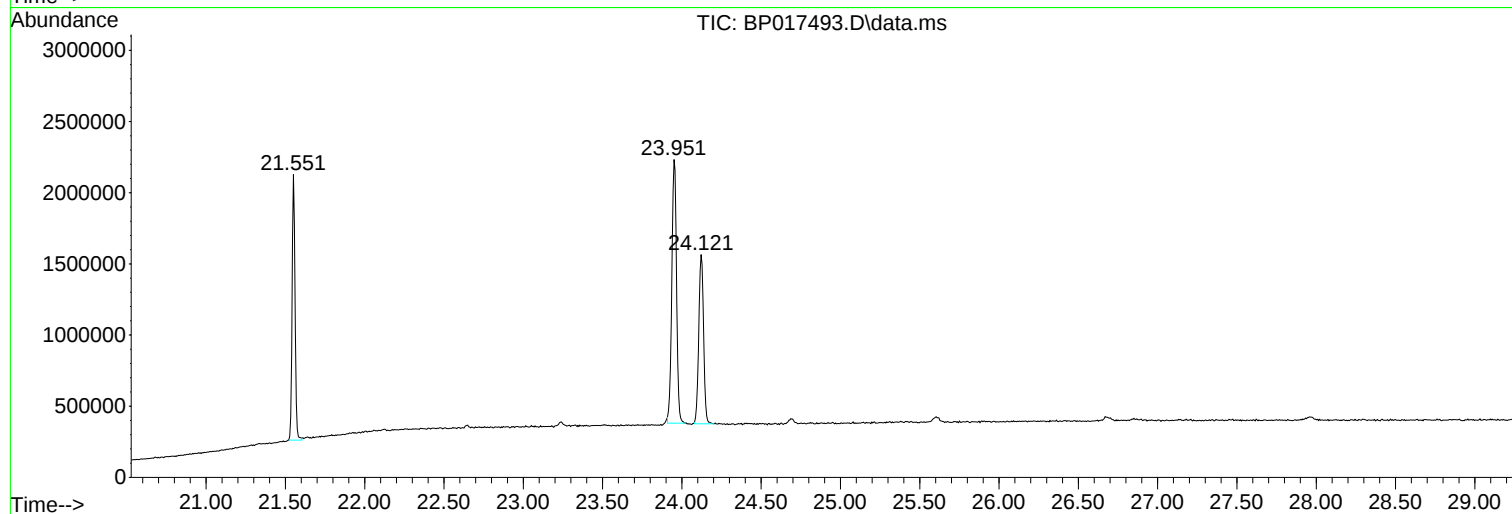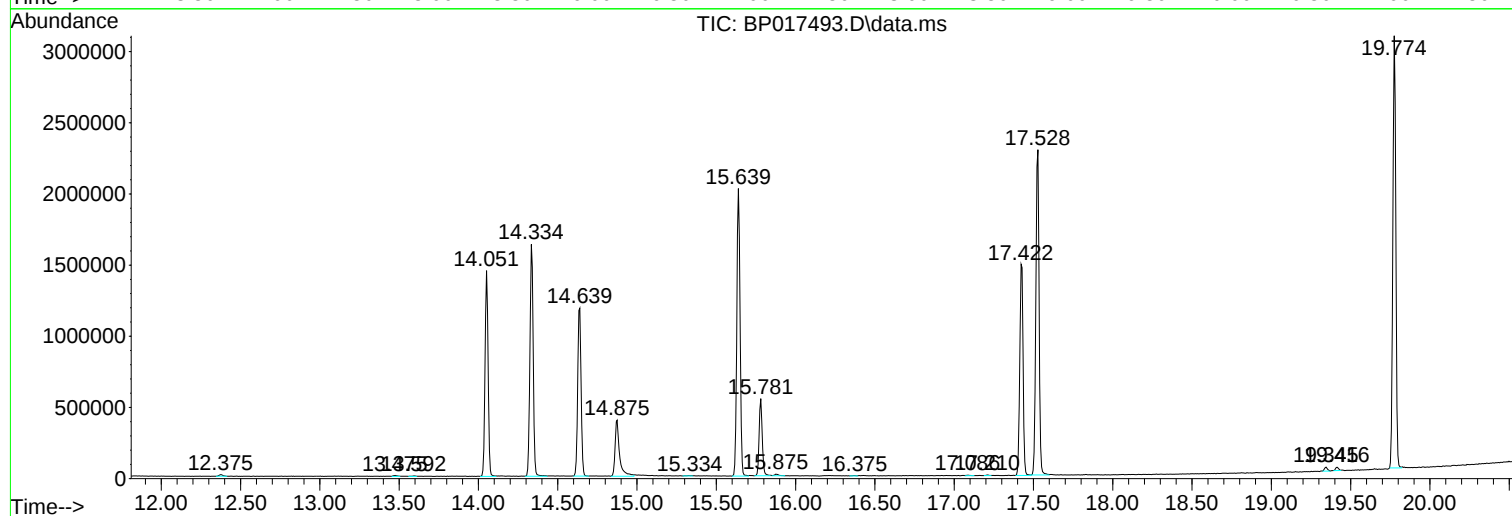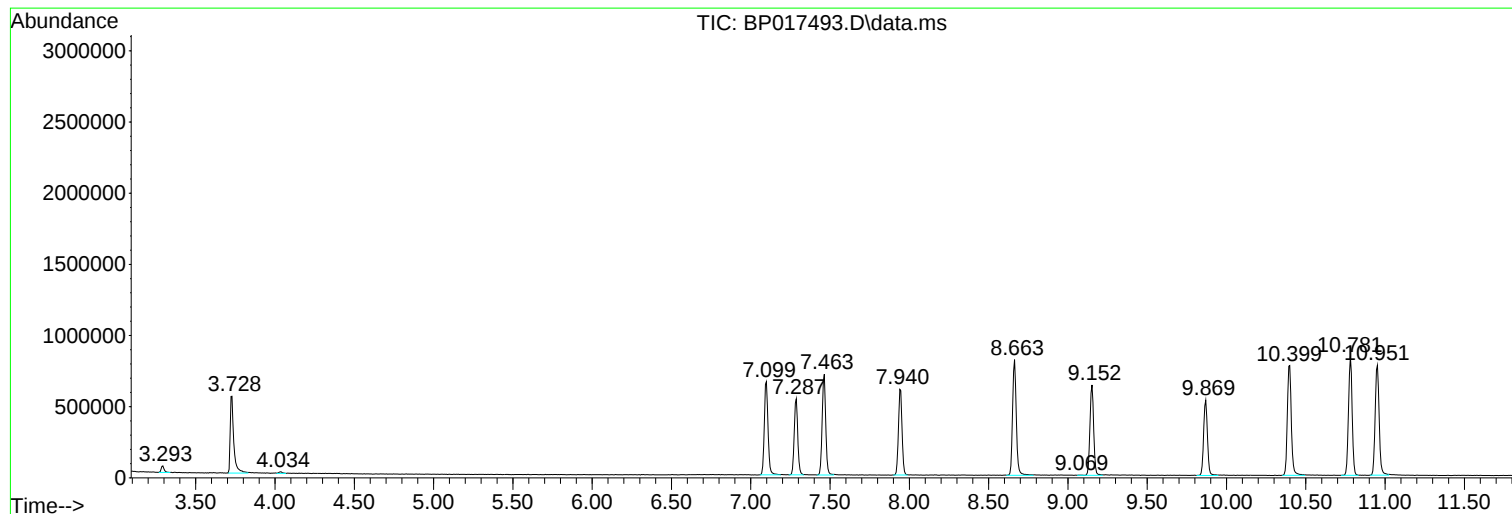

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017493.D
Acq On : 03 Oct 2023 00:48
Operator : MA/JU
Sample : PB155903BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK903

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017493.D
Acq On : 03 Oct 2023 00:48
Operator : MA/JU
Sample : PB155903BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK903

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc