

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
 Data File : BP017494.D
 Acq On : 03 Oct 2023 01:22
 Operator : MA/JU
 Sample : PB155906BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK906

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M

Title : SVOA CALIBRATION

Signal : TIC: BP017494.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	31	34	42	rVB	54843	67384	1.64%	0.155%
2	3.723	104	108	123	rBV	694181	1027398	24.95%	2.370%
3	4.028	158	160	166	rVB2	8078	11401	0.28%	0.026%
4	7.093	674	681	697	rBV	855969	1357279	32.96%	3.131%
5	7.281	707	713	723	rVB	665829	1030994	25.04%	2.378%
6	7.458	736	743	753	rBV	853345	1355398	32.92%	3.126%
7	7.940	818	825	835	rVB	546987	846815	20.57%	1.953%
8	8.658	941	947	963	rBV	1001909	1679933	40.80%	3.875%
9	9.152	1023	1031	1042	rBV	795330	1325055	32.18%	3.056%
10	9.863	1145	1152	1165	rBV	679710	1121159	27.23%	2.586%
11	10.281	1219	1223	1228	rVB8	2641	4906	0.12%	0.011%
12	10.393	1235	1242	1255	rBV	1030119	1721876	41.82%	3.971%
13	10.781	1300	1308	1317	rBV	743594	1238559	30.08%	2.857%
14	10.946	1327	1336	1356	rBV	965931	1729943	42.02%	3.990%
15	12.369	1572	1578	1587	rBV3	14751	30180	0.73%	0.070%
16	13.475	1758	1766	1771	rBV	16704	26788	0.65%	0.062%
17	14.051	1857	1864	1876	rBV	1756082	2338549	56.80%	5.394%
18	14.334	1905	1912	1928	rBV2	1919517	2781062	67.54%	6.414%
19	14.634	1956	1963	1972	rBV	1077942	1528508	37.12%	3.525%
20	14.869	1995	2003	2025	rBV	446590	845249	20.53%	1.950%
21	15.640	2124	2134	2143	rBV	2390197	3335165	81.00%	7.692%
22	15.704	2143	2145	2152	rVV8	5098	10486	0.25%	0.024%
23	15.775	2152	2157	2170	rVV	579439	799504	19.42%	1.844%
24	15.875	2170	2174	2181	rVB4	11576	20886	0.51%	0.048%
25	16.422	2266	2267	2273	rVB6	2941	4958	0.12%	0.011%
26	17.081	2375	2379	2384	rVB8	4399	7428	0.18%	0.017%
27	17.422	2430	2437	2448	rBV	1170219	1627684	39.53%	3.754%
28	17.522	2448	2454	2475	rVV	2466451	3454702	83.91%	7.968%
29	19.339	2759	2763	2770	rBV3	33059	51604	1.25%	0.119%
30	19.416	2772	2776	2780	rVB	22857	33471	0.81%	0.077%
31	19.775	2831	2837	2846	rBV	3319690	4107206	99.75%	9.473%
32	21.551	3134	3139	3146	rBV	1409373	1814934	44.08%	4.186%
33	23.957	3540	3548	3561	rVB2	2026600	4117361	100.00%	9.497%
34	24.121	3570	3576	3587	rVB	897712	1902728	46.21%	4.389%

Sum of corrected areas: 43356553




Instrument :
BNA_P
ClientSampleId :
SBLK906

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017494.D
Acq On : 03 Oct 2023 01:22
Operator : MA/JU
Sample : PB155906BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK906

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

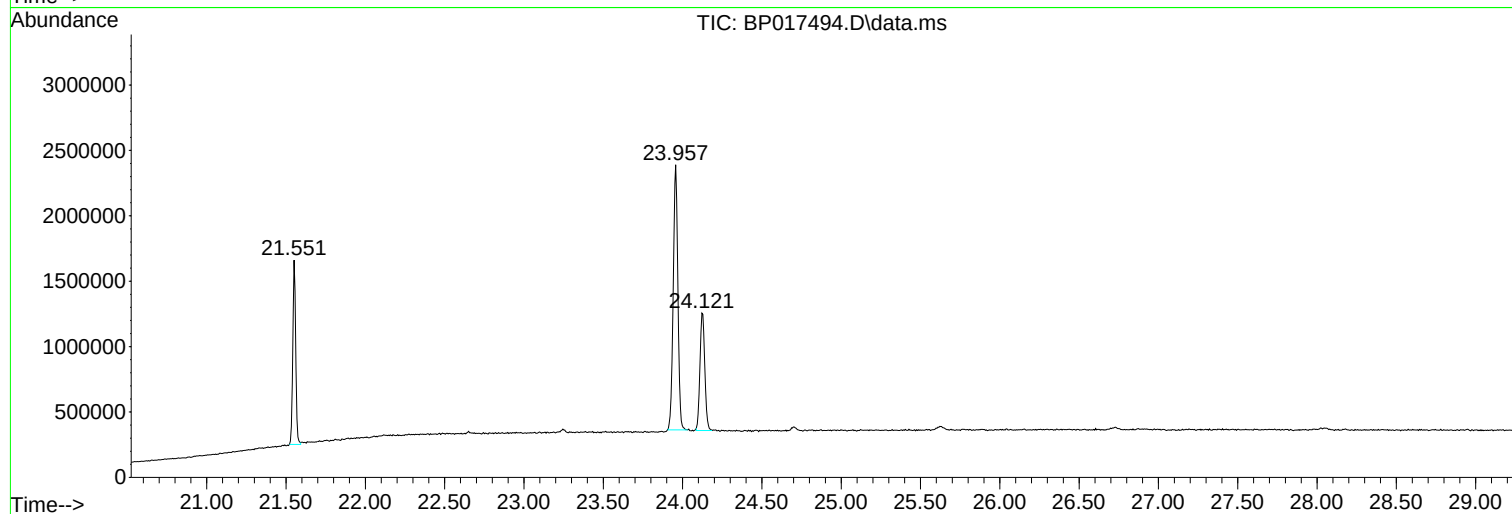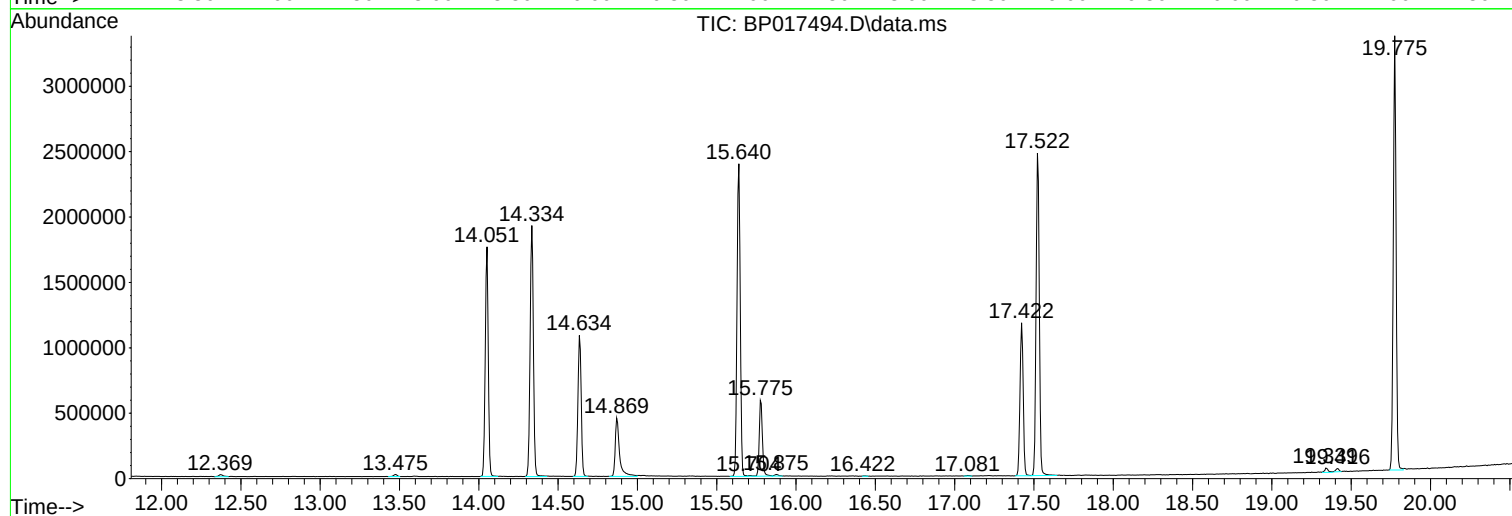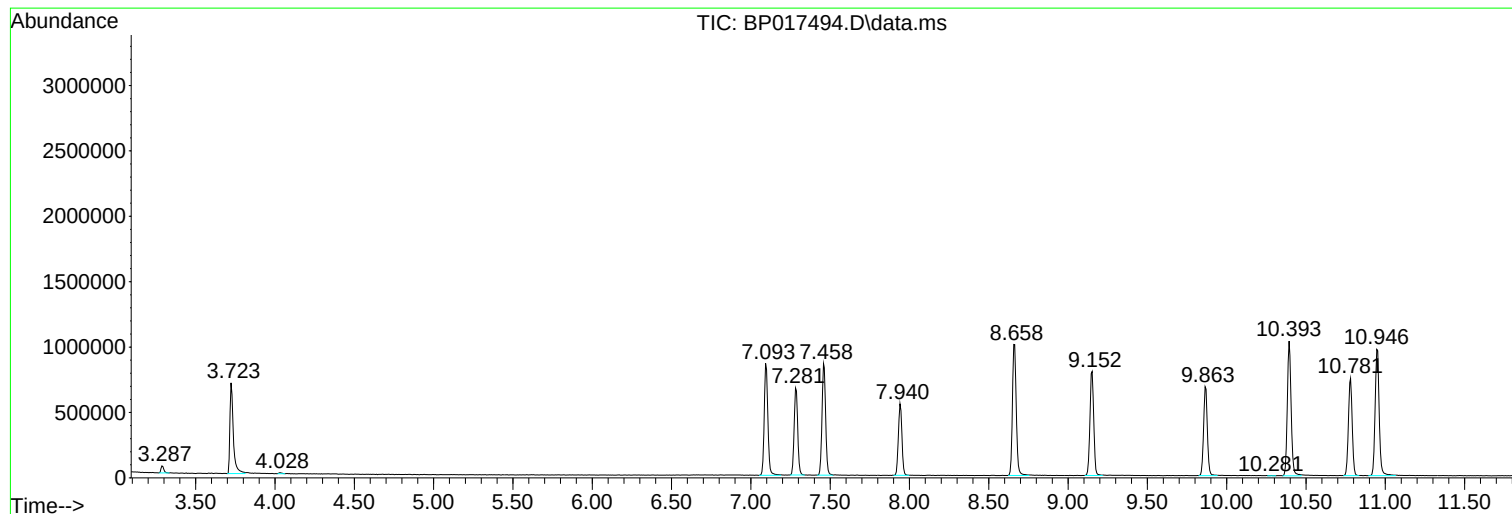

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017494.D
Acq On : 03 Oct 2023 01:22
Operator : MA/JU
Sample : PB155906BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK906

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017494.D
Acq On : 03 Oct 2023 01:22
Operator : MA/JU
Sample : PB155906BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK906

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc