

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
 Data File : BP017500.D
 Acq On : 03 Oct 2023 04:46
 Operator : MA/JU
 Sample : 04571-14
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJ17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017500.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	30	34	42	rVB	40556	54999	0.79%	0.098%
2	3.599	85	87	95	rVB4	5613	9311	0.13%	0.017%
3	3.728	105	109	120	rBV	209345	368478	5.29%	0.654%
4	3.911	135	140	148	rVB	42490	63224	0.91%	0.112%
5	4.028	156	160	163	rVB	11087	14312	0.21%	0.025%
6	4.169	180	184	193	rVB3	16173	24324	0.35%	0.043%
7	4.416	222	226	233	rVB3	11673	21199	0.30%	0.038%
8	4.546	245	248	252	rBV6	4693	7309	0.10%	0.013%
9	4.963	316	319	325	rBV	8250	12183	0.17%	0.022%
10	6.334	548	552	557	rVB2	12744	18750	0.27%	0.033%
11	6.899	644	648	652	rBV7	6018	8902	0.13%	0.016%
12	7.099	673	682	693	rBV	189586	334883	4.81%	0.595%
13	7.275	706	712	721	rBV	667923	1043556	14.98%	1.853%
14	7.457	736	743	754	rBV	723399	1140658	16.37%	2.025%
15	7.552	754	759	763	rVB6	4914	9726	0.14%	0.017%
16	7.934	817	824	836	rBV	683454	1055426	15.15%	1.874%
17	8.663	940	948	958	rBV	564442	933530	13.40%	1.658%
18	9.146	1022	1030	1043	rBV	866823	1426233	20.47%	2.533%
19	9.263	1047	1050	1058	rVV8	7771	17815	0.26%	0.032%
20	9.340	1058	1063	1071	rVB5	10343	21564	0.31%	0.038%
21	9.857	1141	1151	1165	rBV	713630	1199859	17.22%	2.131%
22	10.393	1233	1242	1259	rBV	1029613	1809921	25.98%	3.214%
23	10.775	1298	1307	1318	rBV	937127	1535672	22.04%	2.727%
24	10.946	1328	1336	1359	rBV	731352	1591203	22.84%	2.825%
25	11.834	1483	1487	1493	rBV7	4226	7448	0.11%	0.013%
26	12.363	1569	1577	1585	rVB2	19267	37135	0.53%	0.066%
27	13.375	1745	1749	1753	rBV4	10784	14090	0.20%	0.025%
28	13.475	1760	1766	1772	rVB	34849	58068	0.83%	0.103%
29	13.810	1817	1823	1827	rBV9	4263	8916	0.13%	0.016%
30	14.051	1856	1864	1875	rBV	2149964	2989536	42.91%	5.308%
31	14.175	1881	1885	1891	rBV8	4686	7862	0.11%	0.014%
32	14.334	1903	1912	1920	rBV	2404050	3536276	50.76%	6.279%
33	14.457	1930	1933	1938	rVB6	7507	10775	0.15%	0.019%
34	14.634	1955	1963	1970	rBV	1501181	2118592	30.41%	3.762%
35	14.898	2002	2008	2022	rBV2	110677	270640	3.88%	0.481%
36	15.081	2035	2039	2044	rVB8	5868	9800	0.14%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
 Data File : BP017500.D
 Acq On : 03 Oct 2023 04:46
 Operator : MA/JU
 Sample : 04571-14
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBJ17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

37	15.322	2077	2080	2084	rVB5	6755	7574	0.11%	0.013%
38	15.422	2094	2097	2100	rBV5	12437	13292	0.19%	0.024%
39	15.639	2127	2134	2143	rBV	3216315	4722861	67.79%	8.386%
40	15.775	2151	2157	2170	rBV	674299	944960	13.56%	1.678%
41	15.875	2170	2174	2182	rVB3	14763	26259	0.38%	0.047%
42	16.057	2203	2205	2211	rVB7	5477	7331	0.11%	0.013%
43	16.292	2243	2245	2252	rVV3	13183	21737	0.31%	0.039%
44	16.357	2252	2256	2259	rVB6	5149	7119	0.10%	0.013%
45	16.875	2340	2344	2346	rBV5	4731	7178	0.10%	0.013%
46	17.139	2387	2389	2396	rVB6	10413	14529	0.21%	0.026%
47	17.422	2431	2437	2448	rBV	1982943	2679176	38.46%	4.757%
48	17.522	2448	2454	2462	rBV	3991092	5691503	81.69%	10.106%
49	17.616	2467	2470	2474	rVB5	17305	20595	0.30%	0.037%
50	18.275	2578	2582	2588	rBV3	55951	105818	1.52%	0.188%
51	19.345	2760	2764	2768	rVB2	51692	66349	0.95%	0.118%
52	19.416	2772	2776	2779	rVB	43958	60363	0.87%	0.107%
53	19.780	2832	2838	2845	rBV	5300243	6966909	100.00%	12.371%
54	21.216	3080	3082	3093	rVB5	87904	154604	2.22%	0.275%
55	21.557	3135	3140	3148	rBV	2436572	3019101	43.33%	5.361%
56	23.974	3543	3551	3562	rVB2	3528025	6879115	98.74%	12.215%
57	24.145	3573	3580	3589	rVB	1465213	3107618	44.61%	5.518%




Sum of corrected areas: 56316166

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017500.D
Acq On : 03 Oct 2023 04:46
Operator : MA/JU
Sample : 04571-14
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ17

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

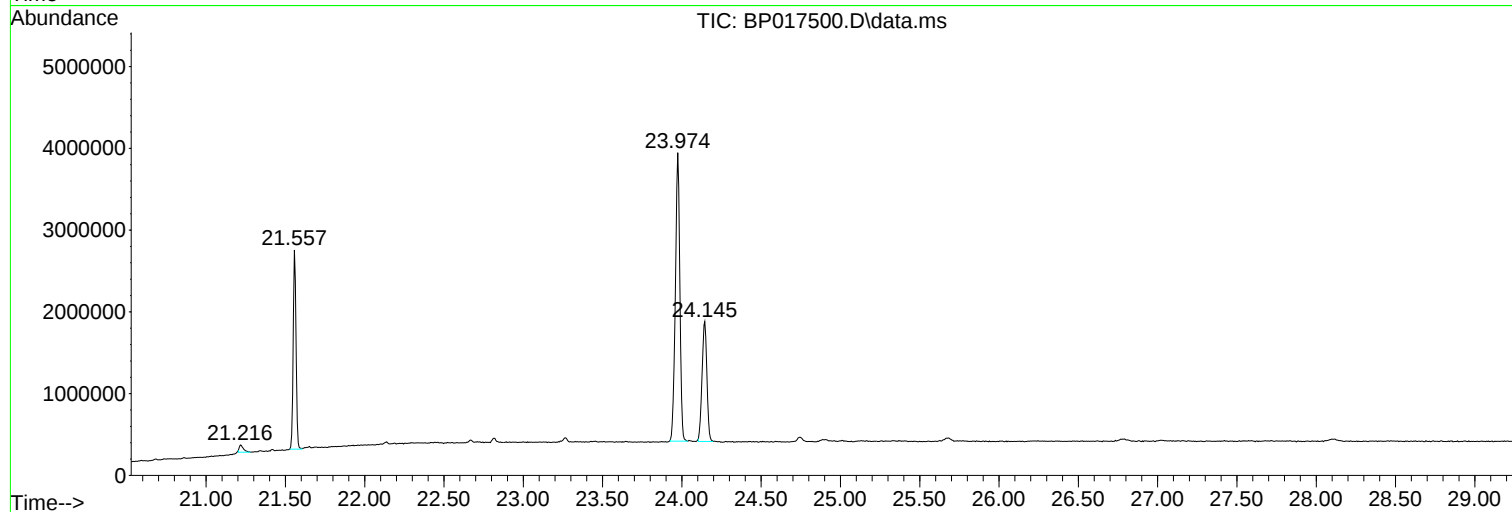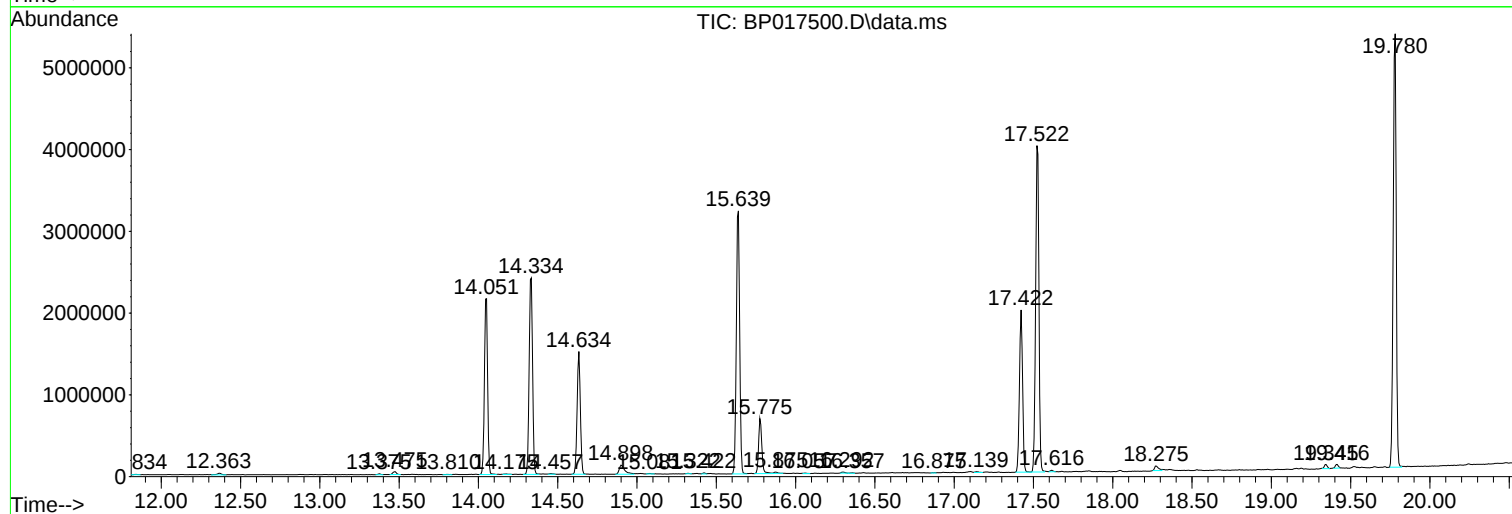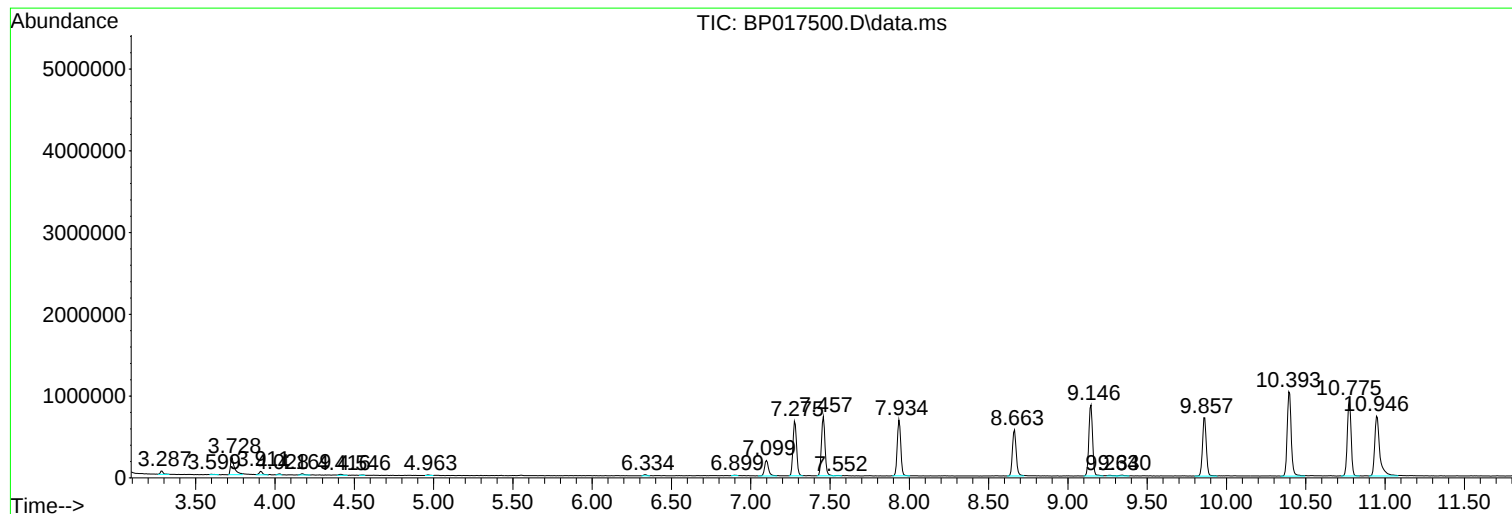

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017500.D
Acq On : 03 Oct 2023 04:46
Operator : MA/JU
Sample : 04571-14
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ17

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017500.D
Acq On : 03 Oct 2023 04:46
Operator : MA/JU
Sample : 04571-14
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBJ17

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc