

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
 Data File : BP017503.D
 Acq On : 03 Oct 2023 06:27
 Operator : MA/JU
 Sample : 04588-05
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017503.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	30	33	37	rBV	29983	37187	0.80%	0.092%
2	3.323	37	40	46	rVB	26634	34324	0.74%	0.085%
3	3.723	105	108	125	rBV	215889	340840	7.32%	0.842%
4	4.028	156	160	164	rVB	8586	11461	0.25%	0.028%
5	4.546	245	248	254	rVB7	5919	9167	0.20%	0.023%
6	7.093	675	681	691	rBV	142679	241460	5.18%	0.596%
7	7.275	705	712	726	rBV	596326	913523	19.61%	2.256%
8	7.458	734	743	755	rBV	564326	924754	19.85%	2.283%
9	7.564	755	761	764	rVB8	2590	6096	0.13%	0.015%
10	7.934	815	824	832	rBV	544076	835207	17.93%	2.062%
11	8.658	941	947	963	rBV	424415	695159	14.92%	1.716%
12	9.140	1023	1029	1036	rBV	715182	1142749	24.53%	2.821%
13	9.340	1059	1063	1068	rVB5	9794	14412	0.31%	0.036%
14	9.857	1143	1151	1162	rBV	557639	932844	20.02%	2.303%
15	10.393	1235	1242	1258	rBV	787135	1354667	29.07%	3.345%
16	10.775	1300	1307	1318	rVB	690526	1155924	24.81%	2.854%
17	10.946	1326	1336	1351	rBV	678987	1218284	26.15%	3.008%
18	11.793	1474	1480	1492	rBV2	64799	162478	3.49%	0.401%
19	12.363	1572	1577	1584	rVB2	14548	22094	0.47%	0.055%
20	13.375	1744	1749	1751	rBV6	3356	4778	0.10%	0.012%
21	13.475	1758	1766	1780	rBV	413988	667550	14.33%	1.648%
22	13.857	1827	1831	1834	rBV6	4675	5950	0.13%	0.015%
23	14.046	1855	1863	1870	rBV	1545998	2091118	44.88%	5.163%
24	14.328	1904	1911	1920	rBV	1771088	2534718	54.40%	6.258%
25	14.634	1955	1963	1970	rBV	1015829	1491798	32.02%	3.683%
26	14.898	2002	2008	2023	rBV2	60263	152175	3.27%	0.376%
27	15.016	2025	2028	2035	rVB9	4112	9494	0.20%	0.023%
28	15.634	2126	2133	2143	rBV	2355255	3202640	68.74%	7.907%
29	15.716	2143	2147	2151	rBV6	8370	11787	0.25%	0.029%
30	15.775	2151	2157	2165	rBV	522549	724594	15.55%	1.789%
31	15.875	2170	2174	2178	rVB5	10633	15466	0.33%	0.038%
32	16.475	2271	2276	2281	rBV7	4548	8369	0.18%	0.021%
33	16.651	2303	2306	2310	rBV2	9176	11108	0.24%	0.027%
34	16.763	2323	2325	2331	rVB7	5960	7559	0.16%	0.019%
35	17.087	2376	2380	2383	rBV6	4563	5733	0.12%	0.014%
36	17.204	2397	2400	2404	rBV5	4555	6949	0.15%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
 Data File : BP017503.D
 Acq On : 03 Oct 2023 06:27
 Operator : MA/JU
 Sample : 04588-05
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

37	17.422	2430	2437	2447	rBV	1318295	1829898	39.27%	4.518%
38	17.522	2447	2454	2466	rBV	2725879	3698153	79.37%	9.131%
39	17.681	2478	2481	2485	rBV6	3981	5355	0.11%	0.013%
40	18.051	2540	2544	2550	rBV8	10970	18287	0.39%	0.045%
41	18.269	2577	2581	2591	rBV	96093	164522	3.53%	0.406%
42	19.186	2734	2737	2742	rVB4	66561	73563	1.58%	0.182%
43	19.339	2760	2763	2767	rVB3	32842	38507	0.83%	0.095%
44	19.410	2771	2775	2780	rVV2	80808	102001	2.19%	0.252%
45	19.510	2789	2792	2801	rBV2	60856	103520	2.22%	0.256%
46	19.775	2831	2837	2846	rBV	3661878	4557018	97.80%	11.251%
47	21.557	3135	3140	3146	rBV2	1652131	2084315	44.73%	5.146%
48	23.969	3542	3550	3561	rBV2	2322083	4659304	100.00%	11.504%
49	24.139	3572	3579	3587	rVB	1051145	2162698	46.42%	5.340%




Sum of corrected areas: 40501557

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017503.D
Acq On : 03 Oct 2023 06:27
Operator : MA/JU
Sample : 04588-05
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHP4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

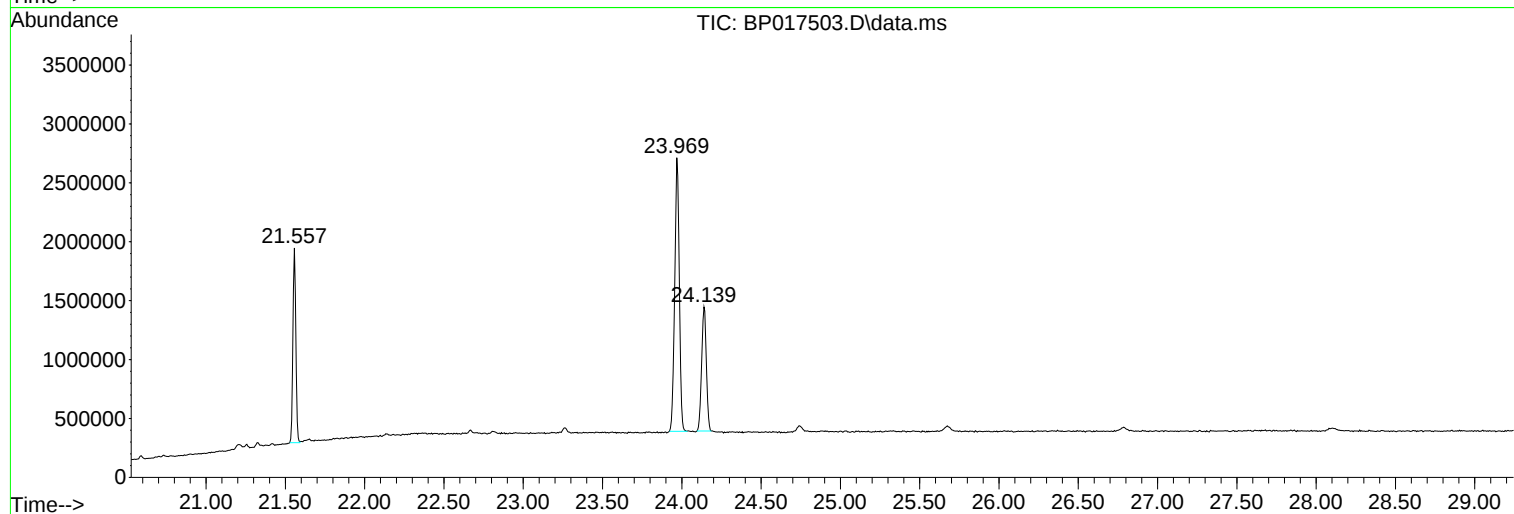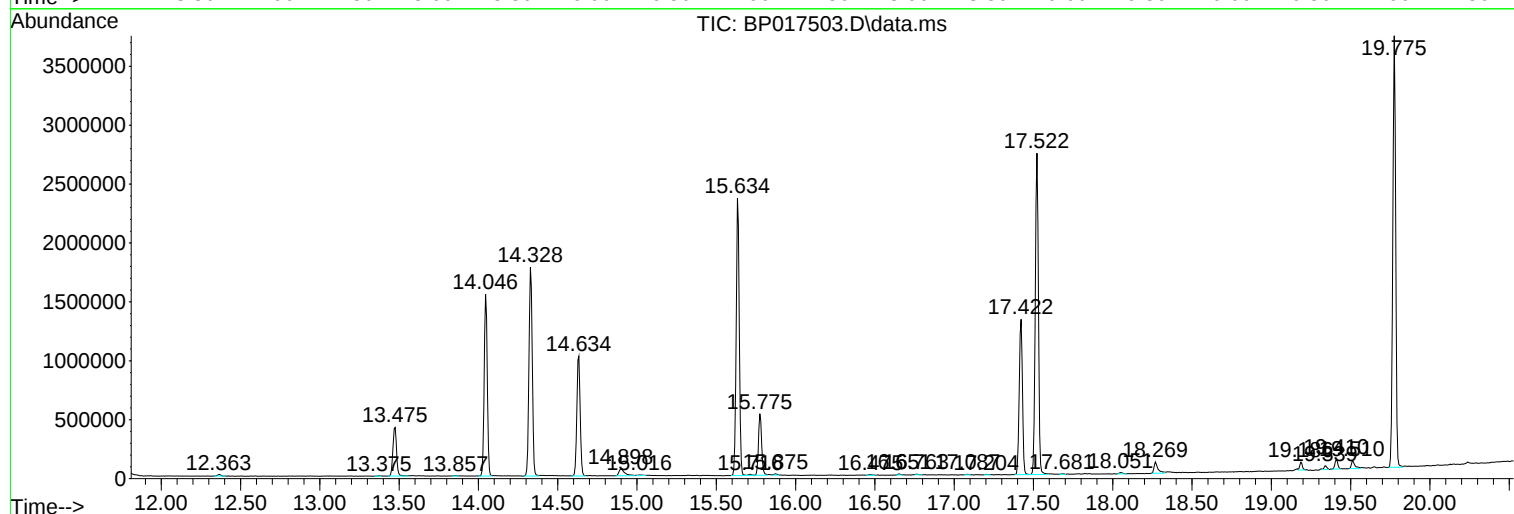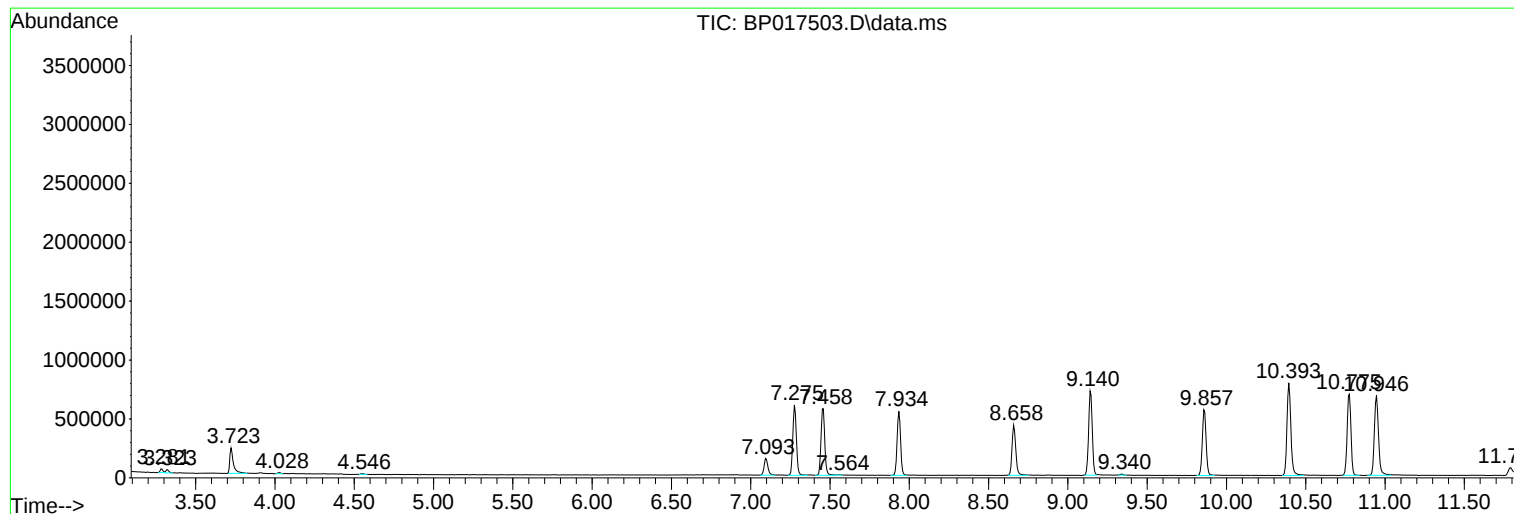

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017503.D
Acq On : 03 Oct 2023 06:27
Operator : MA/JU
Sample : 04588-05
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHP4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2,4,7,9-Tetramethyl-5-decyn... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.475	8.95 ng/ul	667550	Acenaphthene-d10	14.634

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2,4,7,9-Tetramethyl-5-decyn-4,7-...	226	C14H26O2	000126-86-3	91		
2	2,4,7,9-Tetramethyl-5-decyn-4,7-...	226	C14H26O2	000126-86-3	91		
3	Metacetamol	151	C8H9NO2	000621-42-1	64		
4	3-Pyridinol, 4-methyl-, acetate ...	151	C8H9NO2	001006-96-8	59		
5	Pyridine, 2-butyl-, 1-oxide	151	C9H13NO	031396-32-4	59		

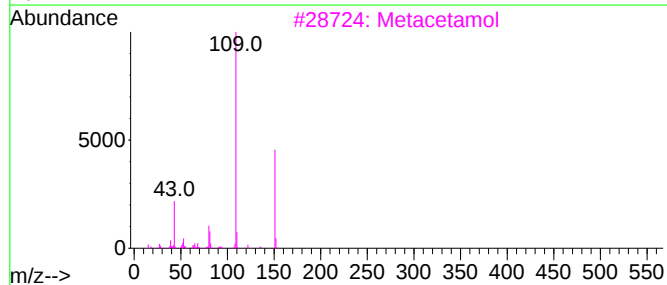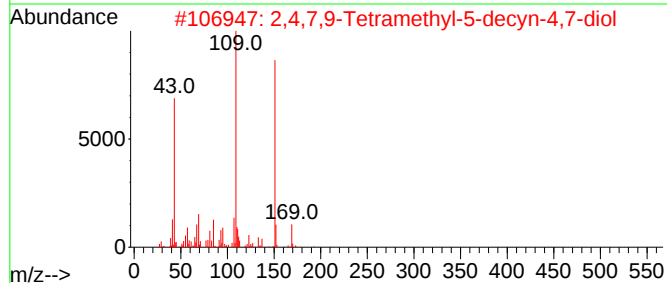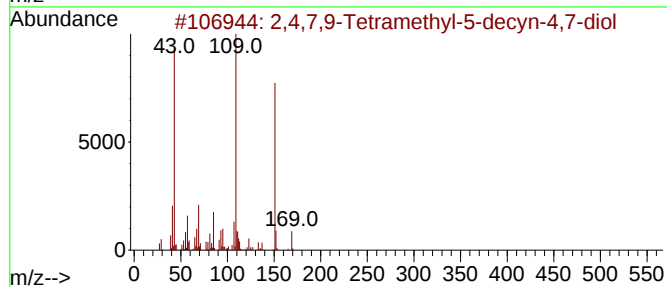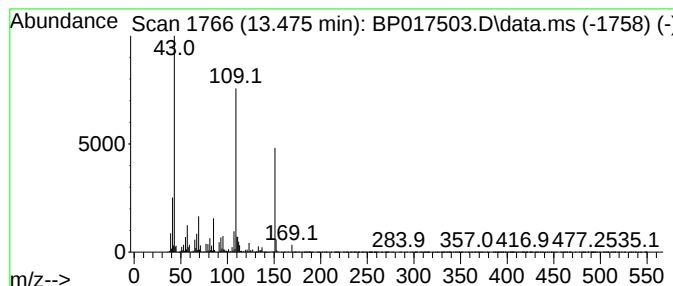

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017503.D
Acq On : 03 Oct 2023 06:27
Operator : MA/JU
Sample : 04588-05
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHP4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2,4,7,9-Tetrame...	13.475	8.9	ng/ul	667550	3	14.634	1491800	20.0