

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
 Data File : BP017523.D
 Acq On : 03 Oct 2023 18:40
 Operator : MA/JU
 Sample : 04588-04
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBHS6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017523.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	30	33	38	rVB	31389	40783	0.17%	0.060%
2	3.722	105	108	124	rBV	263132	412663	1.69%	0.603%
3	4.552	242	249	267	rBV	15227254	24431588	100.00%	35.696%
4	7.093	675	681	696	rBV	201658	339234	1.39%	0.496%
5	7.275	706	712	720	rBV	710630	1119432	4.58%	1.636%
6	7.458	736	743	755	rVB	744011	1183433	4.84%	1.729%
7	7.934	817	824	835	rBV	604347	942151	3.86%	1.377%
8	8.657	940	947	957	rBV	568377	935508	3.83%	1.367%
9	9.146	1019	1030	1043	rBV	889326	1479806	6.06%	2.162%
10	9.857	1143	1151	1164	rBV	746606	1232452	5.04%	1.801%
11	10.393	1233	1242	1258	rBV	1021922	1779078	7.28%	2.599%
12	10.775	1299	1307	1315	rBV	800744	1333410	5.46%	1.948%
13	10.946	1326	1336	1349	rBV	907889	1550442	6.35%	2.265%
14	12.369	1573	1578	1583	rVB	18545	29236	0.12%	0.043%
15	14.045	1856	1863	1876	rBV	1871521	2587300	10.59%	3.780%
16	14.328	1904	1911	1926	rBV	2167905	3118592	12.76%	4.556%
17	14.634	1956	1963	1975	rVB	1115953	1636487	6.70%	2.391%
18	14.892	2001	2007	2021	rBV2	85481	201649	0.83%	0.295%
19	15.634	2127	2133	2142	rBV	2632476	3690913	15.11%	5.393%
20	15.775	2151	2157	2168	rBV	575201	786481	3.22%	1.149%
21	17.422	2430	2437	2443	rBV	1274129	1760272	7.20%	2.572%
22	17.522	2447	2454	2463	rBV	2825117	3896797	15.95%	5.693%
23	18.269	2577	2581	2591	rBV2	58330	99791	0.41%	0.146%
24	19.339	2760	2763	2767	rVB2	33380	37037	0.15%	0.054%
25	19.410	2773	2775	2780	rVB	34760	37793	0.15%	0.055%
26	19.516	2789	2793	2799	rBV7	34039	55843	0.23%	0.082%
27	19.775	2831	2837	2843	rBV	3847795	4723007	19.33%	6.901%
28	21.557	3135	3140	3146	rBV	1496848	1961102	8.03%	2.865%
29	23.968	3542	3550	3560	rVB2	2342095	5011893	20.51%	7.323%
30	24.133	3572	3578	3587	rVB	964445	2029694	8.31%	2.965%




Sum of corrected areas: 68443867

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017523.D
Acq On : 03 Oct 2023 18:40
Operator : MA/JU
Sample : 04588-04
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHS6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

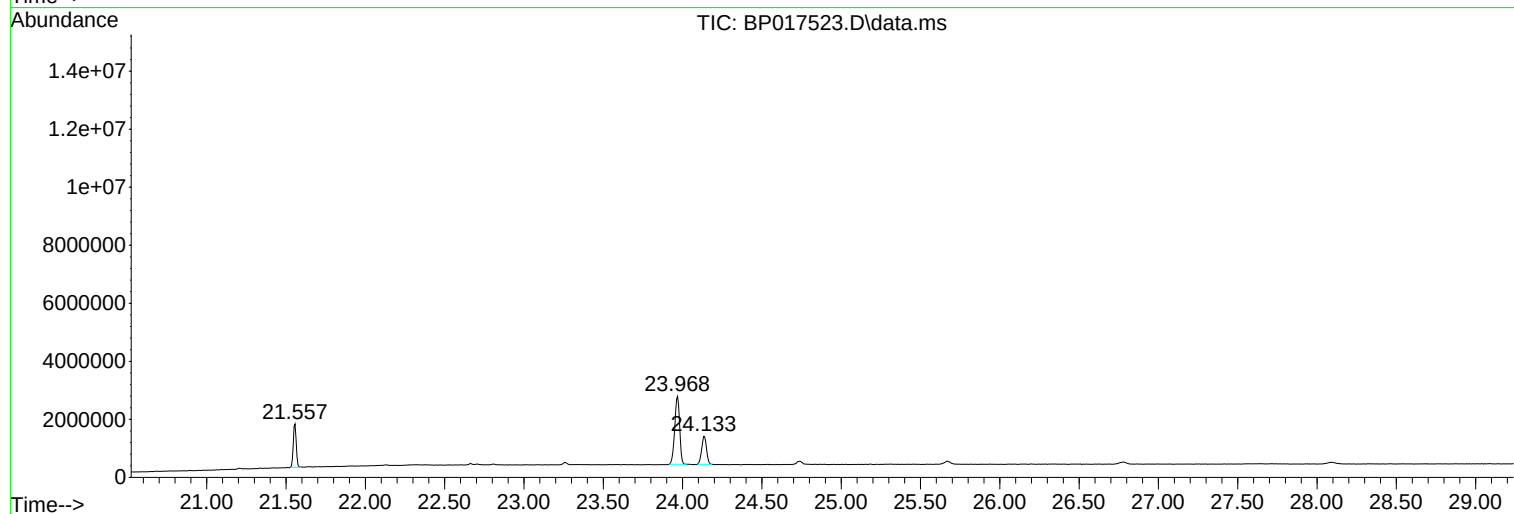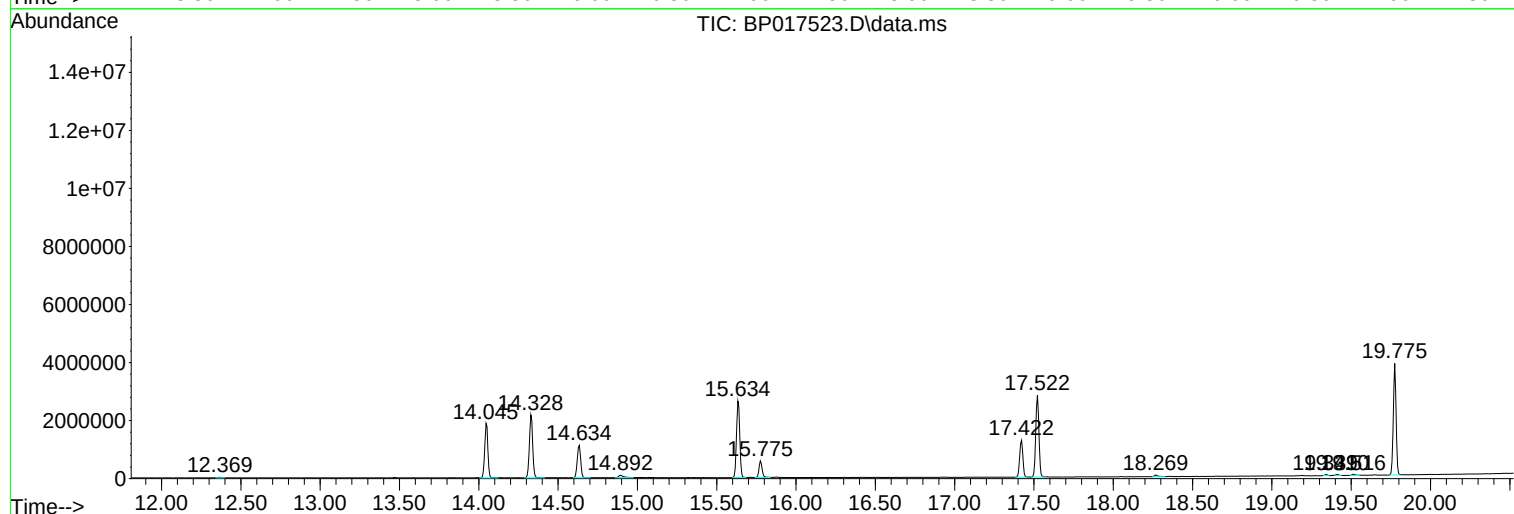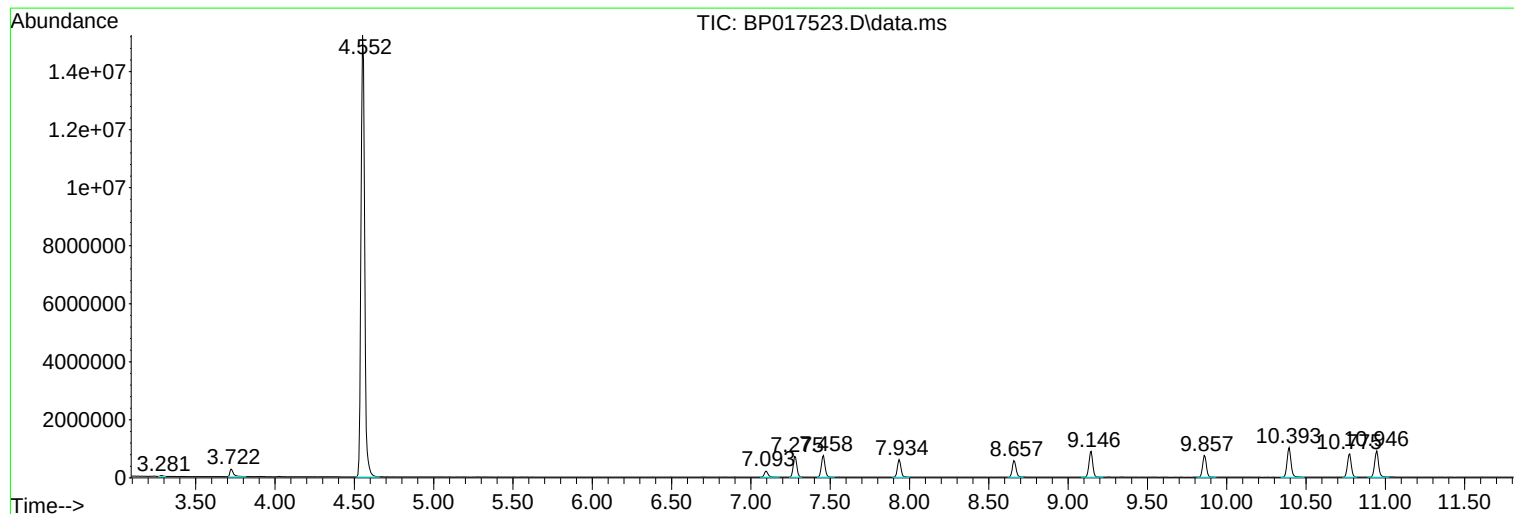

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017523.D
Acq On : 03 Oct 2023 18:40
Operator : MA/JU
Sample : 04588-04
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHS6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.552	518.63 ng/ul	24431600	1,4-Dichlorobenzene-d4	7.934

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	99
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	38

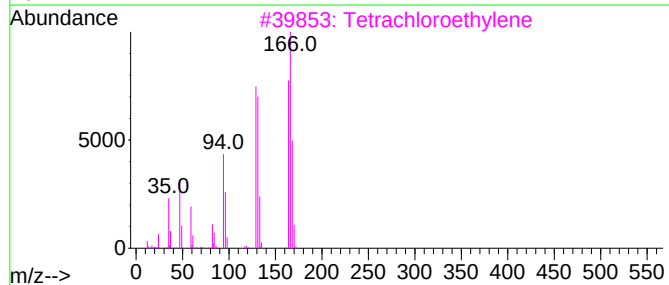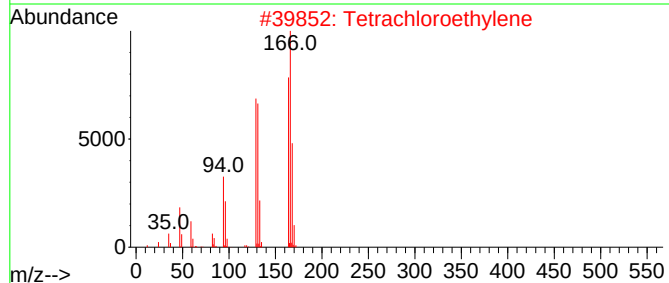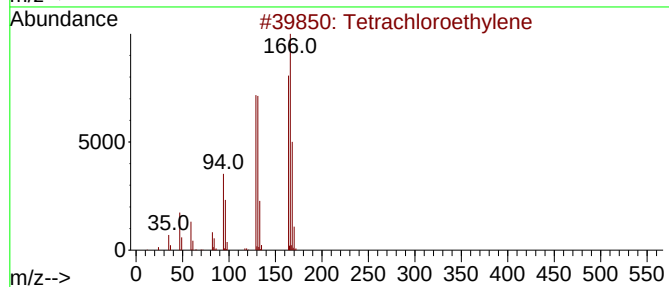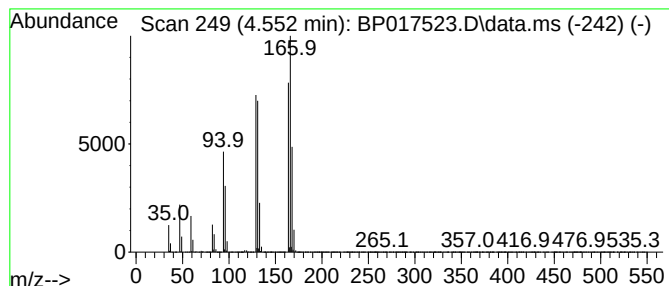

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100223\
Data File : BP017523.D
Acq On : 03 Oct 2023 18:40
Operator : MA/JU
Sample : 04588-04
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBHS6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP092023.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.552	518.6	ng/ul	24431600	1	7.934	942151	20.0