


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP100319\
 Data File : BP000490.D
 Acq On : 03 Oct 2019 12:44
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 01 18:03:42 2019

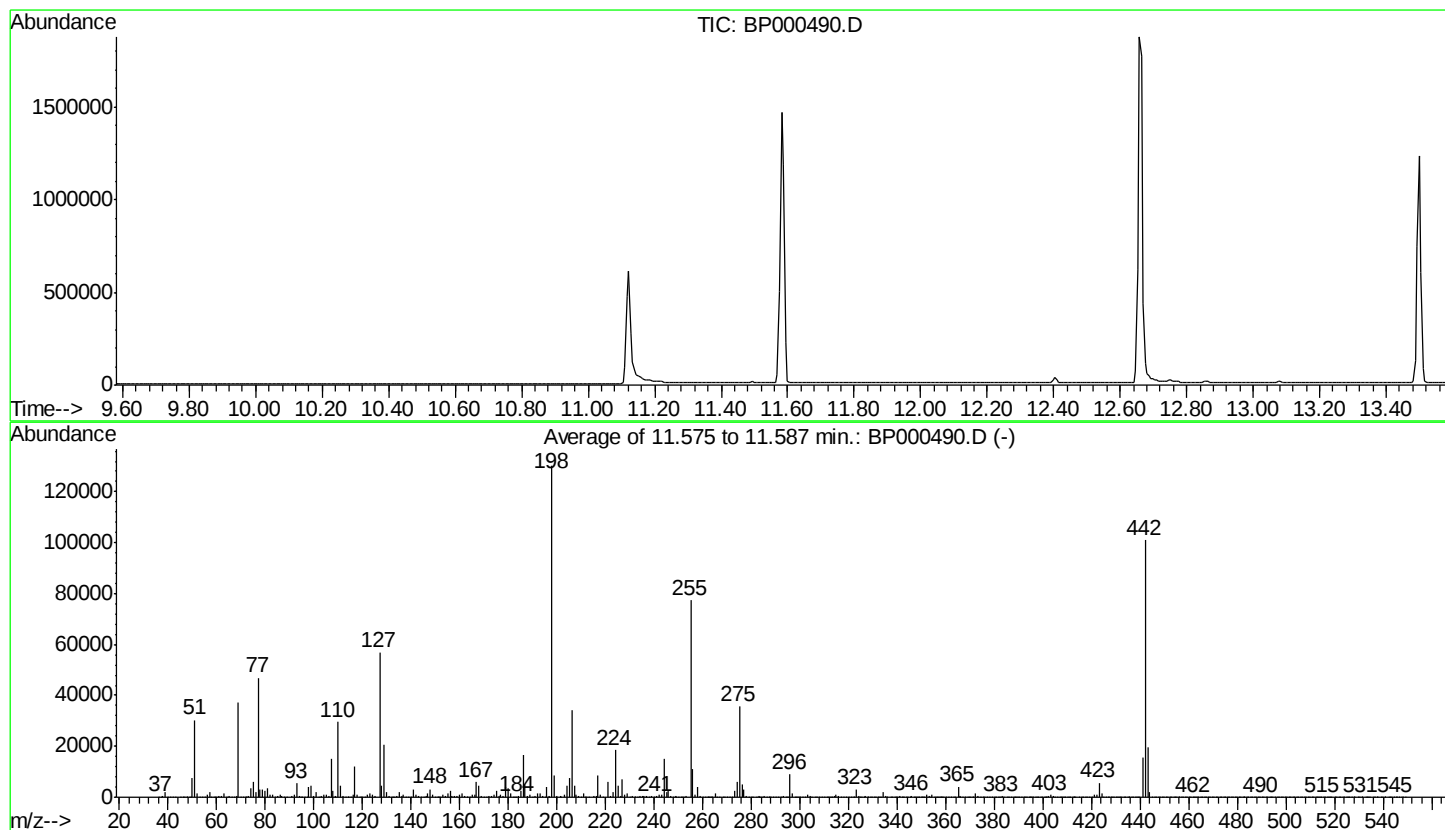

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.2	30281	PASS
68	69	0.00	2	2.0	743	PASS
69	198	0.00	100	28.5	37154	PASS
70	69	0.00	2	0.6	210	PASS
127	198	10	80	43.6	56765	PASS
197	198	0.00	2	0.3	363	PASS
198	198	100	100	100.0	130269	PASS
199	198	5	9	6.7	8666	PASS
275	198	10	60	27.4	35683	PASS
365	198	1	100	3.1	4052	PASS
441	198	0.01	100	12.1	15706	PASS
442	198	50	100	77.5	100983	PASS
443	442	15	24	19.4	19607	PASS