

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
 Data File : BP011871.D
 Acq On : 03 Oct 2022 14:33
 Operator : CG/JU
 Sample : N4859-09
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E10049

Quant Time: Oct 03 23:31:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 01 00:53:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.892	152	244821	20.000	ng/ul	0.00
20) Naphthalene-d8	10.698	136	970389	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.539	164	552176	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.292	188	1105306	20.000	ng/ul	0.00
79) Chrysene-d12	21.374	240	1229818	20.000	ng/ul	-0.01
88) Perylene-d12	23.809	264	1333629	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.304	96	24291	4.376	ng/uL	0.00
4) Pyridine-d5	3.734	84	132517	8.150	ng/ul	0.00
7) Phenol-d5	7.057	99	111740	5.287	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	298145	25.449	ng/ul	0.00
11) 2-Chlorophenol-d4	7.422	132	342083	20.503	ng/ul	0.00
15) 4-Methylphenol-d8	8.604	113	205166	11.743	ng/ul	0.00
21) Nitrobenzene-d5	9.057	128	206880	27.990	ng/ul	0.00
24) 2-Nitrophenol-d4	9.781	143	200578	25.364	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	337373	23.065	ng/ul	0.00
31) 4-Chloroaniline-d4	10.839	131	481452	21.591	ng/ul	0.00
46) Dimethylphthalate-d6	13.945	166	1140727	28.889	ng/ul	0.00
49) Acenaphthylene-d8	14.227	160	1272940	28.278	ng/ul	0.00
54) 4-Nitrophenol-d4	14.745	143	30155	3.688	ng/ul	0.00
60) Fluorene-d10	15.533	176	1007332	29.375	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	145219	21.707	ng/ul	0.00
73) Anthracene-d10	17.392	188	1668803	33.145	ng/ul	0.00
81) Pyrene-d10	19.627	212	2077733	33.359	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.650	264	2304589	34.521	ng/ul	-0.01
Target Compounds						
52) Acenaphthene	14.604	153	83408	2.365	ng/ul	98
82) Pyrene	19.651	202	86563	1.091	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011871.D
Acq On : 03 Oct 2022 14:33
Operator : CG/JU
Sample : N4859-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10049

Quant Time: Oct 03 23:31:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 01 00:53:59 2022
Response via : Initial Calibration




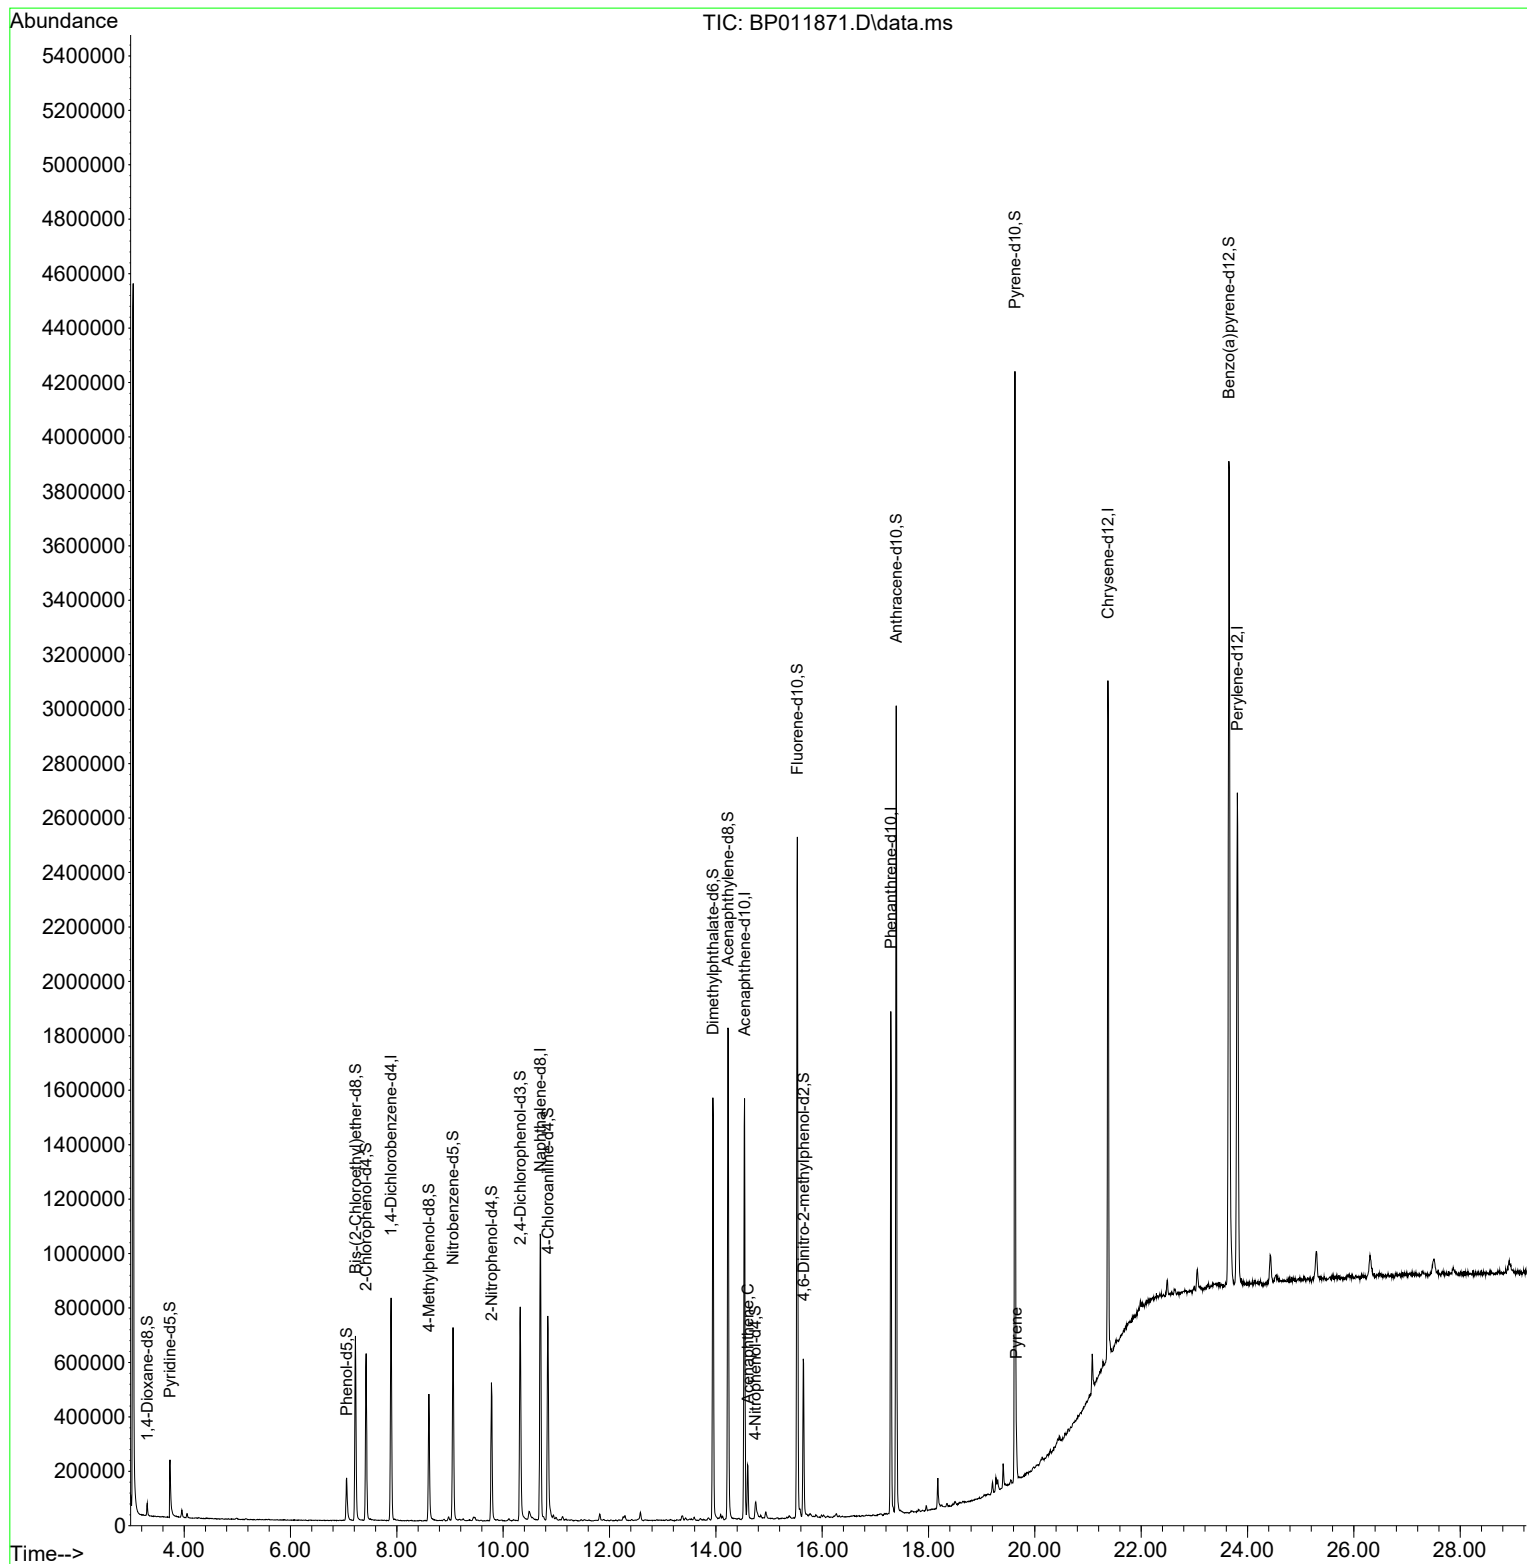


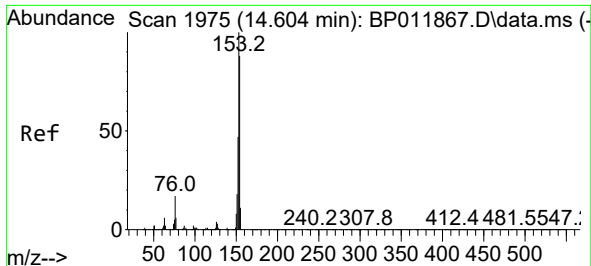

#52
Acenaphthene
Concen: 2.365 ng/ul
RT: 14.604 min Scan# 1975
Delta R.T. -0.000 min
Lab File: BP011871.D
Acq: 03 Oct 2022 14:33

Instrument :
BNA_P
ClientSampleId :
E10049

Tgt Ion:153 Resp: 83408
Ion Ratio Lower Upper
153 100
152 47.8 38.4 57.6
154 85.0 70.6 105.8

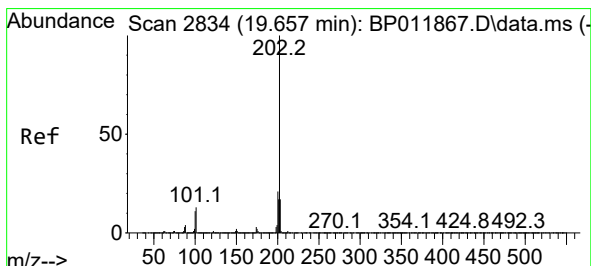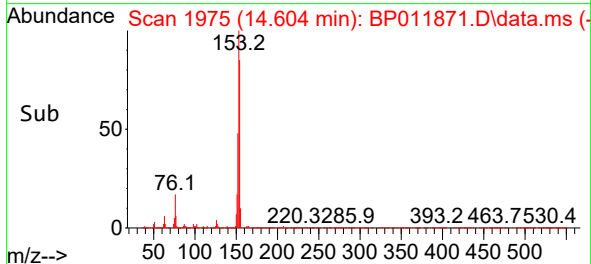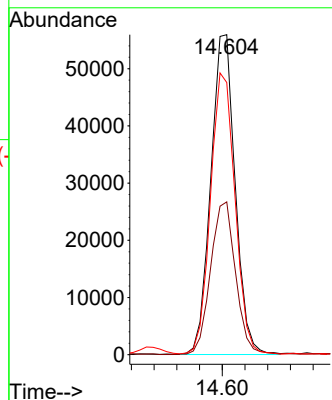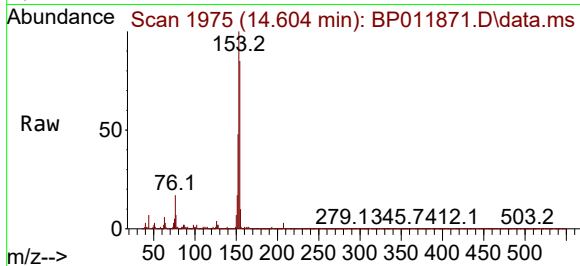

#82
Pyrene
Concen: 1.091 ng/ul
RT: 19.651 min Scan# 2833
Delta R.T. -0.006 min
Lab File: BP011871.D
Acq: 03 Oct 2022 14:33

Tgt Ion:202 Resp: 86563
Ion Ratio Lower Upper
202 100
101 15.0 11.6 17.4
100 11.2 9.4 14.0

