

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
 Data File : BP011872.D
 Acq On : 03 Oct 2022 15:07
 Operator : CG/JU
 Sample : N4749-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8Q1

Quant Time: Oct 03 23:31:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 01 00:53:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	287632	20.000	ng/ul	0.00
20) Naphthalene-d8	10.699	136	1141835	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.534	164	616111	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.292	188	1173703	20.000	ng/ul	0.00
79) Chrysene-d12	21.374	240	1207753	20.000	ng/ul	-0.01
88) Perylene-d12	23.810	264	1324281	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	31170	4.779	ng/uL	0.00
4) Pyridine-d5	3.734	84	139166	7.285	ng/ul	0.00
7) Phenol-d5	7.058	99	171494	6.906	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	392873	28.544	ng/ul	0.00
11) 2-Chlorophenol-d4	7.422	132	465544	23.750	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	289580	14.107	ng/ul	0.00
21) Nitrobenzene-d5	9.057	128	276041	31.739	ng/ul	0.00
24) 2-Nitrophenol-d4	9.781	143	279226	30.008	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	473023	27.483	ng/ul	0.00
31) 4-Chloroaniline-d4	10.840	131	410878	15.659	ng/ul	0.00
46) Dimethylphthalate-d6	13.945	166	1530290	34.733	ng/ul	0.00
49) Acenaphthylene-d8	14.228	160	1708163	34.009	ng/ul	0.00
54) 4-Nitrophenol-d4	14.740	143	51377	5.631	ng/ul	0.00
60) Fluorene-d10	15.534	176	1325106	34.632	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	201249	28.329	ng/ul	0.00
73) Anthracene-d10	17.392	188	2108463	39.437	ng/ul	0.00
81) Pyrene-d10	19.628	212	2496205	40.810	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.651	264	2754882	41.557	ng/ul	-0.01
Target Compounds						
59) Diethylphthalate	15.357	149	95119	2.056	ng/ul	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011872.D
Acq On : 03 Oct 2022 15:07
Operator : CG/JU
Sample : N4749-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8Q1

Quant Time: Oct 03 23:31:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 01 00:53:59 2022
Response via : Initial Calibration

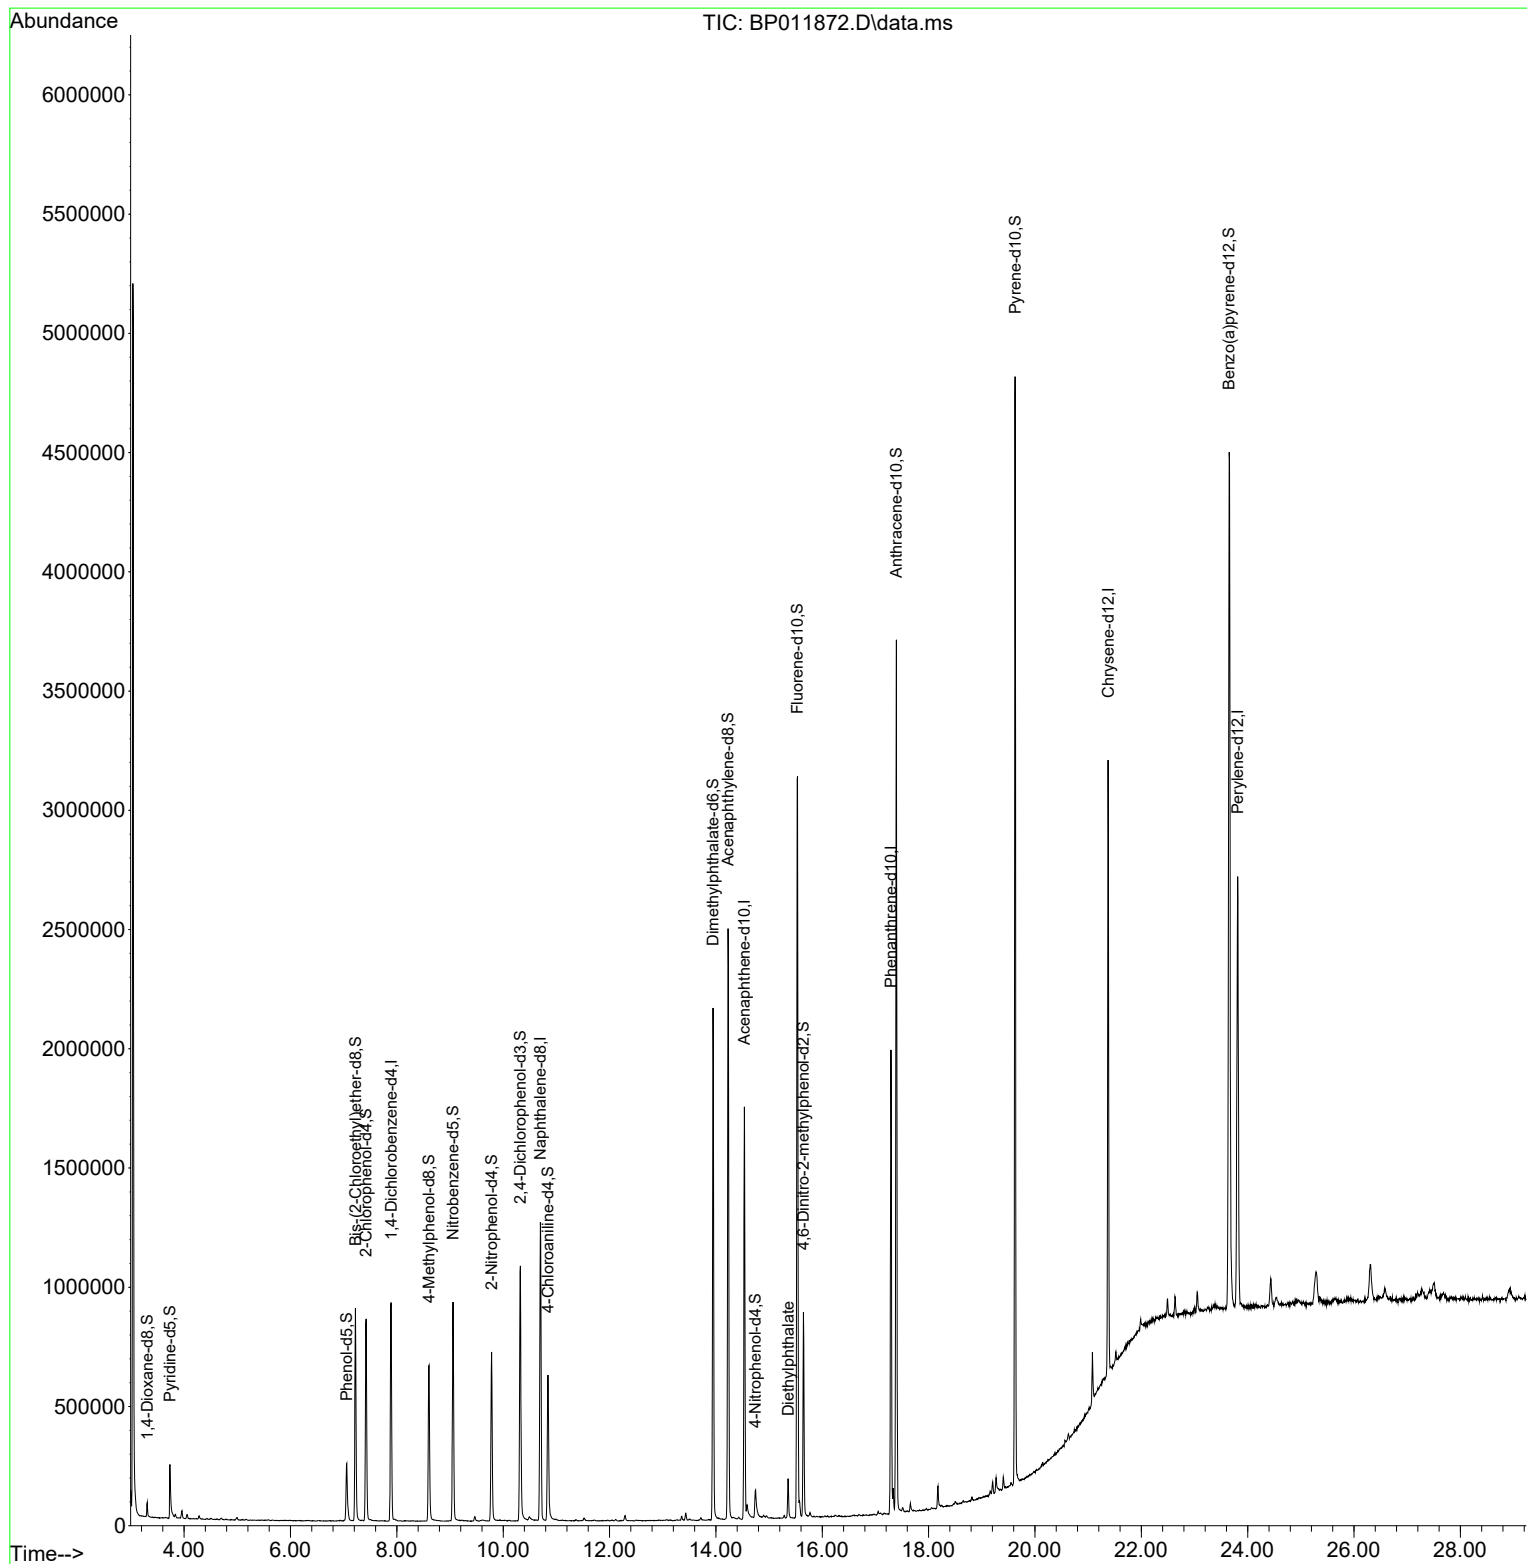

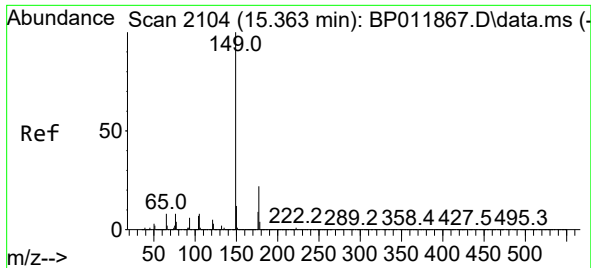

#59

Diethylphthalate

Concen: 2.056 ng/ul

RT: 15.357 min Scan# 2103

Delta R.T. -0.006 min

Lab File: BP011872.D


Acq: 03 Oct 2022 15:07

Instrument :

BNA_P

ClientSampleId :

CB8Q1

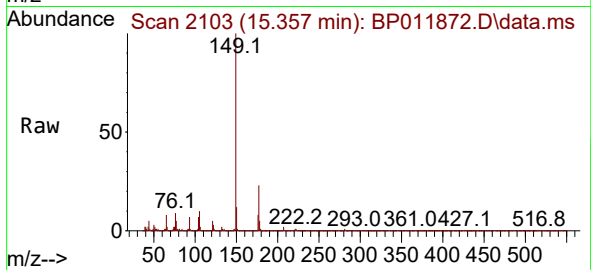

Tgt Ion:149 Resp: 95119

Ion Ratio Lower Upper

149 100

177 22.6 17.8 26.8

150 12.4 9.9 14.9

