

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
 Data File : BP011908.D
 Acq On : 04 Oct 2022 12:43
 Operator : CG/JU
 Sample : N4873-09
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXZ55

Quant Time: Oct 05 04:40:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 01 00:53:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	254313	20.000	ng/u1	0.00
20) Naphthalene-d8	10.693	136	1023103	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.534	164	590787	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.286	188	1237162	20.000	ng/u1	-0.01
79) Chrysene-d12	21.374	240	1295566	20.000	ng/u1	-0.01
88) Perylene-d12	23.810	264	1310474	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	28614	4.962	ng/uL	0.00
4) Pyridine-d5	3.728	84	135552	8.025	ng/u1	0.00
7) Phenol-d5	7.046	99	129349	5.892	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.216	67	360206	29.599	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.416	132	398025	22.966	ng/u1	0.00
15) 4-Methylphenol-d8	8.599	113	238217	13.126	ng/u1	0.00
21) Nitrobenzene-d5	9.052	128	244581	31.385	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.775	143	240325	28.825	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.316	165	409043	26.524	ng/u1	0.00
31) 4-Chloroaniline-d4	10.834	131	583422	24.815	ng/u1	-0.01
46) Dimethylphthalate-d6	13.945	166	1368566	32.394	ng/u1	0.00
49) Acenaphthylene-d8	14.228	160	1557208	32.333	ng/u1	0.00
54) 4-Nitrophenol-d4	14.745	143	35869	4.100	ng/u1	0.00
60) Fluorene-d10	15.528	176	1254467	34.191	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	181003	24.172	ng/u1	0.00
73) Anthracene-d10	17.386	188	2078380	36.880	ng/u1	-0.01
81) Pyrene-d10	19.622	212	2541032	38.727	ng/u1	-0.01
92) Benzo(a)pyrene-d12	23.651	264	2557524	38.986	ng/u1	-0.01


Target Compounds					Qvalue
2) 1,4-Dioxane	3.334	88	13109	2.105	ng/uL 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011908.D
Acq On : 04 Oct 2022 12:43
Operator : CG/JU
Sample : N4873-09
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXZ55

Quant Time: Oct 05 04:40:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 01 00:53:59 2022
Response via : Initial Calibration

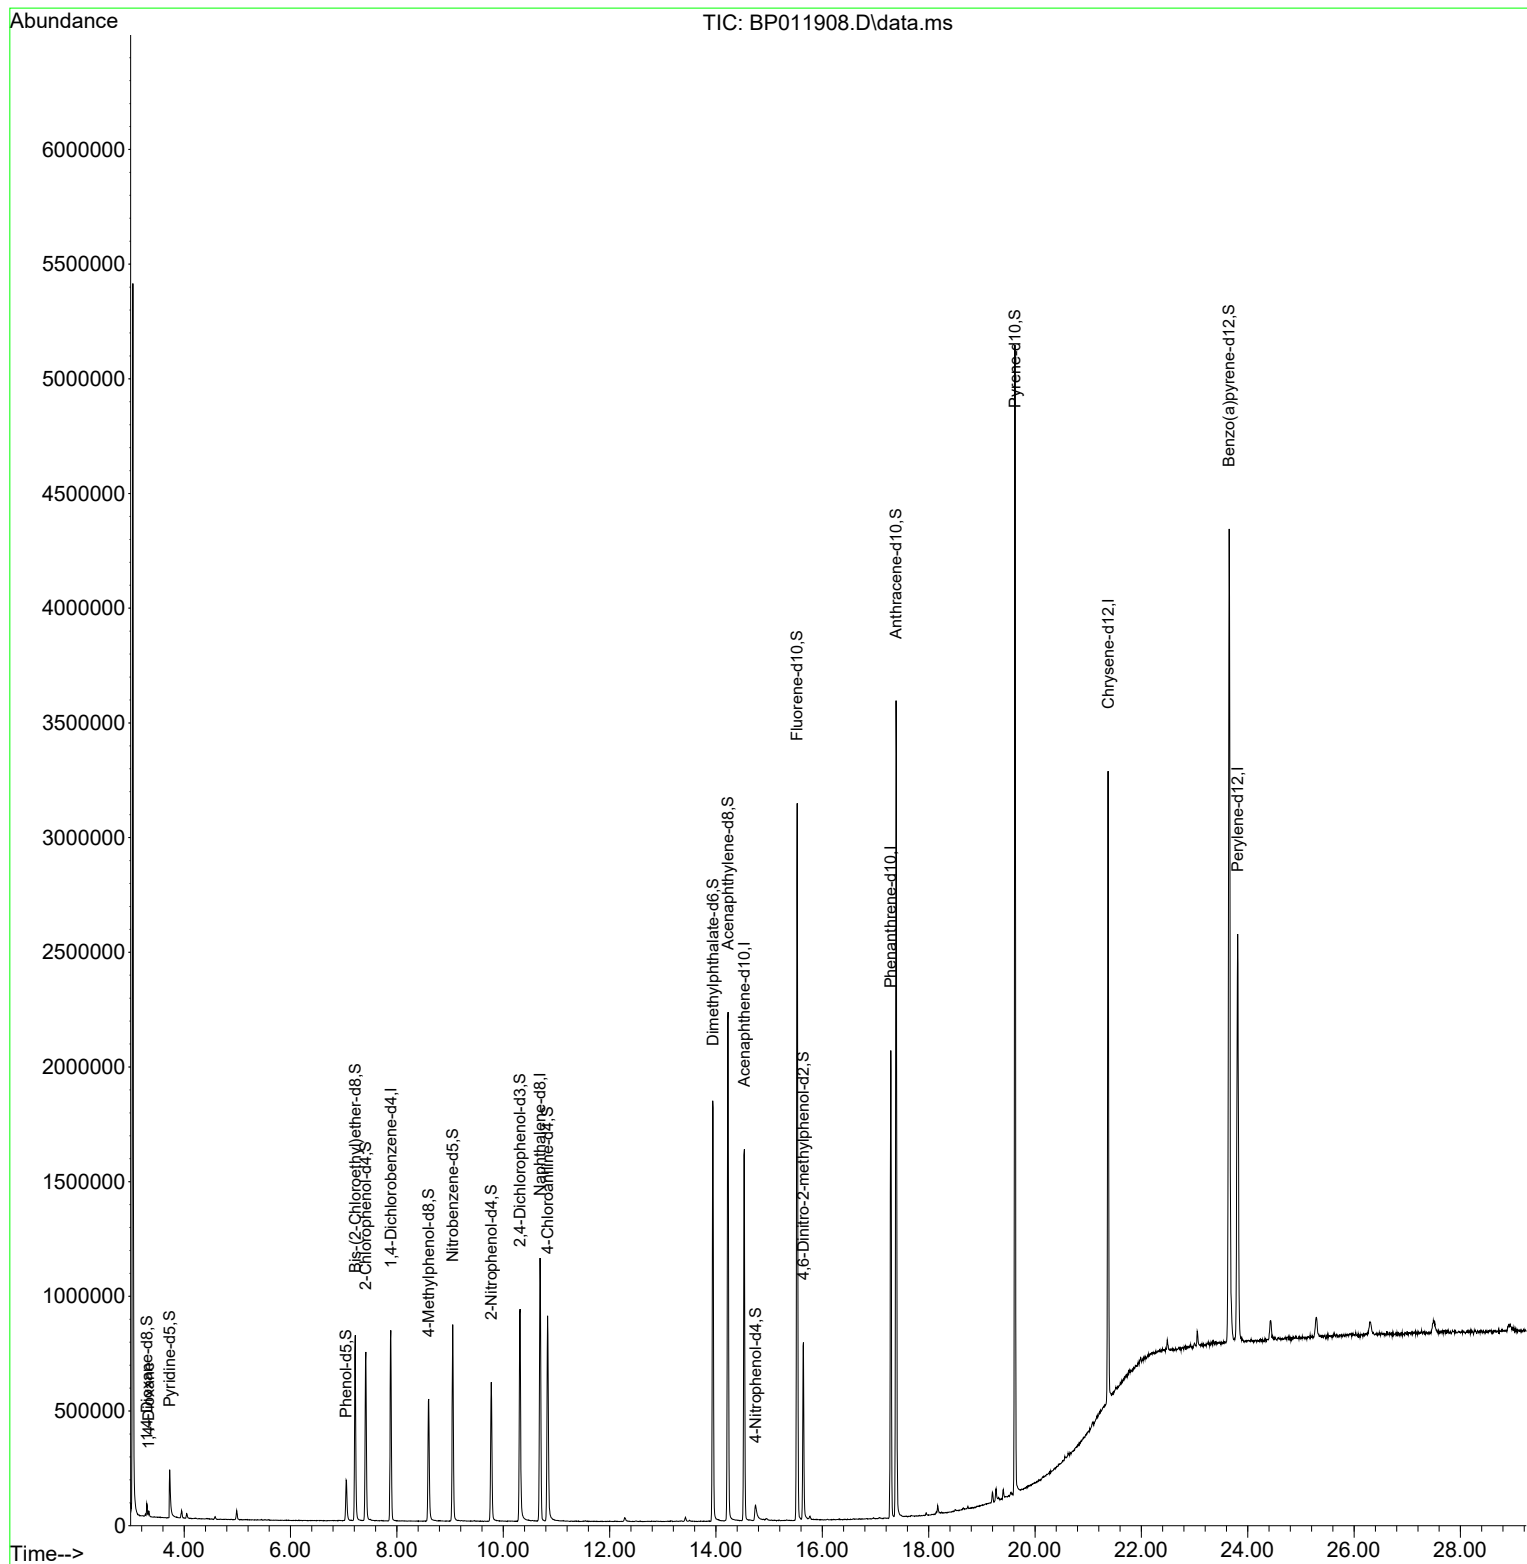

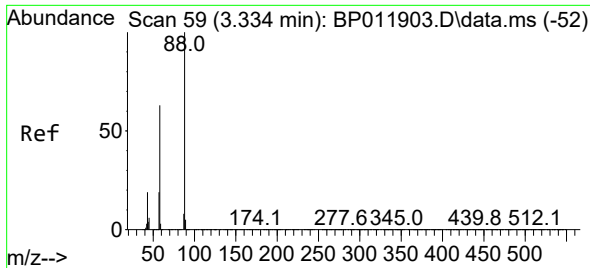

#2
 1,4-Dioxane
 Concen: 2.105 ng/uL
 RT: 3.334 min Scan# 51
 Delta R.T. -0.006 min
 Lab File: BP011908.D
 Acq: 04 Oct 2022 12:43

Instrument :
 BNA_P
 ClientSampleId :
 EXZ55

Tgt Ion: 88 Resp: 13109
 Ion Ratio Lower Upper
 88 100
 43 20.0 15.6 23.4
 58 63.9 48.6 72.8

