

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
 Data File : BP011910.D
 Acq On : 04 Oct 2022 13:52
 Operator : CG/JU
 Sample : N4873-13
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXZ58

Quant Time: Oct 05 04:45:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 01 00:53:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	234003	20.000	ng/u1	0.00
20) Naphthalene-d8	10.693	136	932232	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.534	164	520027	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.286	188	1062217	20.000	ng/u1	-0.01
79) Chrysene-d12	21.374	240	1142769	20.000	ng/u1	-0.01
88) Perylene-d12	23.810	264	1185847	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	24992	4.710	ng/uL	0.00
4) Pyridine-d5	3.734	84	73680	4.741	ng/u1	0.00
7) Phenol-d5	7.046	99	109733	5.432	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.216	67	316353	28.252	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.416	132	354478	22.228	ng/u1	0.00
15) 4-Methylphenol-d8	8.593	113	198811	11.905	ng/u1	-0.01
21) Nitrobenzene-d5	9.051	128	212061	29.865	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.775	143	207682	27.337	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.310	165	352393	25.078	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.834	131	435334	20.322	ng/u1	-0.01
46) Dimethylphthalate-d6	13.939	166	1139986	30.655	ng/u1	-0.01
49) Acenaphthylene-d8	14.222	160	1314064	30.997	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.739	143	28125	3.652	ng/u1	0.00
60) Fluorene-d10	15.528	176	1070151	33.137	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	160138	24.908	ng/u1	0.00
73) Anthracene-d10	17.386	188	1858976	38.420	ng/u1	-0.01
81) Pyrene-d10	19.622	212	2330584	40.269	ng/u1	-0.01
92) Benzo(a)pyrene-d12	23.651	264	2419536	40.759	ng/u1	-0.01


Target Compounds					Qvalue
2) 1,4-Dioxane	3.334	88	13698	2.390 ng/uL#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011910.D
Acq On : 04 Oct 2022 13:52
Operator : CG/JU
Sample : N4873-13
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXZ58

Quant Time: Oct 05 04:45:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 01 00:53:59 2022
Response via : Initial Calibration

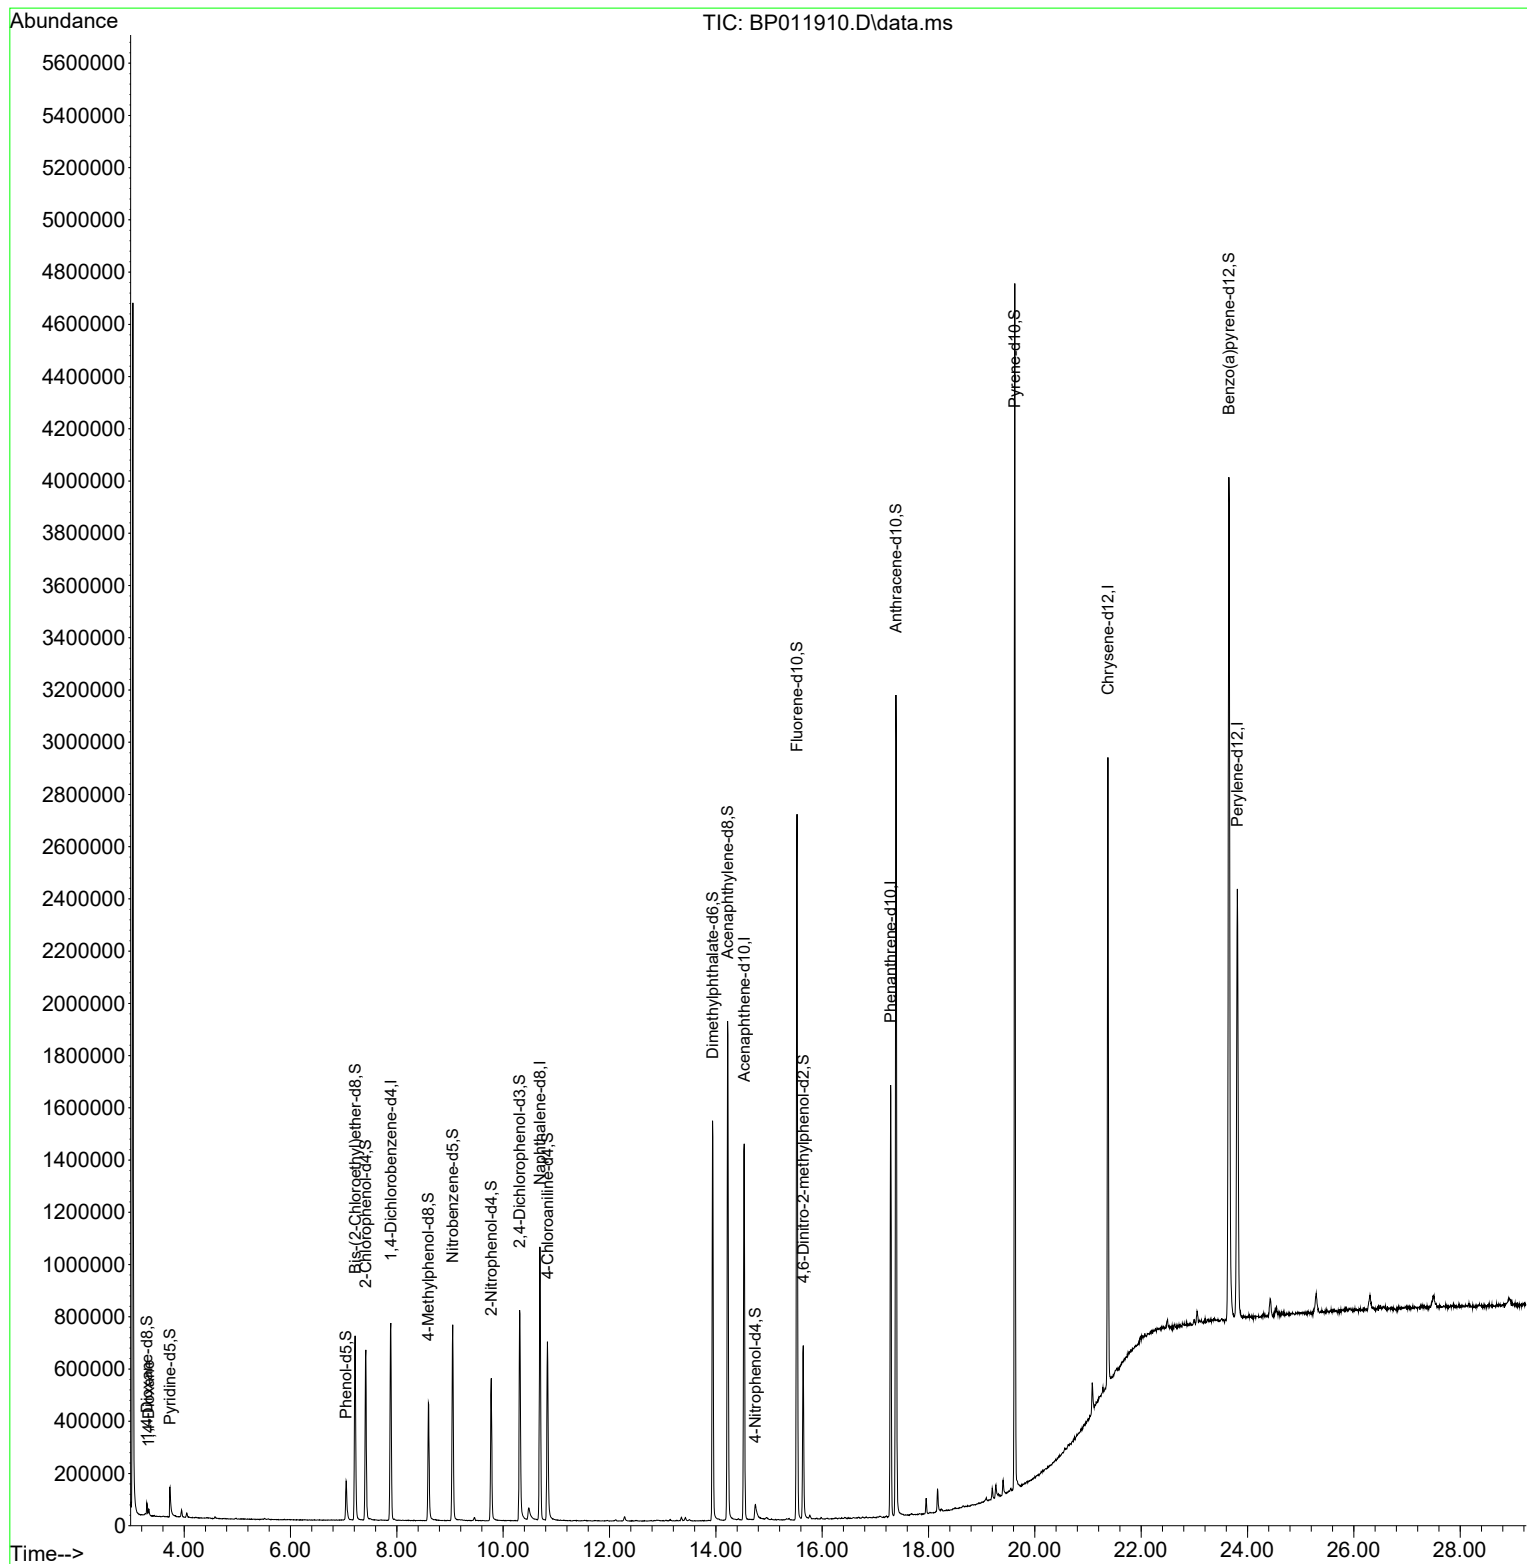

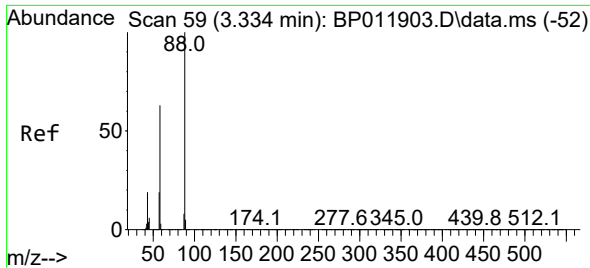

#2
 1,4-Dioxane
 Concen: 2.390 ng/uL
 RT: 3.334 min Scan# 51
 Delta R.T. -0.006 min
 Lab File: BP011910.D
 Acq: 04 Oct 2022 13:52

Instrument :
 BNA_P
 ClientSampleId :
 EXZ58

Tgt Ion: 88 Resp: 13698
 Ion Ratio Lower Upper
 88 100
 43 23.4 15.6 23.4#
 58 62.1 48.6 72.8

