

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
 Data File : BP011912.D
 Acq On : 04 Oct 2022 15:00
 Operator : CG/JU
 Sample : N4873-14
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXZ59

Quant Time: Oct 05 04:52:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 01 00:53:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	234737	20.000	ng/u1	0.00
20) Naphthalene-d8	10.693	136	957416	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.534	164	567258	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.286	188	1209750	20.000	ng/u1	-0.01
79) Chrysene-d12	21.374	240	1308221	20.000	ng/u1	-0.01
88) Perylene-d12	23.810	264	1318828	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	24698	4.640	ng/uL	0.00
4) Pyridine-d5	3.728	84	105000	6.735	ng/u1	0.00
7) Phenol-d5	7.052	99	107129	5.286	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.216	67	298248	26.552	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.416	132	333005	20.816	ng/u1	0.00
15) 4-Methylphenol-d8	8.599	113	195794	11.688	ng/u1	0.00
21) Nitrobenzene-d5	9.051	128	216015	29.621	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.775	143	205257	26.308	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.316	165	361269	25.034	ng/u1	0.00
31) 4-Chloroaniline-d4	10.834	131	392999	17.863	ng/u1	-0.01
46) Dimethylphthalate-d6	13.939	166	1251231	30.845	ng/u1	-0.01
49) Acenaphthylene-d8	14.222	160	1412605	30.547	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.739	143	40674	4.842	ng/u1	0.00
60) Fluorene-d10	15.528	176	1139127	32.336	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200	167279	22.845	ng/u1	0.00
73) Anthracene-d10	17.386	188	1797145	32.612	ng/u1	-0.01
81) Pyrene-d10	19.621	212	2322752	35.058	ng/u1	-0.01
92) Benzo(a)pyrene-d12	23.651	264	2285536	34.619	ng/u1	-0.01


Target Compounds					Qvalue
2) 1,4-Dioxane	3.334	88	6953	1.210 ng/uL#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011912.D
Acq On : 04 Oct 2022 15:00
Operator : CG/JU
Sample : N4873-14
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXZ59

Quant Time: Oct 05 04:52:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 01 00:53:59 2022
Response via : Initial Calibration

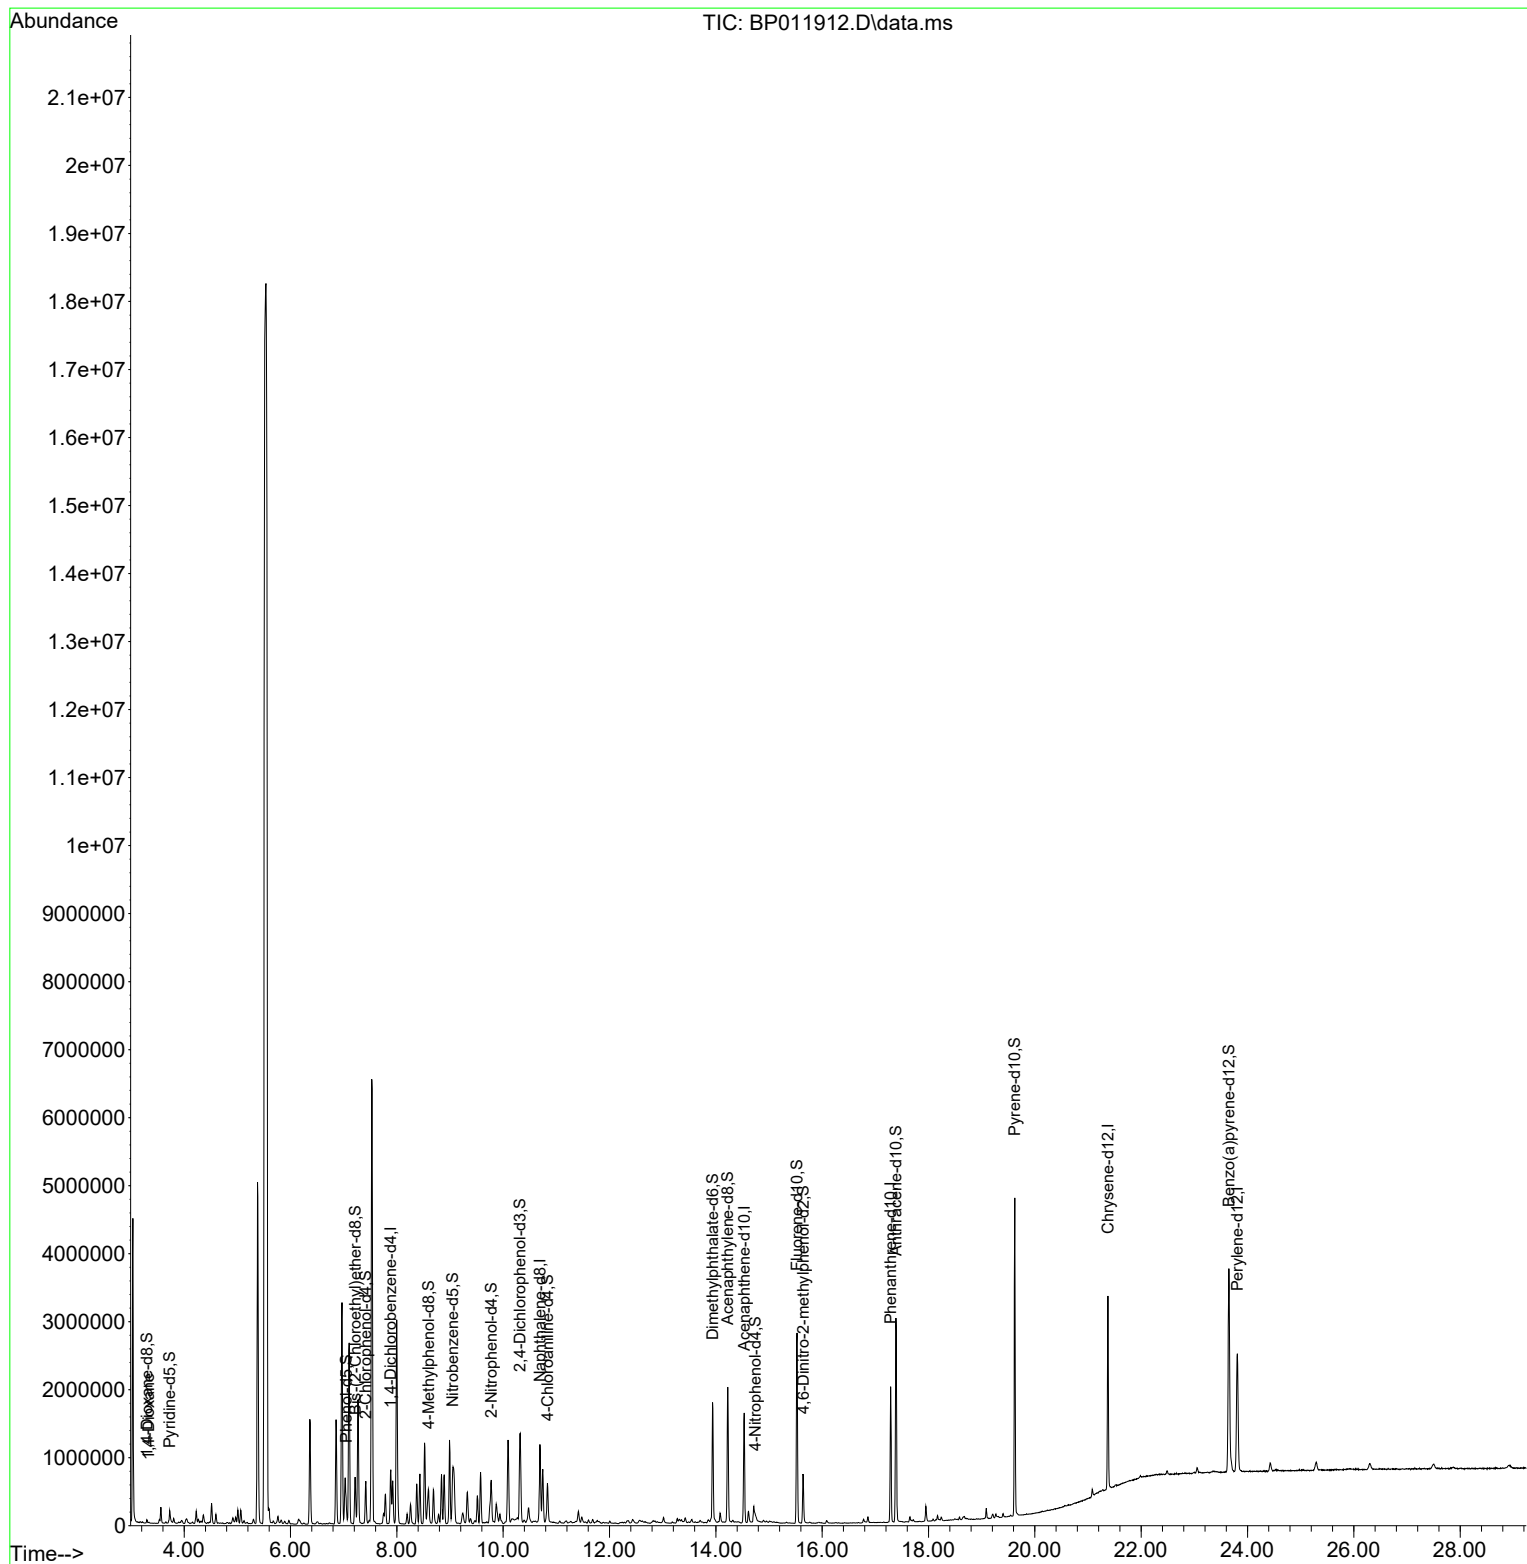

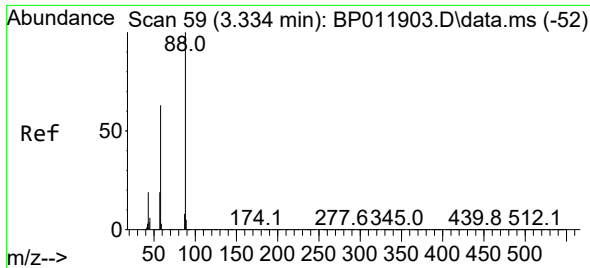

#2
 1,4-Dioxane
 Concen: 1.210 ng/uL
 RT: 3.334 min Scan# 51
 Delta R.T. -0.006 min
 Lab File: BP011912.D
 Acq: 04 Oct 2022 15:00

Instrument :
 BNA_P
 ClientSampleId :
 EXZ59

Tgt Ion: 88 Resp: 6953
 Ion Ratio Lower Upper
 88 100
 43 25.5 15.6 23.4#
 58 65.8 48.6 72.8

