

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
 Data File : BP011871.D
 Acq On : 03 Oct 2022 14:33
 Operator : CG/JU
 Sample : N4859-09
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E10049

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011871.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.040	4	9	30	rVB	4522459	5911594	94.35%	10.438%
2	3.304	50	54	59	rBV	45533	53478	0.85%	0.094%
3	3.734	125	127	143	rBV	211696	329046	5.25%	0.581%
4	3.957	160	165	171	rBV	27172	39109	0.62%	0.069%
5	4.052	177	181	187	rBV	15348	20063	0.32%	0.035%
6	4.993	335	341	344	rVB3	4214	7968	0.13%	0.014%
7	5.163	366	370	376	rVB9	4327	8425	0.13%	0.015%
8	7.057	684	692	703	rBV	156427	286496	4.57%	0.506%
9	7.222	713	720	736	rBV	677778	1098846	17.54%	1.940%
10	7.422	746	754	765	rBV	613456	1022101	16.31%	1.805%
11	7.892	826	834	843	rBV	818243	1304353	20.82%	2.303%
12	8.604	948	955	966	rBV	465977	805205	12.85%	1.422%
13	8.887	997	1003	1009	rVB5	6113	12013	0.19%	0.021%
14	8.975	1013	1018	1025	rVV2	14425	28303	0.45%	0.050%
15	9.057	1025	1032	1047	rVV	710105	1184614	18.91%	2.092%
16	9.175	1050	1052	1057	rVV5	5427	10059	0.16%	0.018%
17	9.251	1060	1065	1072	rVB4	6625	13012	0.21%	0.023%
18	9.439	1091	1097	1099	rBV	12338	18415	0.29%	0.033%
19	9.463	1099	1101	1106	rVB2	11676	17484	0.28%	0.031%
20	9.587	1115	1122	1126	rVB9	2698	6614	0.11%	0.012%
21	9.781	1148	1155	1168	rVV	507315	863117	13.78%	1.524%
22	9.892	1170	1174	1179	rVB7	4065	7497	0.12%	0.013%
23	10.110	1202	1211	1218	rVB9	7898	16983	0.27%	0.030%
24	10.198	1220	1226	1230	rBV7	4131	7594	0.12%	0.013%
25	10.322	1239	1247	1270	rBV	785951	1409345	22.49%	2.488%
26	10.486	1270	1275	1284	rBV2	29369	75766	1.21%	0.134%
27	10.698	1302	1311	1319	rBV	1051195	1837684	29.33%	3.245%
28	10.839	1327	1335	1349	rBV	749779	1380755	22.04%	2.438%
29	10.945	1349	1353	1358	rVV	19261	37217	0.59%	0.066%
30	10.992	1358	1361	1370	rVV5	10285	19185	0.31%	0.034%
31	11.116	1377	1382	1387	rVV2	13306	24739	0.39%	0.044%
32	11.181	1390	1393	1397	rVB5	4832	6514	0.10%	0.012%
33	11.286	1408	1411	1417	rVB7	3848	6635	0.11%	0.012%
34	11.469	1435	1442	1447	rBV9	4700	8901	0.14%	0.016%
35	11.522	1447	1451	1455	rBV6	4274	7281	0.12%	0.013%
36	11.816	1496	1501	1506	rBV2	23724	38767	0.62%	0.068%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
 Data File : BP011871.D
 Acq On : 03 Oct 2022 14:33
 Operator : CG/JU
 Sample : N4859-09
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E10049

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

37	11.892	1511	1514	1523	rVB6	4747	8889	0.14%	0.016%
38	12.257	1571	1576	1578	rBV	12865	19006	0.30%	0.034%
39	12.292	1578	1582	1588	rVB2	17359	30323	0.48%	0.054%
40	12.580	1618	1631	1637	rVB3	29457	57901	0.92%	0.102%
41	13.369	1760	1765	1770	rBV3	15684	32890	0.52%	0.058%
42	13.433	1772	1776	1782	rVB6	8407	14153	0.23%	0.025%
43	13.516	1782	1790	1793	rBV10	4255	9508	0.15%	0.017%
44	13.592	1798	1803	1809	rVB3	11413	19933	0.32%	0.035%
45	13.710	1817	1823	1827	rBV4	7594	14408	0.23%	0.025%
46	13.863	1840	1849	1855	rBV6	9132	21251	0.34%	0.038%
47	13.945	1855	1863	1878	rBV	1551700	2257009	36.02%	3.985%
48	14.092	1884	1888	1891	rBV	13258	14859	0.24%	0.026%
49	14.127	1891	1894	1899	rVB3	13536	19223	0.31%	0.034%
50	14.227	1905	1911	1925	rBV	1803793	2773587	44.27%	4.897%
51	14.433	1942	1946	1950	rVB7	4831	7889	0.13%	0.014%
52	14.539	1953	1964	1970	rBV	1546749	2296747	36.66%	4.055%
53	14.598	1970	1974	1983	rVB	197417	301854	4.82%	0.533%
54	14.751	1994	2000	2010	rBV	61686	153473	2.45%	0.271%
55	14.845	2013	2016	2021	rVB3	11183	15967	0.25%	0.028%
56	14.939	2027	2032	2039	rVB	23452	44287	0.71%	0.078%
57	15.157	2063	2069	2074	rVB9	4952	10828	0.17%	0.019%
58	15.386	2102	2108	2115	rVB9	9071	20427	0.33%	0.036%
59	15.533	2124	2133	2139	rBV	2503175	3644534	58.17%	6.435%
60	15.645	2146	2152	2161	rBV	578762	853787	13.63%	1.507%
61	15.774	2171	2174	2177	rBV3	5709	7492	0.12%	0.013%
62	15.880	2189	2192	2198	rVB4	9157	15110	0.24%	0.027%
63	15.986	2206	2210	2214	rBV7	9775	16466	0.26%	0.029%
64	16.027	2214	2217	2223	rVB7	9299	16225	0.26%	0.029%
65	16.227	2246	2251	2252	rBV5	5547	9503	0.15%	0.017%
66	16.269	2252	2258	2264	rVB3	11907	25152	0.40%	0.044%
67	17.292	2426	2432	2438	rBV	1844671	2602942	41.55%	4.596%
68	17.392	2443	2449	2461	rVV	2962841	4127180	65.87%	7.287%
69	17.957	2542	2545	2549	rVB2	18091	21686	0.35%	0.038%
70	18.174	2577	2582	2590	rBV2	113115	183573	2.93%	0.324%
71	19.204	2754	2757	2761	rVB2	37823	47702	0.76%	0.084%
72	19.268	2765	2768	2771	rBV	49218	64358	1.03%	0.114%
73	19.404	2788	2791	2796	rBV2	87790	115793	1.85%	0.204%
74	19.627	2823	2829	2839	rBV	4078316	5516325	88.05%	9.740%
75	21.374	3121	3126	3132	rBV2	2493074	3432682	54.79%	6.061%
76	23.650	3507	3513	3527	rVB2	3020110	6265270	100.00%	11.062%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011871.D
Acq On : 03 Oct 2022 14:33
Operator : CG/JU
Sample : N4859-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10049

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Title : SVOA CALIBRATION

77 23.809 3534 3540 3550 rVB2 1798091 3601191 57.48% 6.358%




Sum of corrected areas: 56636561

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011871.D
Acq On : 03 Oct 2022 14:33
Operator : CG/JU
Sample : N4859-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10049

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

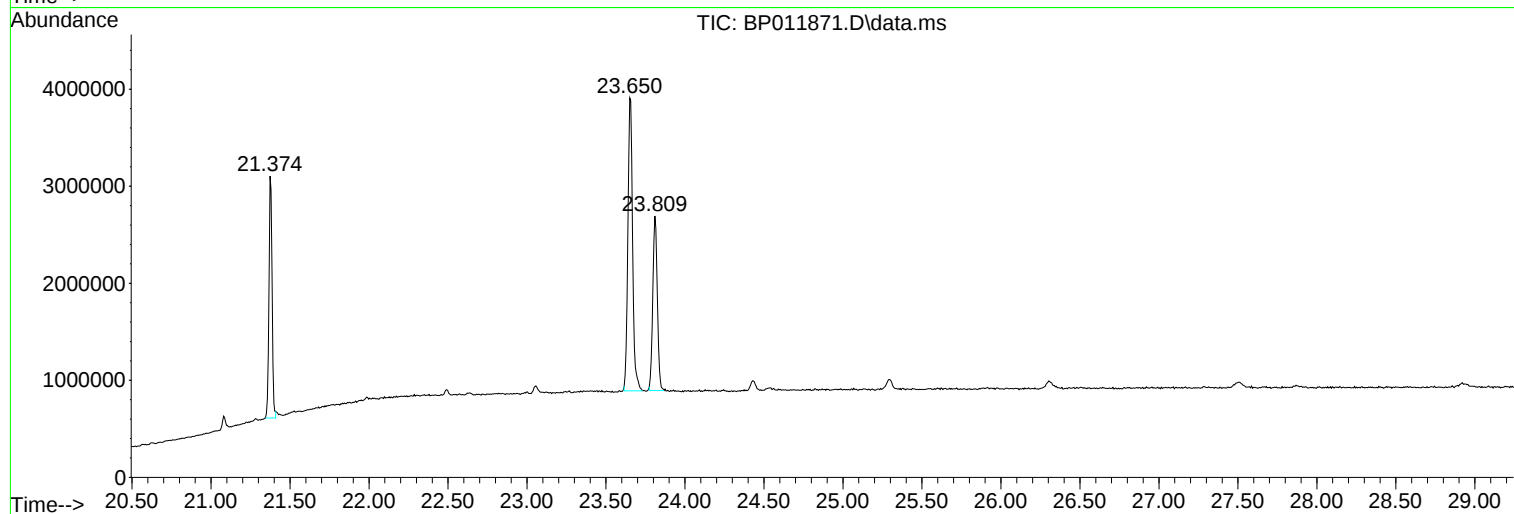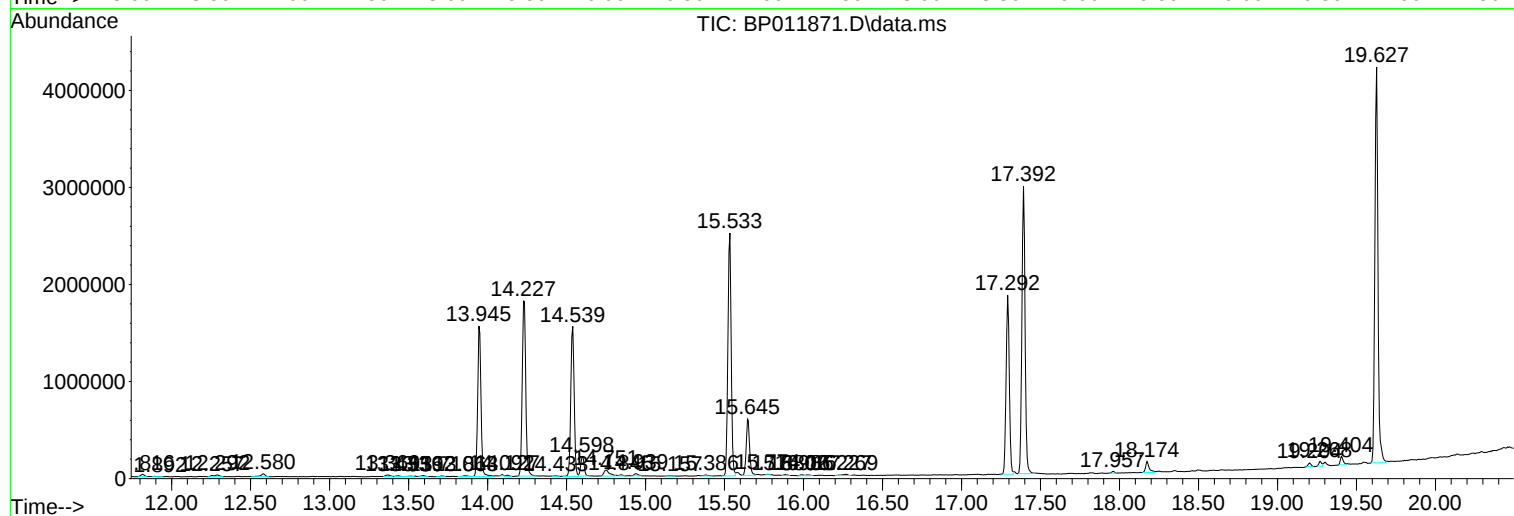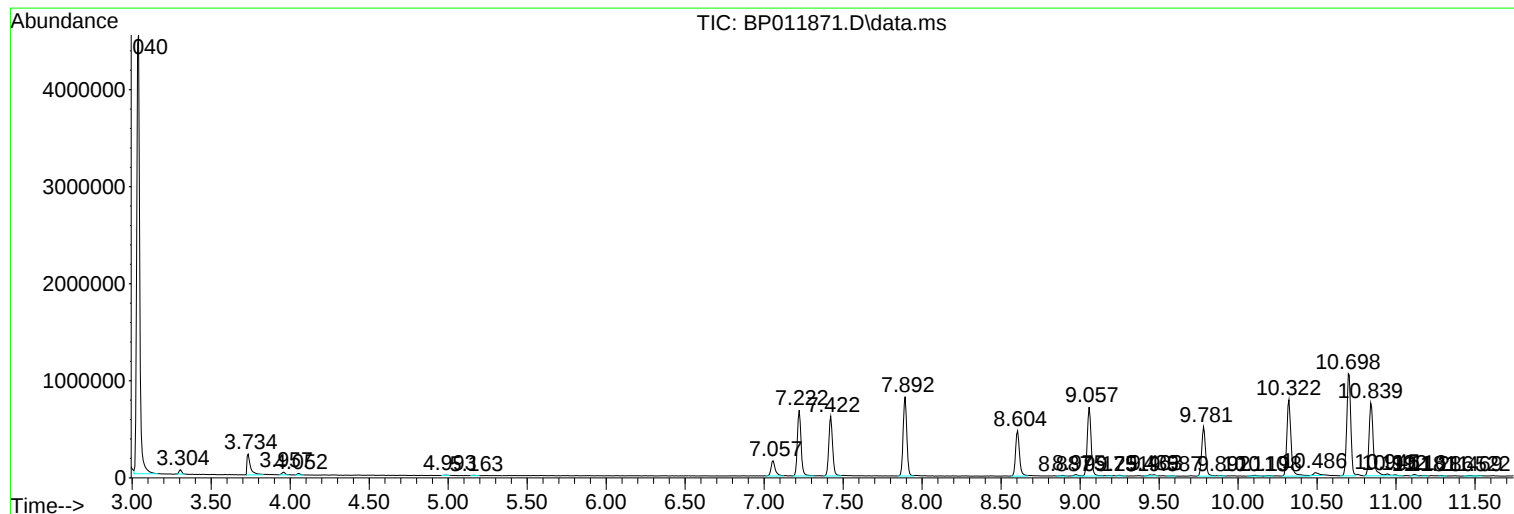

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011871.D
Acq On : 03 Oct 2022 14:33
Operator : CG/JU
Sample : N4859-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10049










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.040	90.64 ng/ul	5911590	1,4-Dichlorobenzene-d4	7.892

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	86		
2	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78		
3	2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40		
4	Pentane, 3-methoxy-	102	C6H14O	036839-67-5	12		
5	N-Ethylformamide	73	C3H7NO	000627-45-2	9		

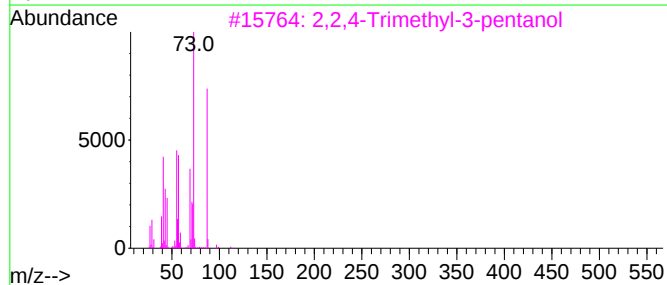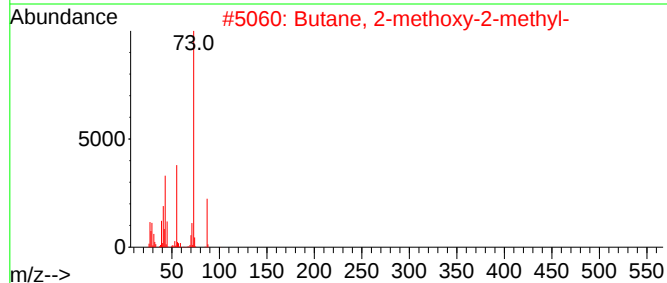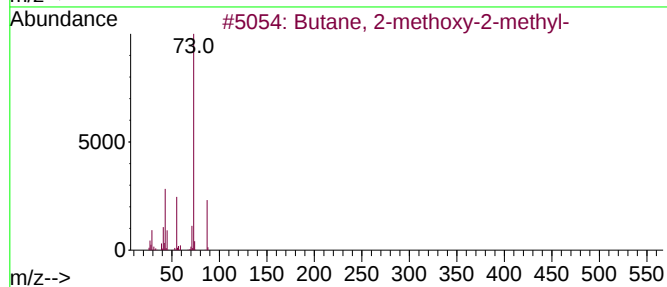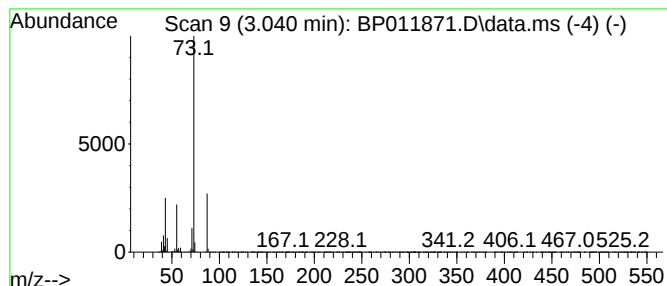

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011871.D
Acq On : 03 Oct 2022 14:33
Operator : CG/JU
Sample : N4859-09
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10049

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.040	90.6	ng/ul	5911590	1	7.892	1304350	20.0