

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
 Data File : BP011875.D
 Acq On : 03 Oct 2022 16:49
 Operator : CG/JU
 Sample : N4847-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8P5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011875.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	4	8	33	rVB	4973977	6327301	83.77%	9.969%
2	3.305	50	54	62	rVB	57051	72621	0.96%	0.114%
3	3.734	125	127	146	rBV	182649	289451	3.83%	0.456%
4	3.958	160	165	171	rVB	29197	47721	0.63%	0.075%
5	4.052	177	181	185	rVB	21622	29027	0.38%	0.046%
6	4.993	336	341	349	rVB2	8531	18009	0.24%	0.028%
7	7.058	681	692	704	rBV	175219	330409	4.37%	0.521%
8	7.222	713	720	732	rBV	739800	1202622	15.92%	1.895%
9	7.422	746	754	764	rBV	682683	1144538	15.15%	1.803%
10	7.893	826	834	842	rBV	823393	1359515	18.00%	2.142%
11	7.964	842	846	851	rVB6	5409	10339	0.14%	0.016%
12	8.605	947	955	970	rBV	528703	930215	12.32%	1.466%
13	9.058	1024	1032	1043	rBV	767625	1320773	17.49%	2.081%
14	9.469	1096	1102	1107	rVV	14869	24891	0.33%	0.039%
15	9.781	1147	1155	1170	rBV	601833	993706	13.16%	1.566%
16	10.322	1239	1247	1269	rBV	870706	1606929	21.27%	2.532%
17	10.699	1303	1311	1325	rBV	1139110	1937169	25.65%	3.052%
18	10.840	1328	1335	1352	rBV	832386	1531753	20.28%	2.413%
19	12.240	1566	1573	1577	rBV2	11438	24140	0.32%	0.038%
20	12.293	1577	1582	1590	rVB	16607	32614	0.43%	0.051%
21	13.357	1754	1763	1769	rBV2	13655	25093	0.33%	0.040%
22	13.428	1769	1775	1781	rVB5	7841	15113	0.20%	0.024%
23	13.504	1781	1788	1796	rBV9	4507	10747	0.14%	0.017%
24	13.946	1857	1863	1879	rBV	1810754	2594264	34.35%	4.087%
25	14.228	1899	1911	1932	rBV	2136137	3237279	42.86%	5.101%
26	14.534	1957	1963	1979	rBV	1604108	2454552	32.50%	3.867%
27	14.746	1993	1999	2013	rBV2	79404	210167	2.78%	0.331%
28	14.957	2030	2035	2039	rBV7	11263	19398	0.26%	0.031%
29	15.528	2126	2132	2146	rBV	2818059	4275527	56.60%	6.736%
30	15.645	2146	2152	2168	rVV	833674	1147679	15.19%	1.808%
31	15.775	2170	2174	2180	rVB4	15118	24933	0.33%	0.039%
32	17.292	2425	2432	2442	rBV	1976102	2859484	37.86%	4.505%
33	17.392	2442	2449	2461	rVV	3711948	5092287	67.42%	8.023%
34	18.175	2577	2582	2591	rBV	135830	213599	2.83%	0.337%
35	19.204	2753	2757	2762	rBV2	45855	60118	0.80%	0.095%
36	19.269	2764	2768	2774	rBV	64645	106810	1.41%	0.168%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011875.D
Acq On : 03 Oct 2022 16:49
Operator : CG/JU
Sample : N4847-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8P5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Title : SVOA CALIBRATION

37	19.404	2787	2791	2798	rBV2	116779	178103	2.36%	0.281%
38	19.628	2823	2829	2835	rBV	4721095	6479489	85.78%	10.209%
39	21.080	3073	3076	3082	rBV3	130873	170692	2.26%	0.269%
40	21.375	3121	3126	3132	rBV	2920775	3668326	48.57%	5.780%
41	23.651	3506	3513	3526	rVB2	3496569	7553268	100.00%	11.901%
42	23.810	3534	3540	3551	rVB2	1931251	3837847	50.81%	6.047%




Sum of corrected areas: 63468518

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011875.D
Acq On : 03 Oct 2022 16:49
Operator : CG/JU
Sample : N4847-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8P5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

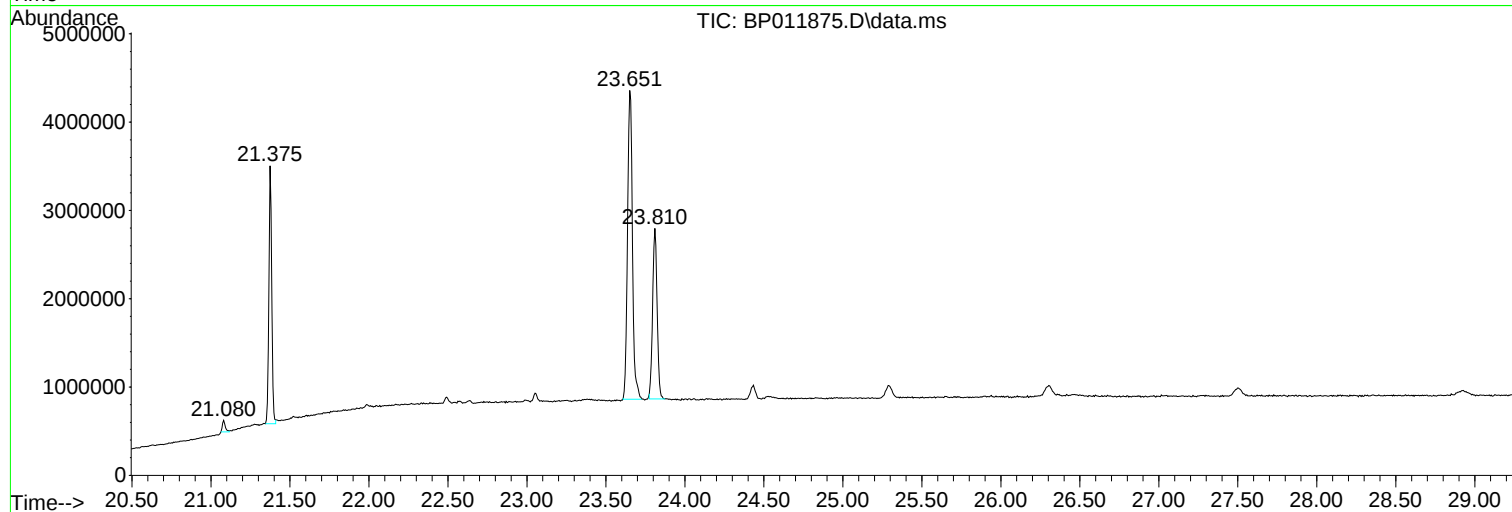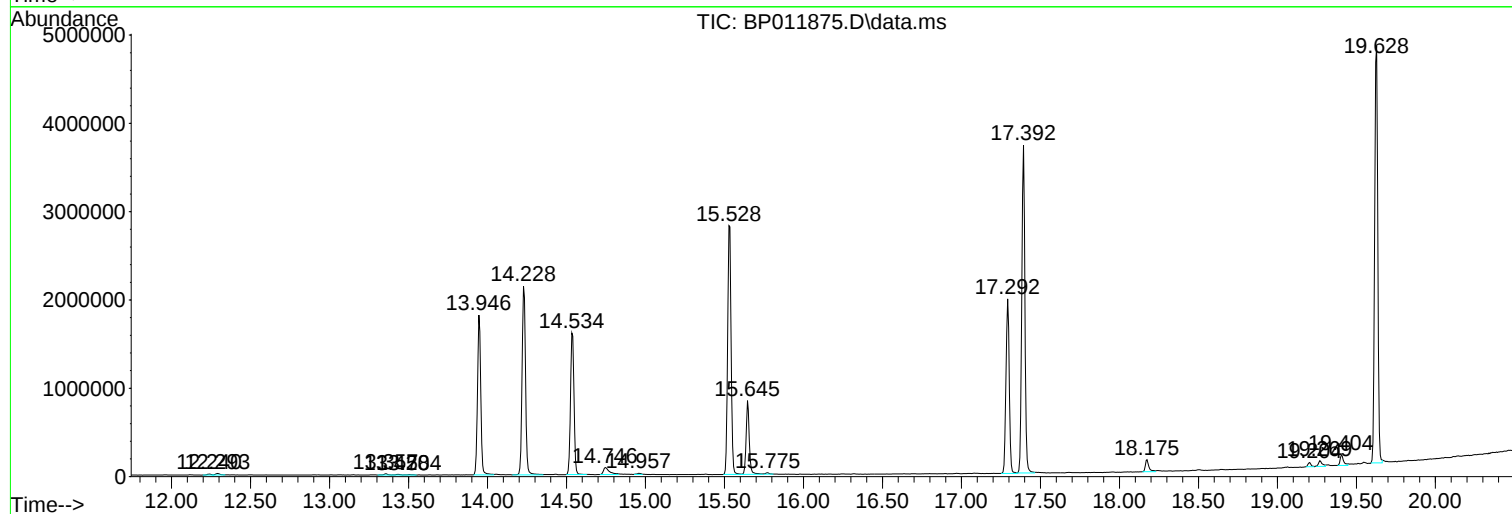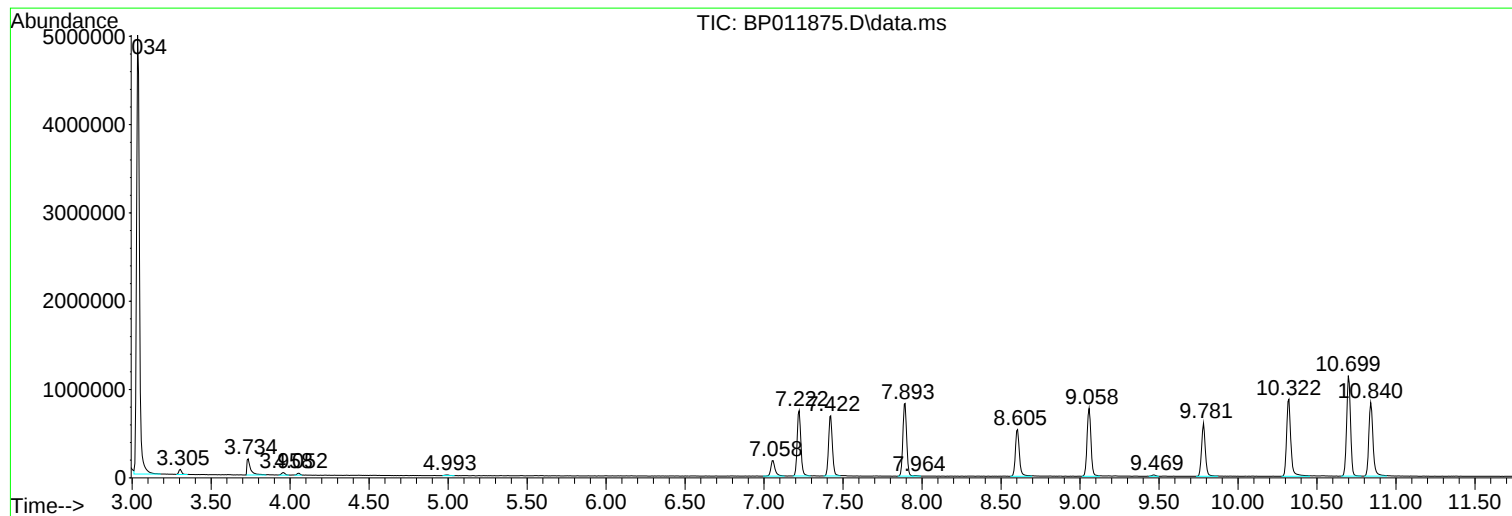

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011875.D
Acq On : 03 Oct 2022 16:49
Operator : CG/JU
Sample : N4847-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8P5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.034	93.08 ng/ul	6327300	1,4-Dichlorobenzene-d4	7.893

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	72
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	43
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9

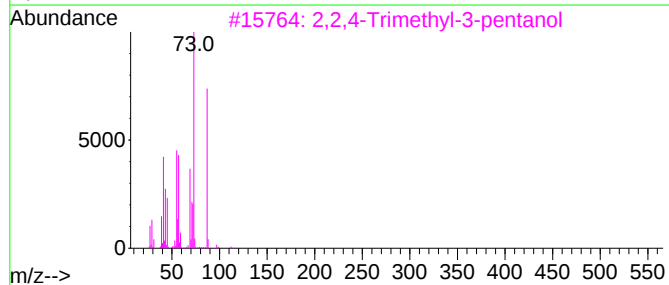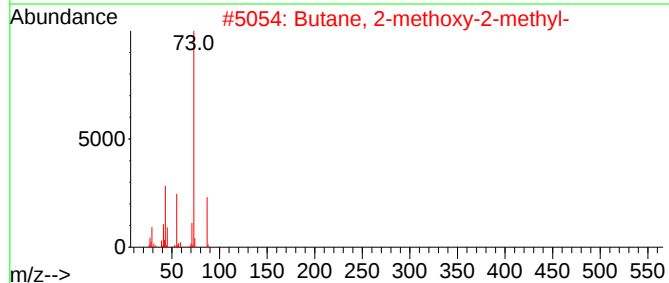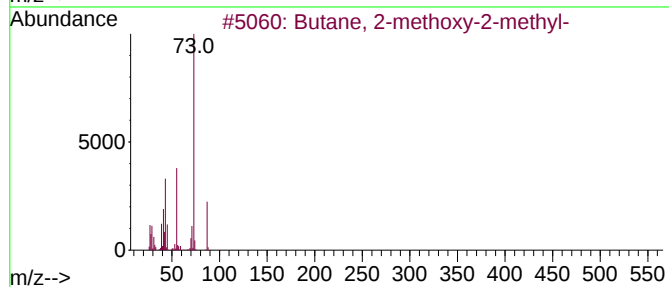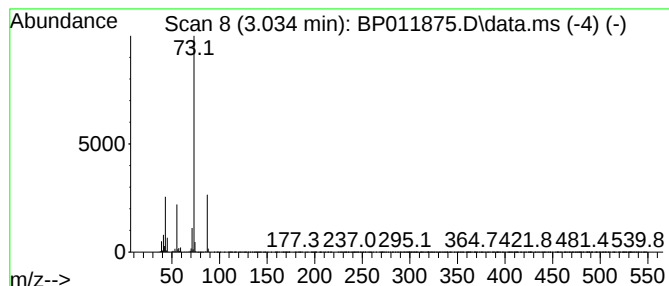

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011875.D
Acq On : 03 Oct 2022 16:49
Operator : CG/JU
Sample : N4847-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8P5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.034	93.1	ng/u1	6327300	1	7.893	1359520	20.0