

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
 Data File : BP011877.D
 Acq On : 03 Oct 2022 17:58
 Operator : CG/JU
 Sample : N4859-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E10020

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011877.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	4	8	30	rVB	4751796	6089397	81.34%	9.603%
2	3.305	50	54	63	rVB	53002	70233	0.94%	0.111%
3	3.405	69	71	76	rVB3	8468	8783	0.12%	0.014%
4	3.734	124	127	139	rBV	162433	258194	3.45%	0.407%
5	3.958	161	165	171	rVB	29880	43182	0.58%	0.068%
6	4.052	177	181	186	rBV	19101	24935	0.33%	0.039%
7	4.528	256	262	267	rBV7	4190	9459	0.13%	0.015%
8	7.052	681	691	705	rBV	177953	342188	4.57%	0.540%
9	7.222	713	720	733	rBV	733892	1234663	16.49%	1.947%
10	7.422	746	754	764	rBV	685020	1153016	15.40%	1.818%
11	7.887	824	833	844	rBV	829642	1385718	18.51%	2.185%
12	8.599	945	954	968	rBV	527010	915554	12.23%	1.444%
13	9.057	1024	1032	1045	rBV	796892	1357704	18.13%	2.141%
14	9.216	1055	1059	1066	rVB4	13628	23328	0.31%	0.037%
15	9.781	1147	1155	1168	rBV	500581	847641	11.32%	1.337%
16	10.316	1239	1246	1270	rBV	868453	1615657	21.58%	2.548%
17	10.699	1303	1311	1323	rBV	1179799	1994636	26.64%	3.146%
18	10.840	1327	1335	1350	rBV	874414	1617544	21.61%	2.551%
19	12.293	1576	1582	1590	rBV2	17232	33106	0.44%	0.052%
20	13.434	1770	1776	1781	rBV2	15919	27576	0.37%	0.043%
21	13.504	1784	1788	1799	rVB6	4749	10406	0.14%	0.016%
22	13.945	1856	1863	1875	rBV	1844859	2593798	34.64%	4.090%
23	14.228	1902	1911	1927	rBV	2229851	3350001	44.75%	5.283%
24	14.534	1955	1963	1973	rBV	1706395	2604072	34.78%	4.107%
25	14.745	1994	1999	2021	rBV	52873	166475	2.22%	0.263%
26	14.963	2030	2036	2041	rVB10	9310	17951	0.24%	0.028%
27	15.222	2076	2080	2087	rBV7	6036	8855	0.12%	0.014%
28	15.528	2126	2132	2146	rBV	2928909	4388442	58.62%	6.921%
29	15.645	2146	2152	2163	rBV	422940	634871	8.48%	1.001%
30	15.775	2169	2174	2180	rVB2	13856	22822	0.30%	0.036%
31	17.292	2425	2432	2442	rBV	2166677	3117939	41.65%	4.917%
32	17.392	2442	2449	2461	rVV	3576684	5338659	71.31%	8.419%
33	18.175	2579	2582	2588	rBV5	12023	18976	0.25%	0.030%
34	19.204	2753	2757	2762	rBV	50329	67201	0.90%	0.106%
35	19.269	2765	2768	2773	rVV	55567	76429	1.02%	0.121%
36	19.628	2823	2829	2839	rBV	4925724	6629459	88.55%	10.455%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011877.D
Acq On : 03 Oct 2022 17:58
Operator : CG/JU
Sample : N4859-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10020

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Title : SVOA CALIBRATION

37	21.374	3121	3126	3133	rBV	3040040	3815007	50.96%	6.016%
38	23.651	3506	3513	3526	rVB2	3613494	7486801	100.00%	11.807%
39	23.810	3534	3540	3551	rVB2	2057777	4010198	53.56%	6.324%




Sum of corrected areas: 63410876

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011877.D
Acq On : 03 Oct 2022 17:58
Operator : CG/JU
Sample : N4859-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10020

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

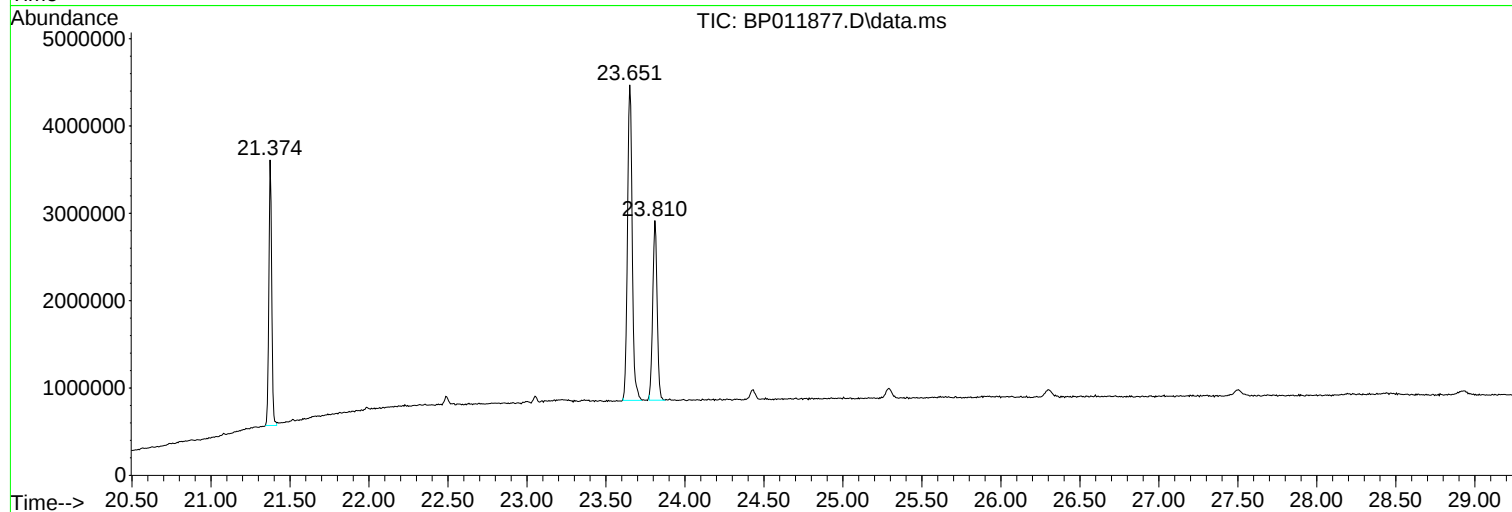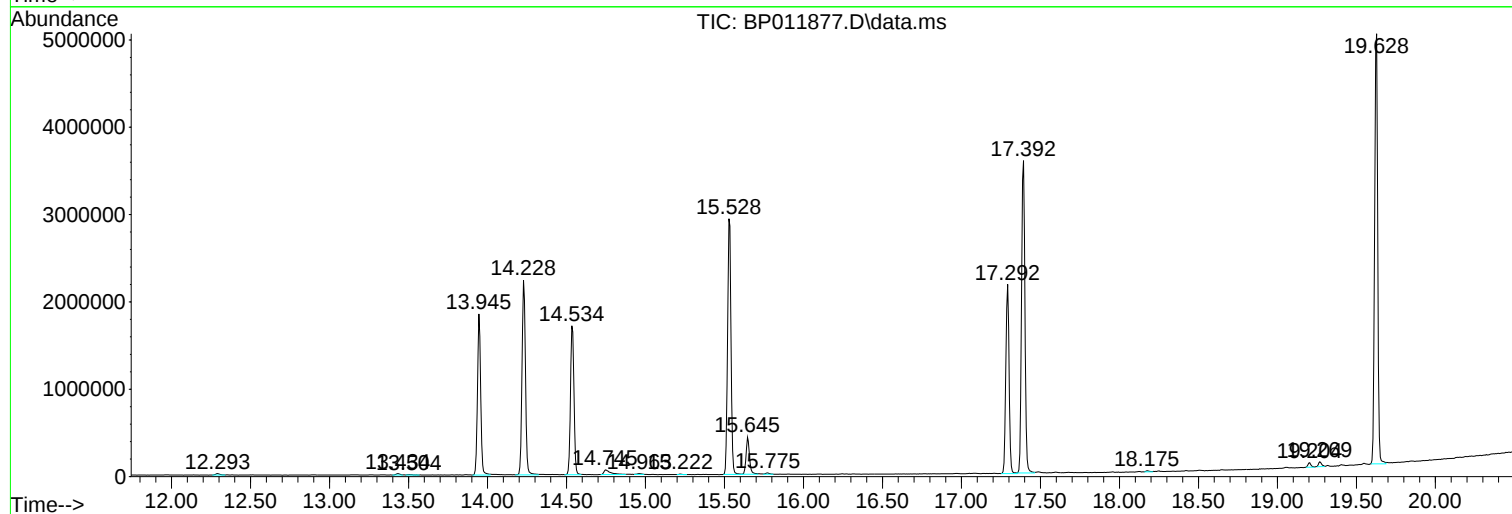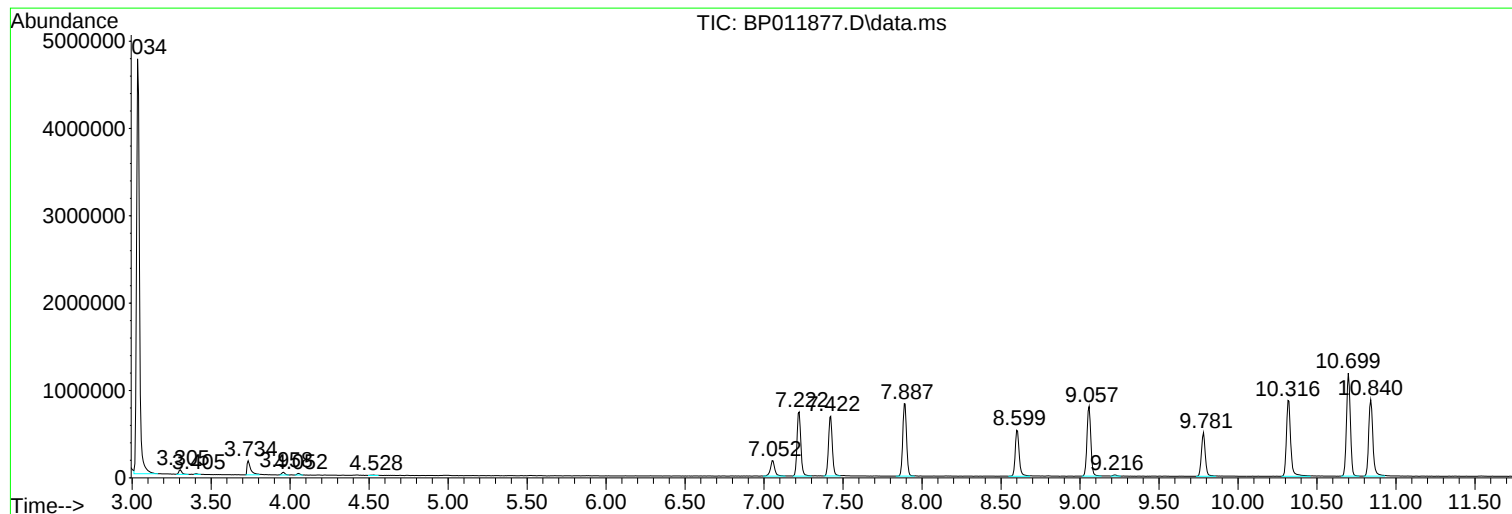

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011877.D
Acq On : 03 Oct 2022 17:58
Operator : CG/JU
Sample : N4859-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10020










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.034	87.89 ng/ul	6089400	1,4-Dichlorobenzene-d4	7.893

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	72
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	43
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9

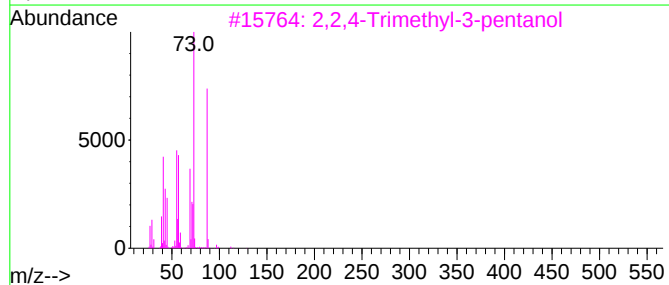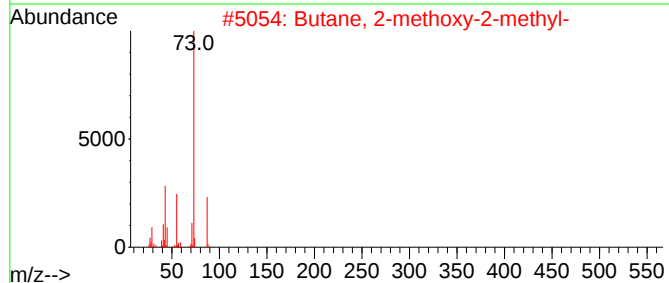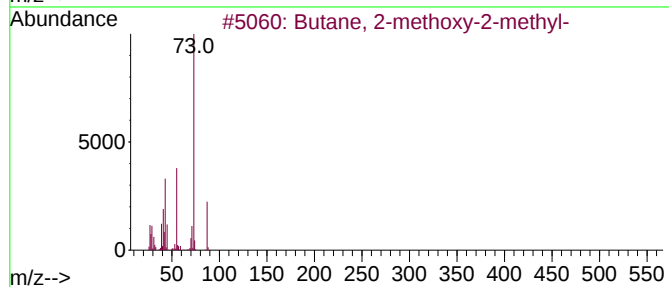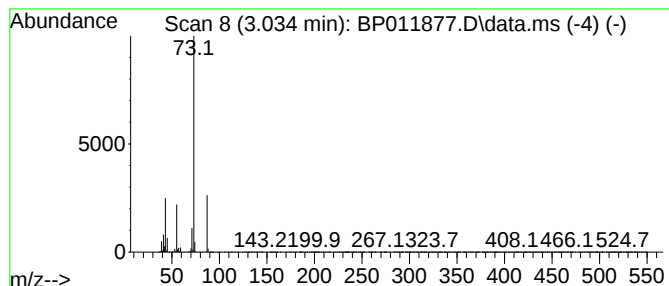

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011877.D
Acq On : 03 Oct 2022 17:58
Operator : CG/JU
Sample : N4859-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10020

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.034	87.9	ng/ul	6089400	1	7.893	1385720	20.0