

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
 Data File : BP011882.D
 Acq On : 03 Oct 2022 20:48
 Operator : CG/JU
 Sample : N4847-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8Q9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011882.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	4	8	31	rVB	5192214	6604808	100.00%	11.869%
2	3.305	50	54	59	rBV	48427	58275	0.88%	0.105%
3	3.728	124	126	140	rBV	236820	363853	5.51%	0.654%
4	3.957	159	165	170	rVB	33659	53058	0.80%	0.095%
5	4.052	177	181	186	rVB	16737	22582	0.34%	0.041%
6	4.987	335	340	348	rVB4	6104	13819	0.21%	0.025%
7	7.051	685	691	705	rVB	163777	288834	4.37%	0.519%
8	7.216	713	719	734	rBV	666355	1108171	16.78%	1.991%
9	7.416	746	753	765	rBV	629352	1047203	15.86%	1.882%
10	7.504	765	768	773	rVB5	4503	7164	0.11%	0.013%
11	7.887	827	833	842	rBV	776134	1257345	19.04%	2.260%
12	8.598	946	954	965	rBV	466533	802976	12.16%	1.443%
13	9.057	1023	1032	1046	rBV	695275	1203713	18.22%	2.163%
14	9.469	1096	1102	1110	rVB3	9880	18397	0.28%	0.033%
15	9.781	1147	1155	1165	rBV	529260	897826	13.59%	1.613%
16	10.316	1237	1246	1260	rBV	784061	1415142	21.43%	2.543%
17	10.698	1303	1311	1325	rBV	1029631	1768552	26.78%	3.178%
18	10.839	1327	1335	1358	rBV	665911	1247502	18.89%	2.242%
19	11.528	1444	1452	1457	rBV	2905	7569	0.11%	0.014%
20	12.239	1566	1573	1576	rBV6	7018	12443	0.19%	0.022%
21	12.286	1576	1581	1591	rVB3	14726	29767	0.45%	0.053%
22	12.522	1616	1621	1626	rVB7	6234	11336	0.17%	0.020%
23	13.357	1758	1763	1768	rBV3	9296	15432	0.23%	0.028%
24	13.427	1770	1775	1784	rVV2	15080	27339	0.41%	0.049%
25	13.504	1784	1788	1794	rVB9	4734	8954	0.14%	0.016%
26	13.945	1856	1863	1874	rBV	1560626	2180765	33.02%	3.919%
27	14.227	1904	1911	1930	rBV	1866075	2806557	42.49%	5.044%
28	14.427	1939	1945	1950	rVB8	4504	8933	0.14%	0.016%
29	14.533	1956	1963	1974	rBV	1444876	2163963	32.76%	3.889%
30	14.751	1993	2000	2014	rBV2	60576	175841	2.66%	0.316%
31	14.957	2029	2035	2045	rVB2	5965	15207	0.23%	0.027%
32	15.280	2085	2090	2097	rBV	142770	197410	2.99%	0.355%
33	15.380	2104	2107	2113	rVB6	6100	9122	0.14%	0.016%
34	15.527	2125	2132	2139	rBV	2449084	3601342	54.53%	6.472%
35	15.645	2146	2152	2169	rBV	629366	877760	13.29%	1.577%
36	15.769	2170	2173	2181	rVB4	11809	22404	0.34%	0.040%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
 Data File : BP011882.D
 Acq On : 03 Oct 2022 20:48
 Operator : CG/JU
 Sample : N4847-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB8Q9

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

37	17.292	2425	2432	2442	rBV	1721940	2488062	37.67%	4.471%
38	17.392	2442	2449	2462	rVV	2836184	4093516	61.98%	7.356%
39	18.174	2577	2582	2588	rBV3	35947	62370	0.94%	0.112%
40	19.198	2754	2756	2761	rVB3	32131	40312	0.61%	0.072%
41	19.268	2765	2768	2772	rBV	39549	49598	0.75%	0.089%
42	19.621	2823	2828	2839	rBV	3953276	5309343	80.39%	9.541%
43	21.080	3073	3076	3082	rBV3	115065	168545	2.55%	0.303%
44	21.374	3121	3126	3134	rBV	2582080	3332835	50.46%	5.989%
45	23.650	3506	3513	3528	rVB2	3014261	6246084	94.57%	11.224%
46	23.809	3534	3540	3552	rVB2	1692675	3504906	53.07%	6.298%




Sum of corrected areas: 55646935

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011882.D
Acq On : 03 Oct 2022 20:48
Operator : CG/JU
Sample : N4847-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8Q9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

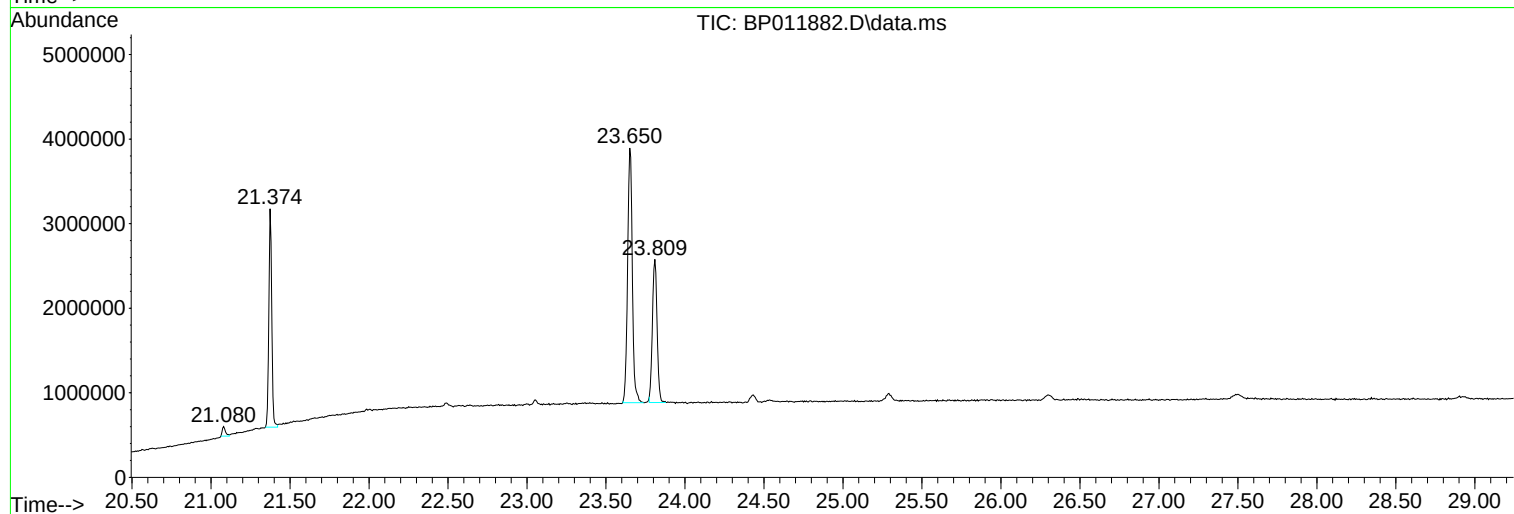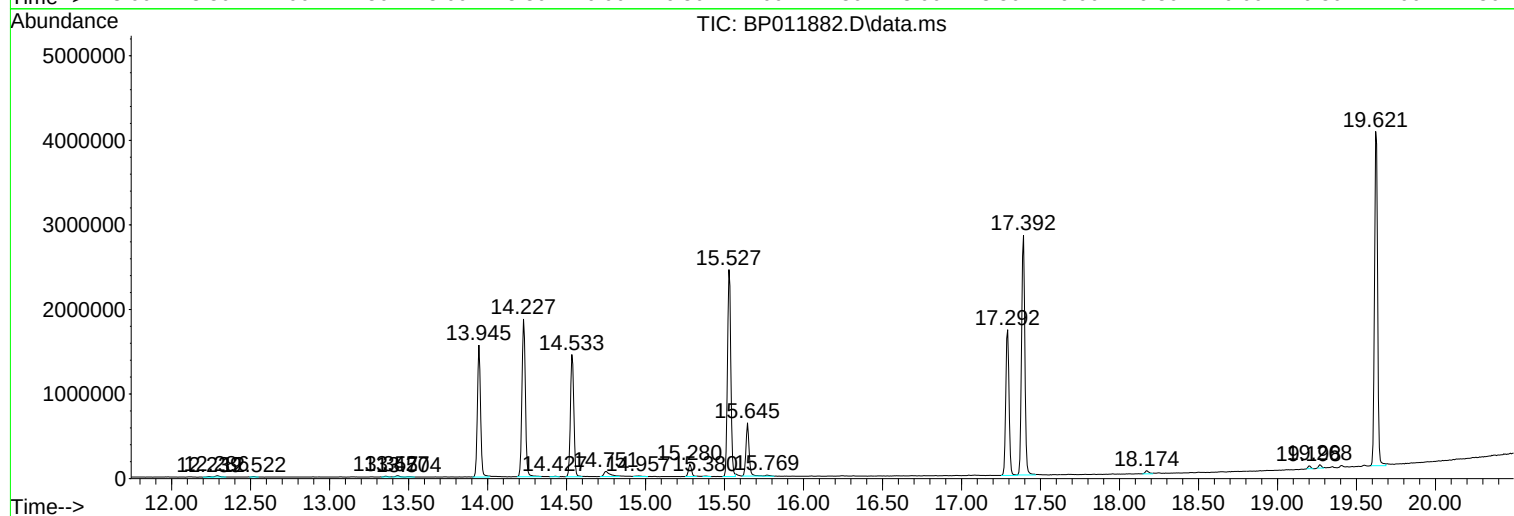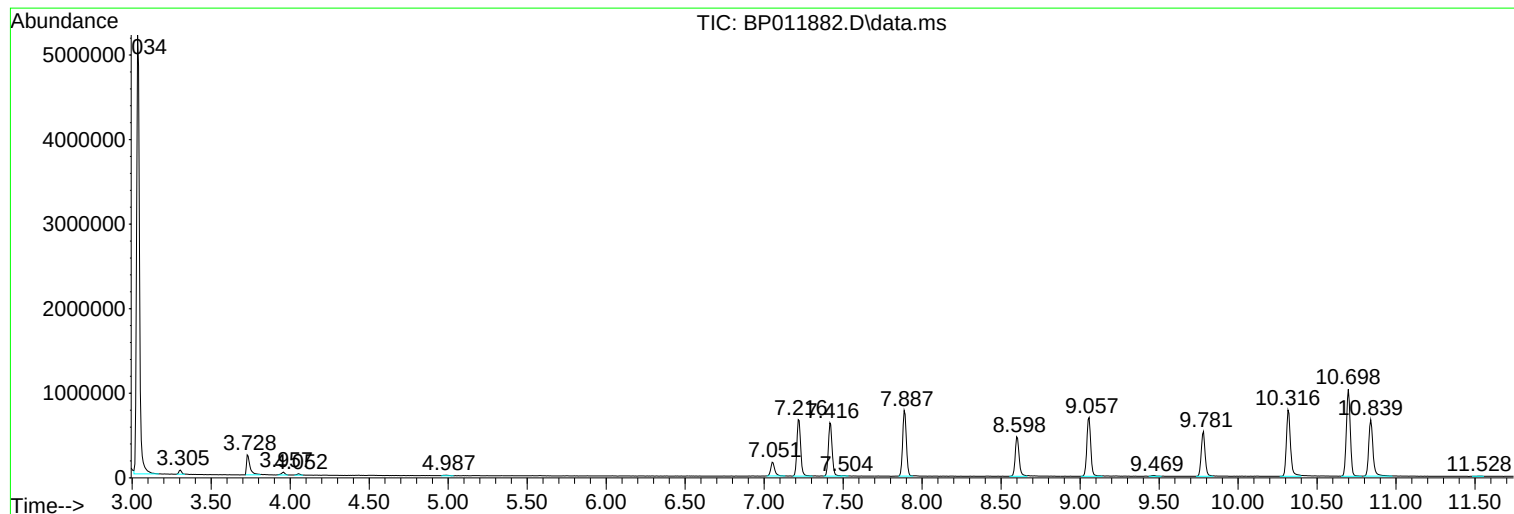

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011882.D
Acq On : 03 Oct 2022 20:48
Operator : CG/JU
Sample : N4847-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8Q9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.034	105.06 ng/ul	6604810	1,4-Dichlorobenzene-d4	7.887

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	72
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	43
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
5			N-Ethylformamide	73	C3H7NO	000627-45-2	9

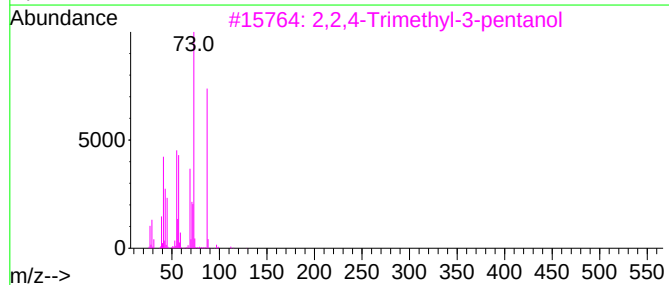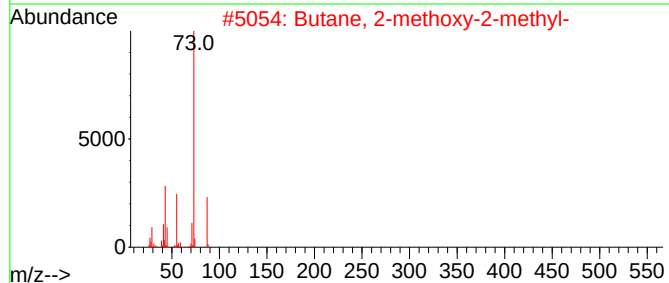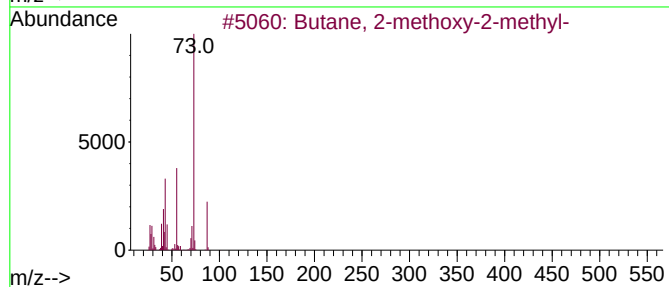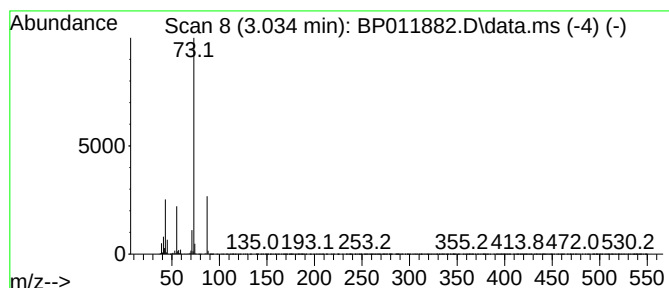

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011882.D
Acq On : 03 Oct 2022 20:48
Operator : CG/JU
Sample : N4847-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB8Q9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.034	105.1	ng/ul	6604810	1	7.887	1257350	20.0