

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
 Data File : BP011895.D
 Acq On : 04 Oct 2022 04:44
 Operator : CG/JU
 Sample : N4859-11
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E10051

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011895.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	3	8	33	rVB	5443850	6798276	71.06%	9.002%
2	3.299	50	53	62	rVB	64928	82142	0.86%	0.109%
3	3.728	123	126	140	rBV	200248	317666	3.32%	0.421%
4	3.958	159	165	176	rVB	34062	56566	0.59%	0.075%
5	4.052	177	181	186	rVB	16046	21461	0.22%	0.028%
6	7.052	683	691	703	rBV	175588	303039	3.17%	0.401%
7	7.216	711	719	731	rBV	864437	1376341	14.39%	1.822%
8	7.416	746	753	764	rBV	780020	1257874	13.15%	1.666%
9	7.499	764	767	773	rVB5	5364	10063	0.11%	0.013%
10	7.887	824	833	843	rBV	869327	1412219	14.76%	1.870%
11	8.599	947	954	971	rBV	592217	1035210	10.82%	1.371%
12	9.052	1024	1031	1051	rBV	963299	1622595	16.96%	2.148%
13	9.775	1144	1154	1166	rBV	723773	1224350	12.80%	1.621%
14	10.316	1238	1246	1268	rBV	1094703	1983519	20.73%	2.626%
15	10.693	1302	1310	1325	rBV	1298996	2234543	23.36%	2.959%
16	10.834	1327	1334	1354	rBV	963580	1807458	18.89%	2.393%
17	12.287	1575	1581	1590	rBV2	20164	39292	0.41%	0.052%
18	13.428	1769	1775	1783	rBV2	32783	54548	0.57%	0.072%
19	13.510	1783	1789	1796	rVB6	5019	10951	0.11%	0.015%
20	13.945	1856	1863	1879	rBV	2150393	3073790	32.13%	4.070%
21	14.228	1903	1911	1927	rBV	2669369	4026679	42.09%	5.332%
22	14.534	1955	1963	1978	rBV	1965625	2886723	30.18%	3.822%
23	14.745	1993	1999	2020	rBV2	66419	213931	2.24%	0.283%
24	14.957	2030	2035	2040	rVB9	8070	16694	0.17%	0.022%
25	15.528	2124	2132	2145	rBV	3725026	5312504	55.53%	7.034%
26	15.645	2146	2152	2167	rVV	928884	1329766	13.90%	1.761%
27	15.769	2169	2173	2180	rVB4	17865	32518	0.34%	0.043%
28	17.286	2425	2431	2442	rBV	2311002	3420852	35.76%	4.530%
29	17.386	2442	2448	2461	rVV	4130989	6195046	64.76%	8.203%
30	17.651	2490	2493	2497	rBV	8852	15617	0.16%	0.021%
31	18.169	2577	2581	2587	rBV4	38458	62155	0.65%	0.082%
32	19.198	2753	2756	2762	rVB	55581	69590	0.73%	0.092%
33	19.269	2764	2768	2774	rBV	63364	103417	1.08%	0.137%
34	19.404	2788	2791	2796	rBV4	37321	54145	0.57%	0.072%
35	19.622	2822	2828	2839	rBV	6366323	8193209	85.65%	10.849%
36	21.374	3121	3126	3133	rBV	3512750	4493652	46.97%	5.950%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011895.D
Acq On : 04 Oct 2022 04:44
Operator : CG/JU
Sample : N4859-11
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10051

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Title : SVOA CALIBRATION

37	23.651	3506	3513	3528	rVB2	4823329	9566371	100.00%	12.667%
38	23.810	3534	3540	3550	rVB	2492214	4808920	50.27%	6.367%




Sum of corrected areas: 75523692

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011895.D
Acq On : 04 Oct 2022 04:44
Operator : CG/JU
Sample : N4859-11
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10051

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

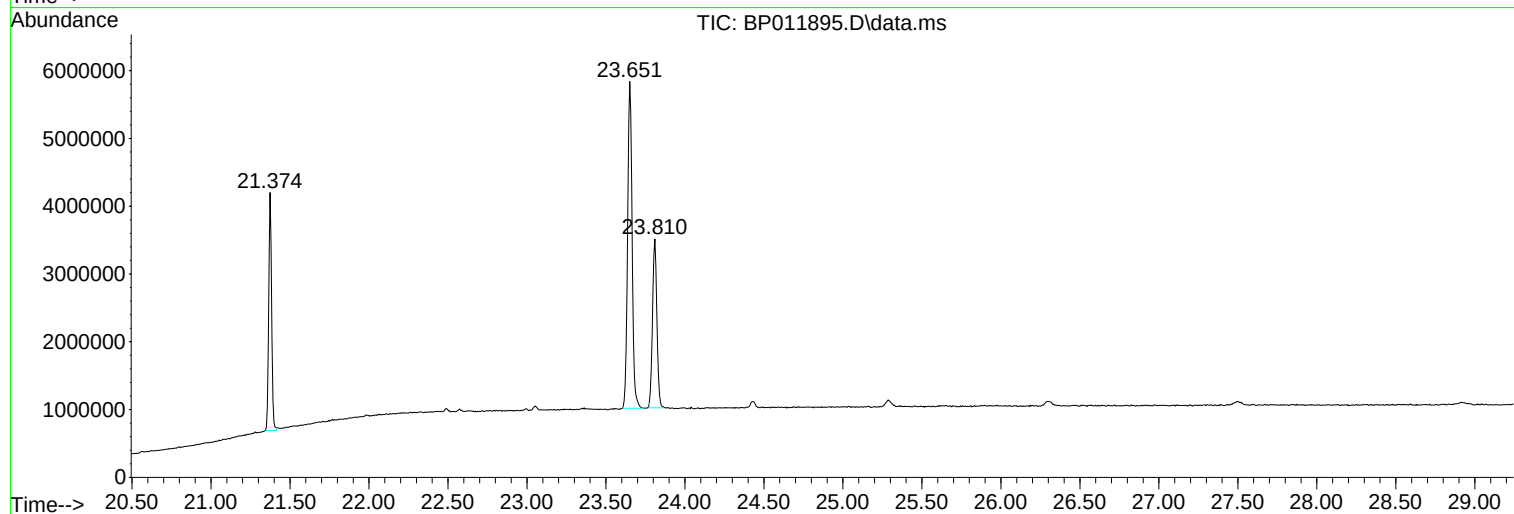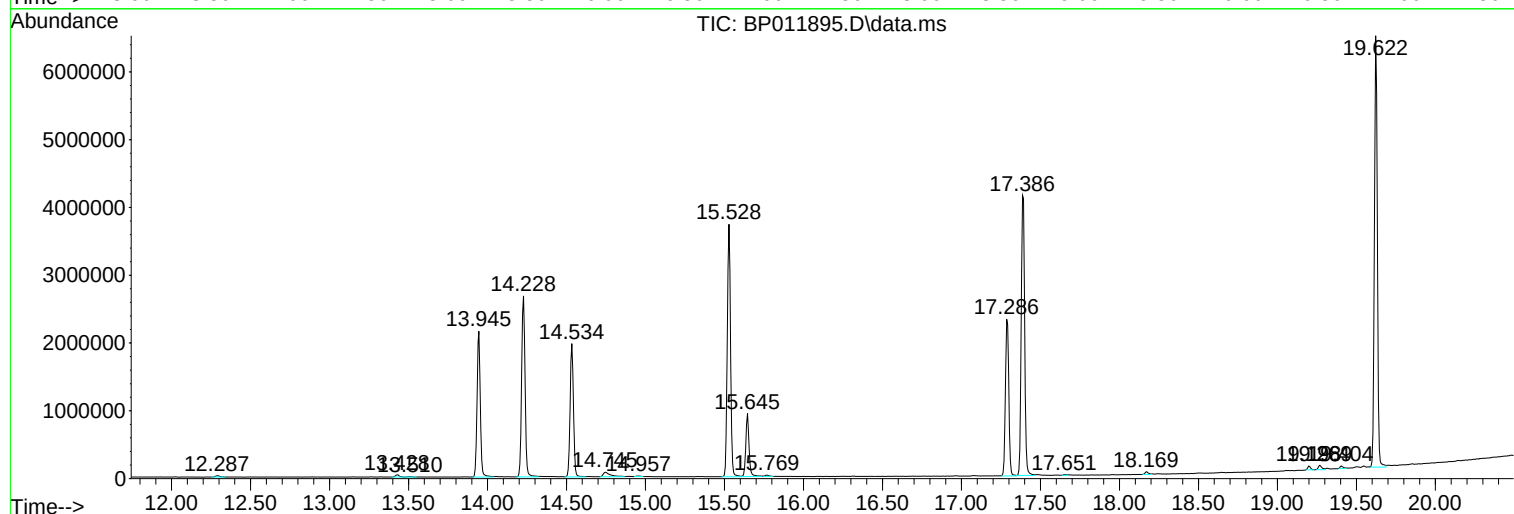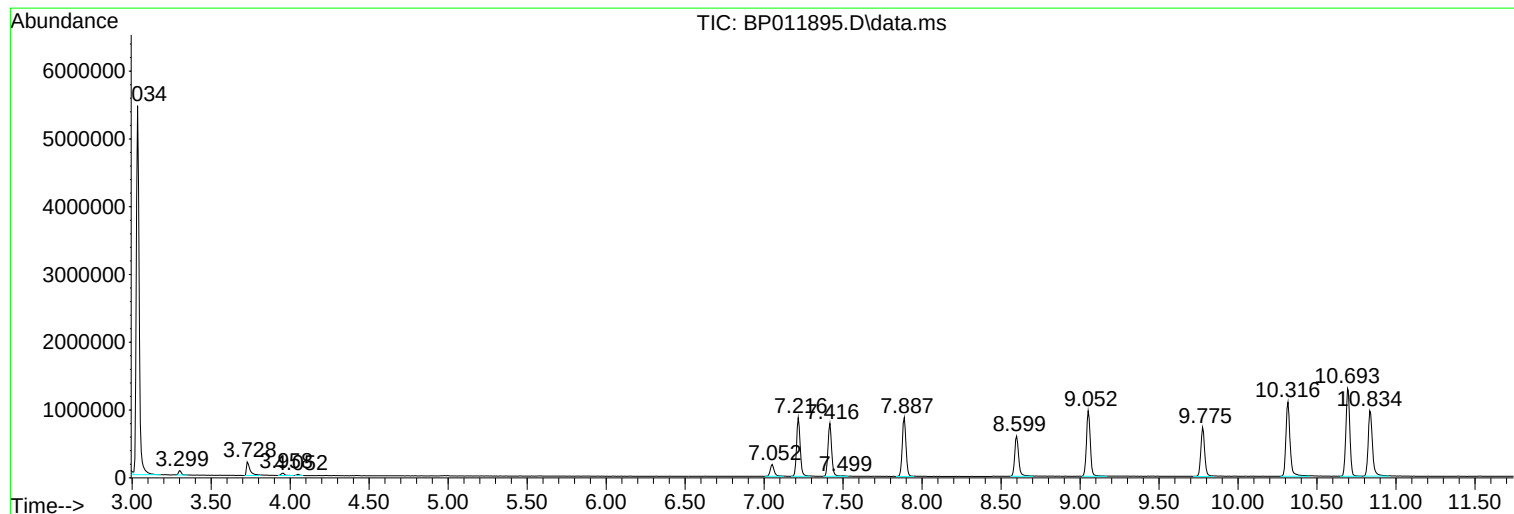

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011895.D
Acq On : 04 Oct 2022 04:44
Operator : CG/JU
Sample : N4859-11
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10051










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.034	96.28 ng/ul	6798280	1,4-Dichlorobenzene-d4	7.887

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78		
2	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	64		
3	2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40		
4	Pentane, 3-methoxy-	102	C6H14O	036839-67-5	12		
5	Silane, tetramethyl-	88	C4H12Si	000075-76-3	9		

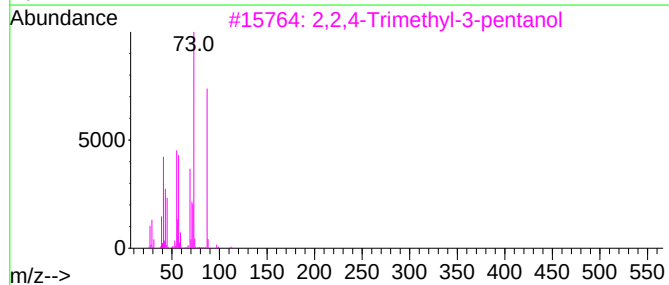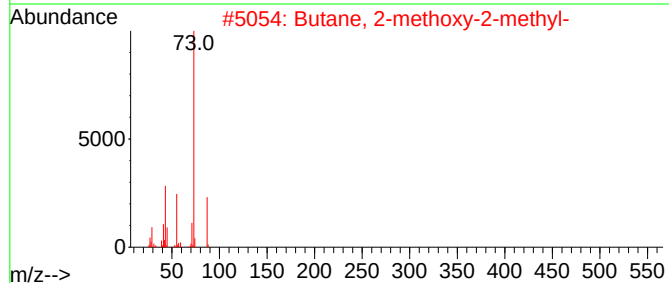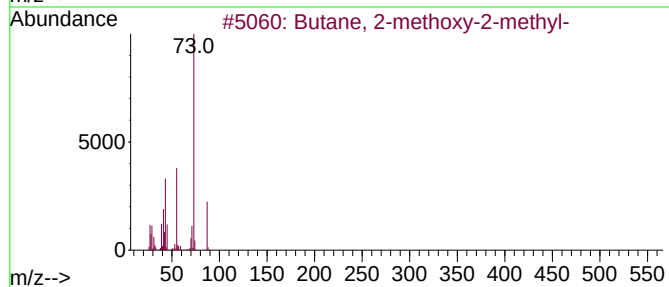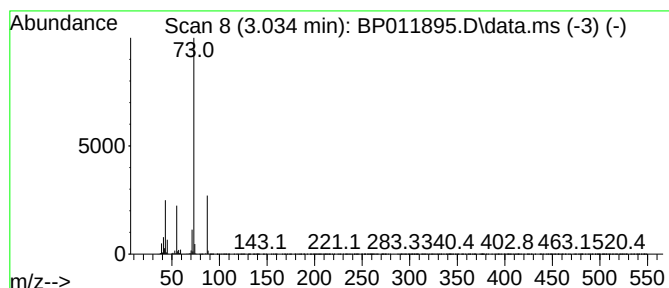

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011895.D
Acq On : 04 Oct 2022 04:44
Operator : CG/JU
Sample : N4859-11
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10051

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.034	96.3	ng/u1	6798280	1	7.887	1412220	20.0