

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
 Data File : BP011897.D
 Acq On : 04 Oct 2022 05:52
 Operator : CG/JU
 Sample : N4859-15
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E10047

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011897.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	3	8	31	rVB	4331650	5346155	66.44%	7.990%
2	3.299	50	53	61	rVB	51554	65731	0.82%	0.098%
3	3.734	125	127	141	rBV	121847	197403	2.45%	0.295%
4	3.952	160	164	170	rVB	27106	39348	0.49%	0.059%
5	4.052	176	181	186	rBV	21678	28577	0.36%	0.043%
6	4.987	335	340	346	rBV	36747	55945	0.70%	0.084%
7	7.052	683	691	702	rBV	171957	298945	3.71%	0.447%
8	7.217	711	719	731	rBV	807670	1291988	16.06%	1.931%
9	7.417	746	753	763	rBV	733252	1188897	14.77%	1.777%
10	7.887	825	833	841	rBV	785379	1268268	15.76%	1.895%
11	8.599	947	954	966	rBV	549841	916405	11.39%	1.370%
12	9.052	1024	1031	1047	rBV	865239	1467374	18.23%	2.193%
13	9.463	1095	1101	1107	rVB3	10800	17608	0.22%	0.026%
14	9.775	1142	1154	1169	rBV	674785	1135362	14.11%	1.697%
15	10.316	1238	1246	1267	rBV	999017	1794881	22.30%	2.682%
16	10.693	1303	1310	1322	rBV	1073921	1866513	23.19%	2.789%
17	10.834	1327	1334	1349	rBV	825827	1495346	18.58%	2.235%
18	11.522	1446	1451	1453	rBV6	4795	8696	0.11%	0.013%
19	12.287	1575	1581	1592	rVB2	22333	41730	0.52%	0.062%
20	13.351	1758	1762	1769	rVB	11489	14951	0.19%	0.022%
21	13.428	1771	1775	1780	rVB5	7472	9909	0.12%	0.015%
22	13.946	1856	1863	1878	rBV	1989418	2973873	36.96%	4.444%
23	14.228	1901	1911	1928	rBV	2508963	3844266	47.77%	5.745%
24	14.534	1956	1963	1976	rBV	1712143	2509783	31.19%	3.751%
25	14.740	1992	1998	2012	rBV	86398	222585	2.77%	0.333%
26	14.951	2028	2034	2042	rVB10	10300	20787	0.26%	0.031%
27	15.528	2124	2132	2145	rBV	3708484	5132776	63.78%	7.671%
28	15.645	2146	2152	2164	rVV	946512	1356752	16.86%	2.028%
29	15.769	2168	2173	2180	rVB3	17636	31881	0.40%	0.048%
30	16.098	2221	2229	2231	rBV9	4032	8882	0.11%	0.013%
31	16.692	2327	2330	2337	rBV7	5653	9939	0.12%	0.015%
32	17.287	2425	2431	2440	rBV	2121416	3057533	38.00%	4.569%
33	17.387	2442	2448	2463	rVV	3983942	5888324	73.17%	8.800%
34	18.169	2577	2581	2587	rBV	68776	99528	1.24%	0.149%
35	19.198	2753	2756	2762	rBV	53180	69684	0.87%	0.104%
36	19.269	2764	2768	2774	rBV	64440	114162	1.42%	0.171%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
 Data File : BP011897.D
 Acq On : 04 Oct 2022 05:52
 Operator : CG/JU
 Sample : N4859-15
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E10047

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

37	19.404	2788	2791	2795	rBV3	32992	41468	0.52%	0.062%
38	19.622	2823	2828	2835	rBV	5560949	7298837	90.70%	10.908%
39	21.080	3073	3076	3080	rBV	105062	137534	1.71%	0.206%
40	21.375	3121	3126	3135	rBV	2854072	3704903	46.04%	5.537%
41	23.651	3506	3513	3527	rVB2	3918429	8047090	100.00%	12.026%
42	23.810	3534	3540	3551	rVB2	1904173	3792230	47.13%	5.667%




Sum of corrected areas: 66912849

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011897.D
Acq On : 04 Oct 2022 05:52
Operator : CG/JU
Sample : N4859-15
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10047

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

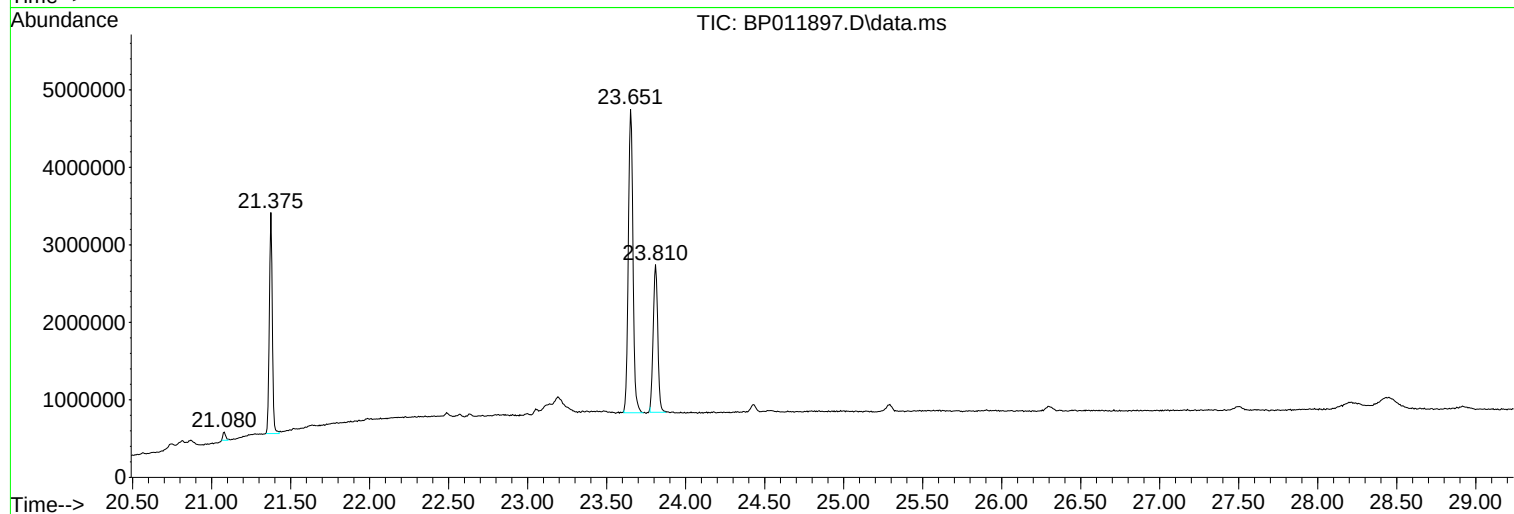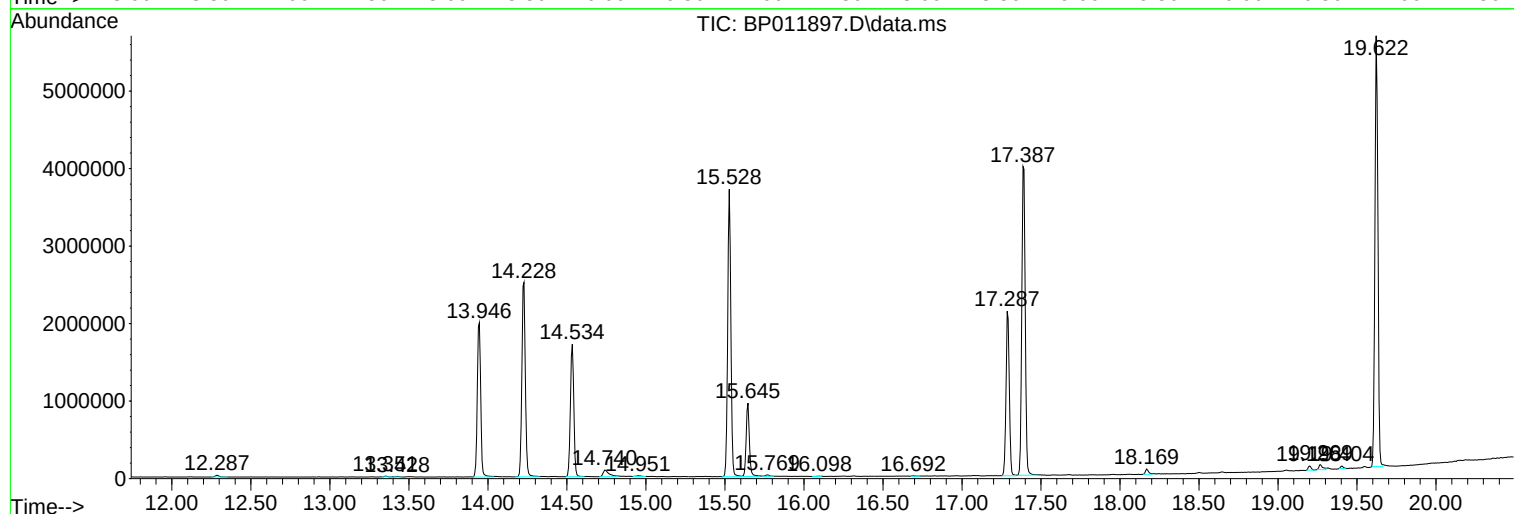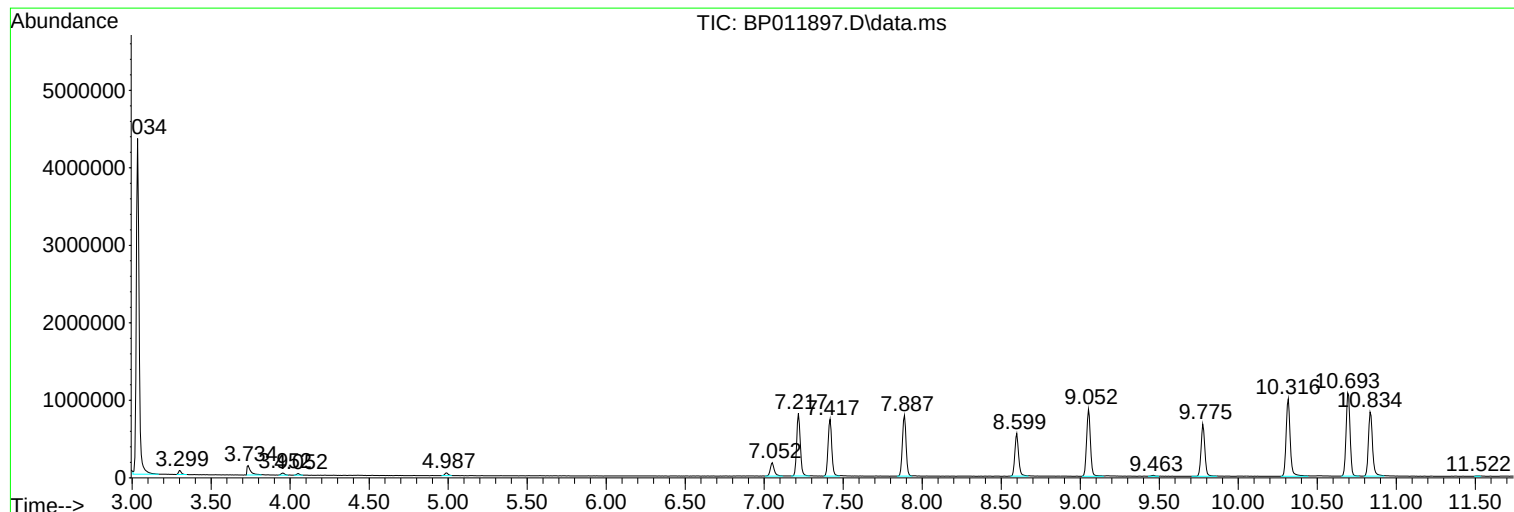

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011897.D
Acq On : 04 Oct 2022 05:52
Operator : CG/JU
Sample : N4859-15
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10047










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.034	84.31 ng/ul	5346160	1,4-Dichlorobenzene-d4	7.887

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	72
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	43
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9

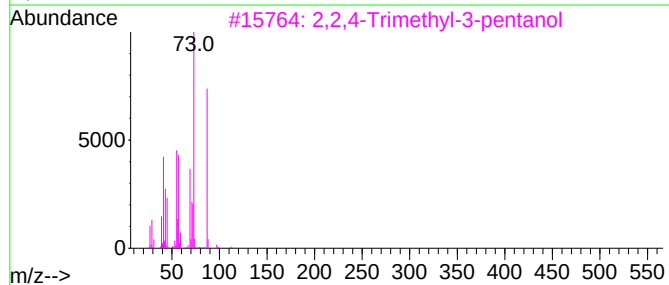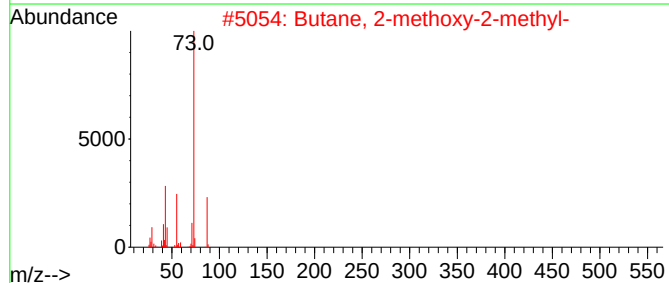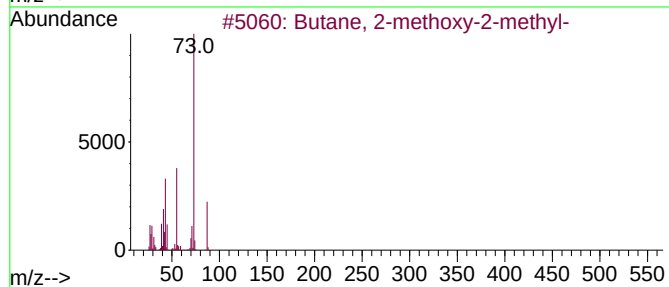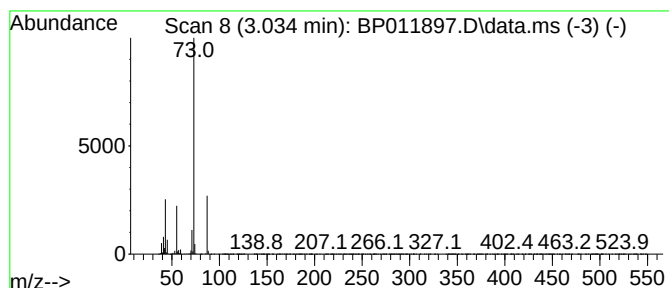

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011897.D
Acq On : 04 Oct 2022 05:52
Operator : CG/JU
Sample : N4859-15
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10047

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.034	84.3	ng/ul	5346160	1	7.887	1268270	20.0