

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
 Data File : BP011898.D
 Acq On : 04 Oct 2022 06:26
 Operator : CG/JU
 Sample : N4859-16
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E10048

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011898.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	3	8	29	rVB	4752354	5825671	73.10%	8.954%
2	3.299	50	53	58	rBV	43745	53340	0.67%	0.082%
3	3.734	126	127	141	rBV	71863	116305	1.46%	0.179%
4	3.952	160	164	169	rVB	29621	42197	0.53%	0.065%
5	4.052	177	181	184	rBV	19424	26158	0.33%	0.040%
6	4.987	335	340	349	rVB2	26436	41194	0.52%	0.063%
7	7.052	682	691	709	rVB	220842	384053	4.82%	0.590%
8	7.216	712	719	731	rBV	838511	1335342	16.76%	2.052%
9	7.416	745	753	764	rBV	767333	1261523	15.83%	1.939%
10	7.887	826	833	842	rBV	805529	1294721	16.25%	1.990%
11	8.599	946	954	968	rBV	668118	1136706	14.26%	1.747%
12	9.052	1023	1031	1045	rBV	887091	1493701	18.74%	2.296%
13	9.775	1146	1154	1167	rBV	652765	1124015	14.10%	1.728%
14	10.316	1238	1246	1264	rBV	992400	1772869	22.25%	2.725%
15	10.699	1302	1311	1325	rVB	1055384	1852294	23.24%	2.847%
16	10.834	1327	1334	1350	rBV	739914	1391393	17.46%	2.139%
17	11.522	1445	1451	1454	rBV6	6413	11265	0.14%	0.017%
18	12.287	1575	1581	1590	rBV3	19381	38786	0.49%	0.060%
19	13.434	1771	1776	1779	rVB4	5796	8674	0.11%	0.013%
20	13.945	1855	1863	1881	rBV	2043177	2905848	36.46%	4.466%
21	14.228	1904	1911	1923	rBV	2395646	3599083	45.16%	5.532%
22	14.534	1955	1963	1977	rBV	1611908	2348717	29.47%	3.610%
23	14.740	1992	1998	2015	rBV2	86736	244670	3.07%	0.376%
24	14.957	2030	2035	2041	rBV10	11606	22330	0.28%	0.034%
25	15.528	2125	2132	2144	rBV	3347326	4829734	60.60%	7.423%
26	15.645	2146	2152	2168	rVV	889481	1280453	16.07%	1.968%
27	15.769	2169	2173	2180	rVB2	15571	27272	0.34%	0.042%
28	17.286	2425	2431	2442	rBV	1891718	2780609	34.89%	4.274%
29	17.386	2442	2448	2464	rVV	3648591	5423537	68.05%	8.336%
30	18.169	2578	2581	2586	rBV4	26507	41934	0.53%	0.064%
31	18.645	2659	2662	2666	rBV5	14922	25133	0.32%	0.039%
32	19.204	2753	2757	2763	rVB3	47926	62483	0.78%	0.096%
33	19.269	2764	2768	2773	rBV	63158	93023	1.17%	0.143%
34	19.622	2823	2828	2841	rBV	5213621	7071453	88.73%	10.869%
35	21.375	3121	3126	3133	rBV	2759678	3499223	43.91%	5.378%
36	23.651	3506	3513	3529	rVB2	3778554	7969490	100.00%	12.249%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011898.D
Acq On : 04 Oct 2022 06:26
Operator : CG/JU
Sample : N4859-16
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10048

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Title : SVOA CALIBRATION

37 23.810 3534 3540 3551 rVB2 1779543 3627428 45.52% 5.575%




Sum of corrected areas: 65062627

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011898.D
Acq On : 04 Oct 2022 06:26
Operator : CG/JU
Sample : N4859-16
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10048

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

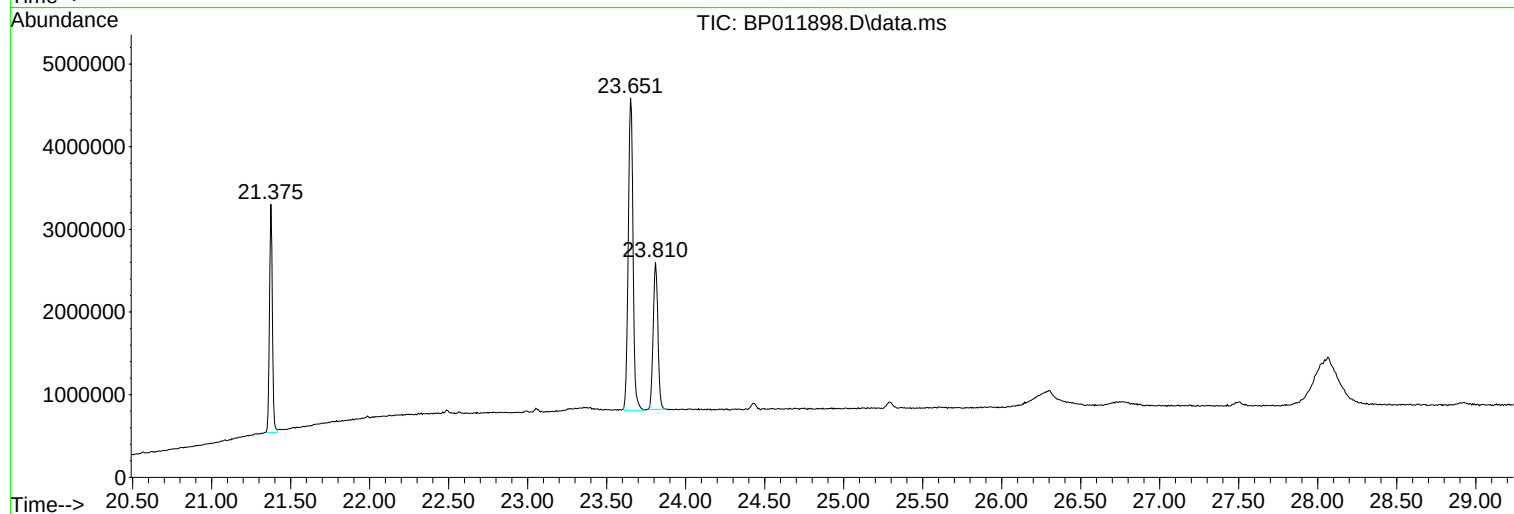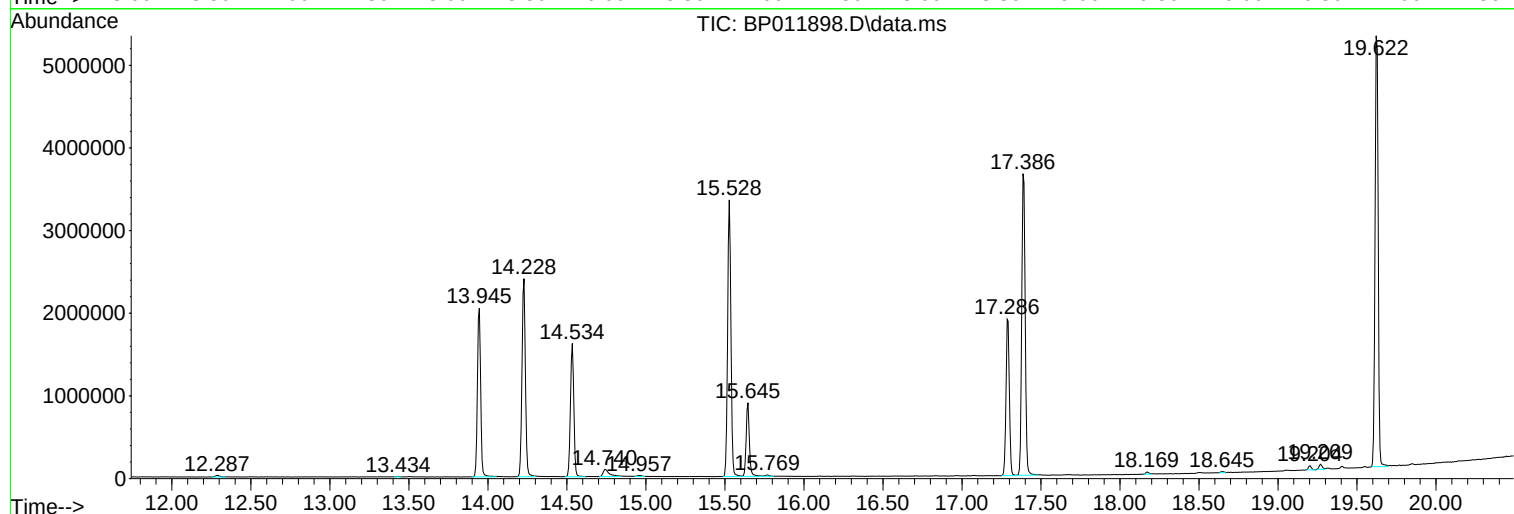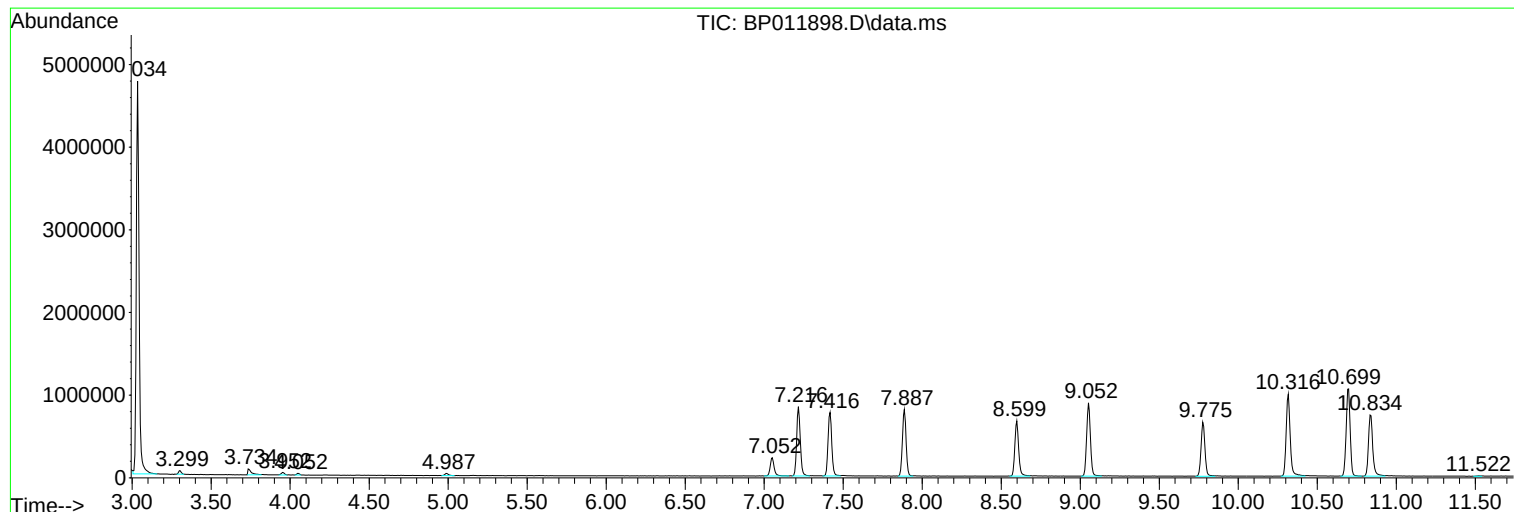

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011898.D
Acq On : 04 Oct 2022 06:26
Operator : CG/JU
Sample : N4859-16
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10048










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.034	89.99 ng/ul	5825670	1,4-Dichlorobenzene-d4	7.887

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	86		
2	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78		
3	2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	43		
4	Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17		
5	Silane, tetramethyl-	88	C4H12Si	000075-76-3	9		

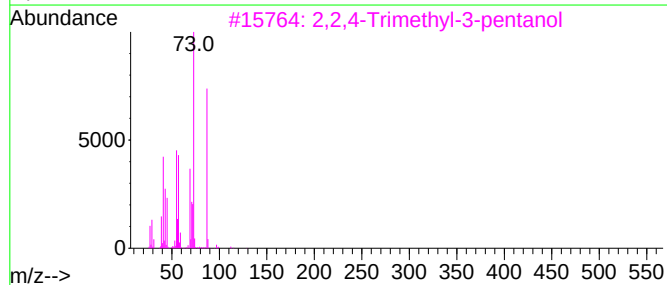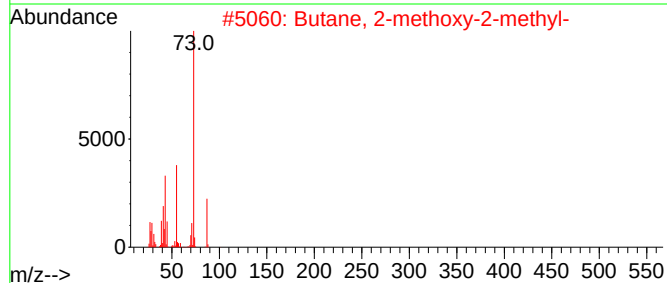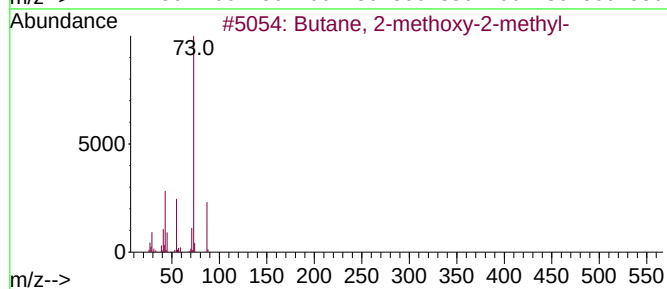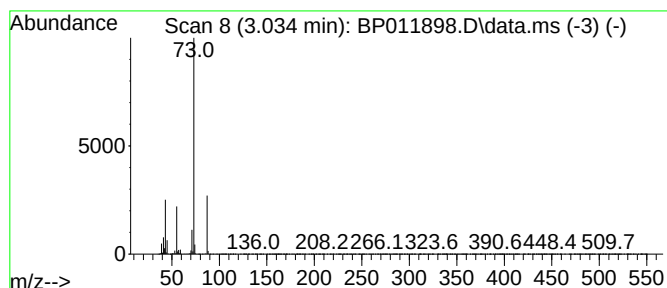

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011898.D
Acq On : 04 Oct 2022 06:26
Operator : CG/JU
Sample : N4859-16
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10048

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.034	90.0	ng/ul	5825670	1	7.887	1294720	20.0