

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
 Data File : BP011899.D
 Acq On : 04 Oct 2022 07:01
 Operator : CG/JU
 Sample : N4859-17
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E10053

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011899.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	3	8	33	rVB	4605314	5667515	76.00%	8.671%
2	3.270	45	48	50	rBV3	11316	12499	0.17%	0.019%
3	3.299	50	53	60	rVB	52616	66281	0.89%	0.101%
4	3.734	125	127	139	rBV	130143	214424	2.88%	0.328%
5	3.952	159	164	170	rBV	27776	41596	0.56%	0.064%
6	4.052	176	181	186	rBV	20343	30454	0.41%	0.047%
7	4.987	335	340	346	rVB2	15864	26850	0.36%	0.041%
8	6.299	557	563	569	rBV5	4730	8594	0.12%	0.013%
9	7.052	681	691	702	rBV	241689	428979	5.75%	0.656%
10	7.216	712	719	736	rBV	820508	1319180	17.69%	2.018%
11	7.416	745	753	764	rBV	745212	1210213	16.23%	1.851%
12	7.887	826	833	842	rBV	818219	1338133	17.94%	2.047%
13	8.599	945	954	968	rBV	618513	1047961	14.05%	1.603%
14	9.052	1024	1031	1041	rBV	878930	1476778	19.80%	2.259%
15	9.175	1047	1052	1057	rVB6	4618	8075	0.11%	0.012%
16	9.457	1094	1100	1106	rBV2	14405	29153	0.39%	0.045%
17	9.775	1146	1154	1168	rBV	658656	1114426	14.94%	1.705%
18	10.316	1238	1246	1269	rBV	987010	1787618	23.97%	2.735%
19	10.504	1272	1278	1290	rVB5	10141	35968	0.48%	0.055%
20	10.693	1301	1310	1322	rBV	1157741	1967074	26.38%	3.009%
21	10.834	1327	1334	1357	rVV	644905	1208416	16.20%	1.849%
22	11.516	1445	1450	1458	rVB	4712	12594	0.17%	0.019%
23	12.116	1548	1552	1557	rVB5	5937	9608	0.13%	0.015%
24	12.287	1575	1581	1590	rBV3	20728	37661	0.51%	0.058%
25	13.351	1752	1762	1769	rVV2	20696	42486	0.57%	0.065%
26	13.428	1769	1775	1781	rVV4	17405	32109	0.43%	0.049%
27	13.504	1781	1788	1796	rVB8	5175	13843	0.19%	0.021%
28	13.945	1856	1863	1877	rBV	2037870	2954912	39.63%	4.521%
29	14.228	1903	1911	1923	rBV	2513726	3736318	50.10%	5.716%
30	14.422	1942	1944	1950	rVB4	7331	10808	0.14%	0.017%
31	14.534	1954	1963	1978	rBV	1800140	2634985	35.34%	4.031%
32	14.745	1992	1999	2011	rBV	79567	210828	2.83%	0.323%
33	14.957	2029	2035	2040	rVB9	9983	20532	0.28%	0.031%
34	15.381	2104	2107	2112	rVB3	6955	9394	0.13%	0.014%
35	15.528	2125	2132	2146	rBV	3514447	4968530	66.63%	7.601%
36	15.645	2146	2152	2168	rVV	930020	1287088	17.26%	1.969%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
 Data File : BP011899.D
 Acq On : 04 Oct 2022 07:01
 Operator : CG/JU
 Sample : N4859-17
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E10053

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

37	15.769	2169	2173	2180	rVB3	16057	28366	0.38%	0.043%
38	16.322	2262	2267	2271	rVB8	5416	8598	0.12%	0.013%
39	16.828	2350	2353	2357	rBV3	6924	8975	0.12%	0.014%
40	16.969	2373	2377	2380	rBV6	4807	7788	0.10%	0.012%
41	17.292	2425	2432	2442	rBV	2221377	3157749	42.35%	4.831%
42	17.392	2442	2449	2459	rBV	3439047	4966283	66.60%	7.598%
43	17.645	2489	2492	2494	rBV3	10319	12332	0.17%	0.019%
44	17.957	2542	2545	2550	rVB4	12790	15748	0.21%	0.024%
45	18.169	2577	2581	2589	rBV	82702	128369	1.72%	0.196%
46	18.498	2634	2637	2644	rBV2	23489	37850	0.51%	0.058%
47	18.645	2658	2662	2667	rBV2	34791	57997	0.78%	0.089%
48	19.204	2753	2757	2762	rBV2	50669	70644	0.95%	0.108%
49	19.269	2764	2768	2773	rBV	83386	131831	1.77%	0.202%
50	19.404	2788	2791	2795	rBV4	40172	54178	0.73%	0.083%
51	19.628	2823	2829	2835	rBV	4780127	6488216	87.01%	9.926%
52	21.080	3073	3076	3081	rBV3	113597	172507	2.31%	0.264%
53	21.374	3121	3126	3135	rBV	2809337	3718023	49.86%	5.688%
54	23.651	3506	3513	3529	rVB	3653989	7457103	100.00%	11.408%
55	23.810	3534	3540	3552	rVB2	1900103	3820523	51.23%	5.845%




Sum of corrected areas: 65364963

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011899.D
Acq On : 04 Oct 2022 07:01
Operator : CG/JU
Sample : N4859-17
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10053

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

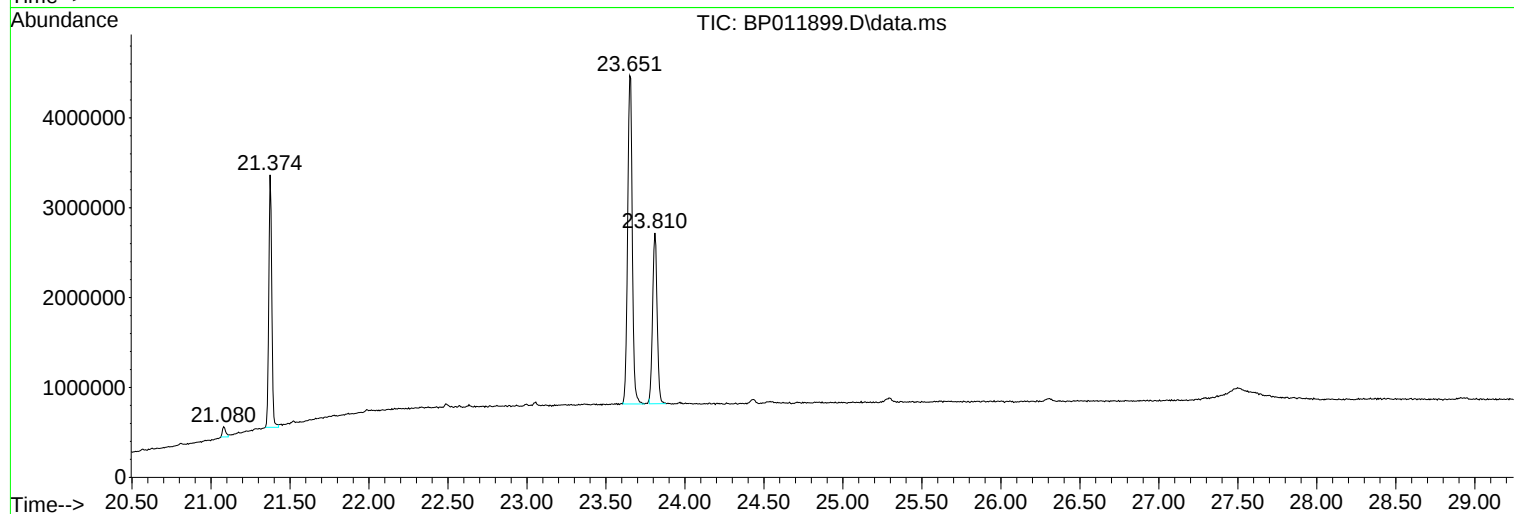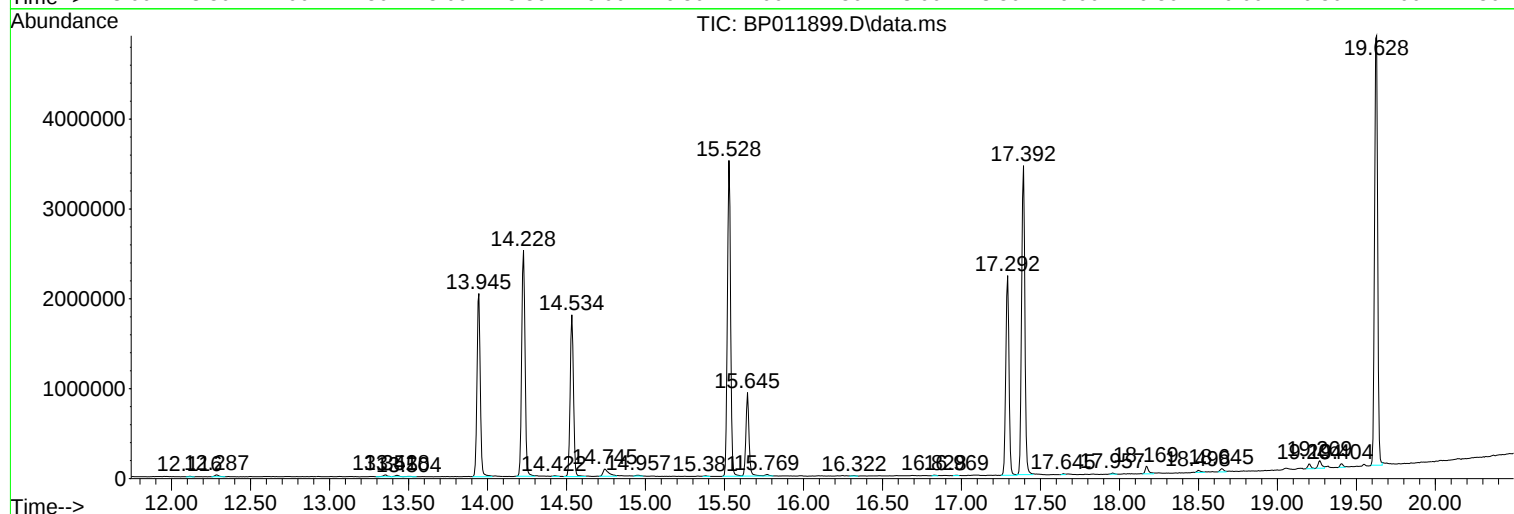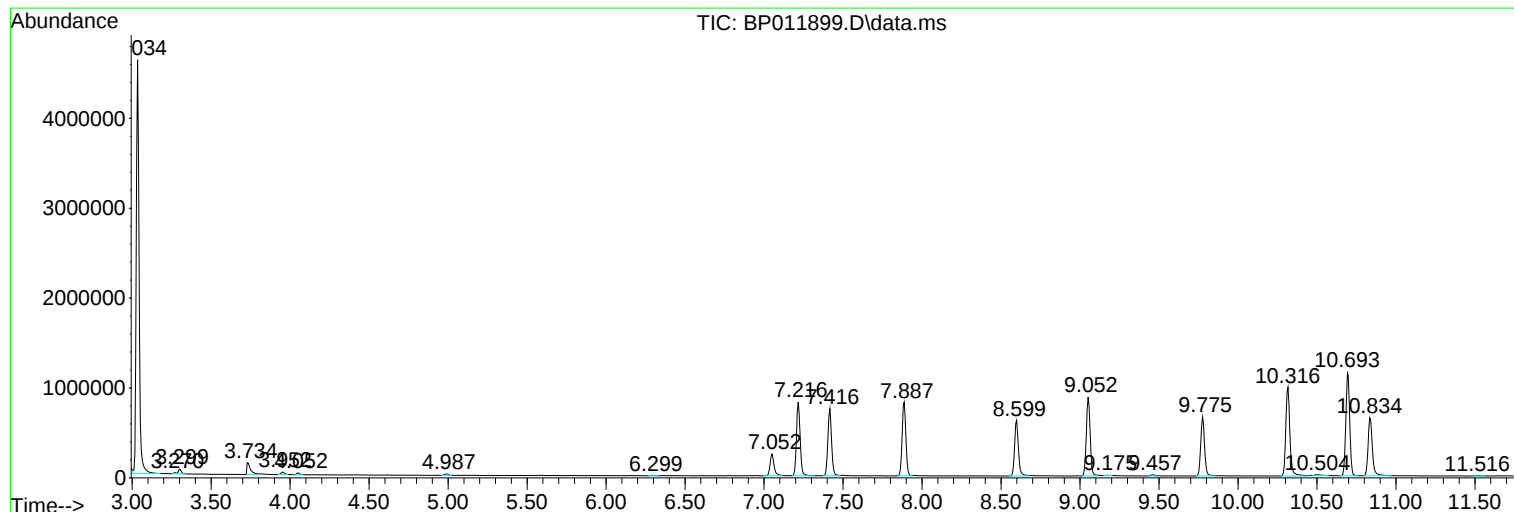

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011899.D
Acq On : 04 Oct 2022 07:01
Operator : CG/JU
Sample : N4859-17
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10053










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.034	84.71 ng/ul	5667520	1,4-Dichlorobenzene-d4	7.887

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78		
2	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	72		
3	2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	43		
4	Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17		
5	N-Ethylformamide	73	C3H7NO	000627-45-2	9		

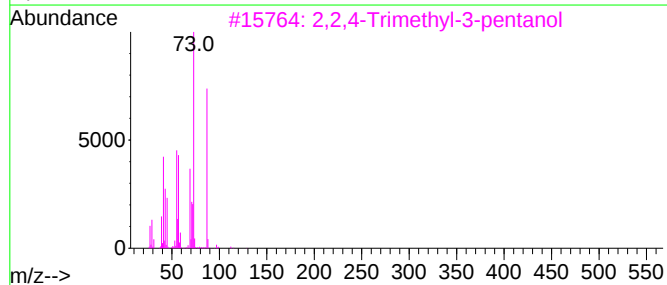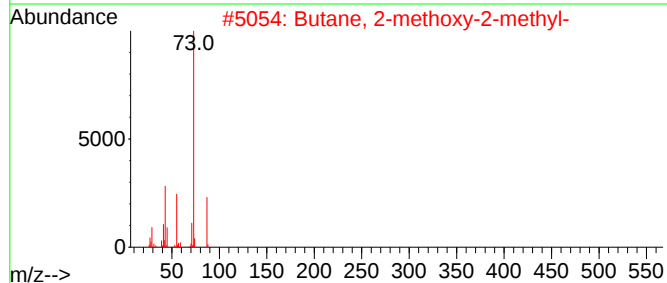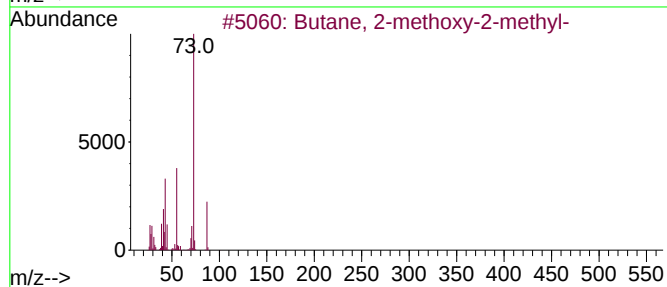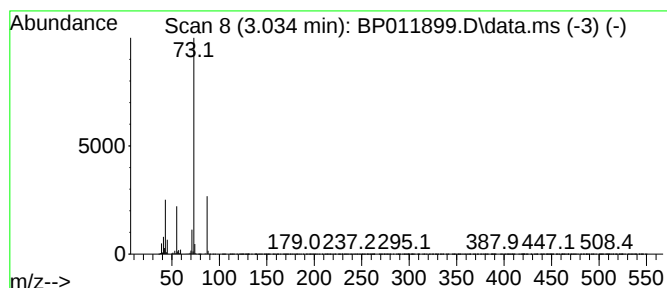

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011899.D
Acq On : 04 Oct 2022 07:01
Operator : CG/JU
Sample : N4859-17
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E10053

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.034	84.7	ng/ul	5667520	1	7.887	1338130	20.0