

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
 Data File : BP011908.D
 Acq On : 04 Oct 2022 12:43
 Operator : CG/JU
 Sample : N4873-09
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXZ55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011908.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	3	8	26	rVB	5369107	6672099	96.09%	10.450%
2	3.299	50	53	57	rVV	55012	66821	0.96%	0.105%
3	3.334	57	59	66	rVB	26100	33319	0.48%	0.052%
4	3.728	123	126	147	rBV	209169	336401	4.84%	0.527%
5	3.952	159	164	171	rVB	33692	49024	0.71%	0.077%
6	4.046	177	180	185	rBV	20146	26305	0.38%	0.041%
7	4.581	266	271	277	rVB6	12448	20413	0.29%	0.032%
8	4.987	335	340	349	rVB2	40265	65856	0.95%	0.103%
9	7.046	685	690	703	rBV	176426	305006	4.39%	0.478%
10	7.216	712	719	733	rBV	806918	1300175	18.72%	2.036%
11	7.416	746	753	764	rBV	734994	1197834	17.25%	1.876%
12	7.887	823	833	848	rBV	831547	1369211	19.72%	2.144%
13	8.599	946	954	972	rBV	531917	938532	13.52%	1.470%
14	9.052	1022	1031	1043	rBV	857026	1429646	20.59%	2.239%
15	9.775	1145	1154	1169	rBV	607073	1055358	15.20%	1.653%
16	10.316	1238	1246	1266	rBV	924900	1693720	24.39%	2.653%
17	10.693	1302	1310	1320	rBV	1146415	1945312	28.02%	3.047%
18	10.834	1326	1334	1351	rBV	893891	1652698	23.80%	2.588%
19	12.281	1575	1580	1591	rBV3	16586	36464	0.53%	0.057%
20	13.428	1768	1775	1783	rBV3	18136	28618	0.41%	0.045%
21	13.940	1856	1862	1881	rBV	1833879	2710081	39.03%	4.245%
22	14.228	1899	1911	1922	rBV	2217989	3417627	49.22%	5.353%
23	14.534	1955	1963	1976	rBV	1619079	2488250	35.83%	3.897%
24	14.745	1991	1999	2016	rBV	66935	212435	3.06%	0.333%
25	14.945	2031	2033	2040	rVB8	6571	12071	0.17%	0.019%
26	15.528	2124	2132	2145	rBV	3126571	4557359	65.63%	7.138%
27	15.645	2145	2152	2166	rVV	773477	1136453	16.37%	1.780%
28	15.769	2169	2173	2180	rVB3	15118	26431	0.38%	0.041%
29	17.286	2425	2431	2442	rBV	2038120	2940613	42.35%	4.606%
30	17.386	2442	2448	2462	rVV	3556767	5167542	74.42%	8.094%
31	17.957	2542	2545	2550	rBV6	10680	12498	0.18%	0.020%
32	18.145	2573	2577	2578	rBV3	12561	14472	0.21%	0.023%
33	18.169	2578	2581	2586	rVB2	32869	44092	0.63%	0.069%
34	19.198	2753	2756	2762	rVB2	41954	55075	0.79%	0.086%
35	19.269	2764	2768	2774	rBV	53103	83247	1.20%	0.130%
36	19.404	2788	2791	2795	rBV4	39611	53857	0.78%	0.084%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011908.D
Acq On : 04 Oct 2022 12:43
Operator : CG/JU
Sample : N4873-09
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXZ55

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Title : SVOA CALIBRATION

37	19.622	2823	2828	2843	rBV	4999353	6510814	93.76%	10.197%
38	21.374	3121	3126	3136	rBV	2744531	3585020	51.63%	5.615%
39	23.651	3507	3513	3527	rVB2	3534607	6943769	100.00%	10.875%
40	23.810	3534	3540	3553	rVB2	1772412	3653430	52.61%	5.722%




Sum of corrected areas: 63847948

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011908.D
Acq On : 04 Oct 2022 12:43
Operator : CG/JU
Sample : N4873-09
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXZ55

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

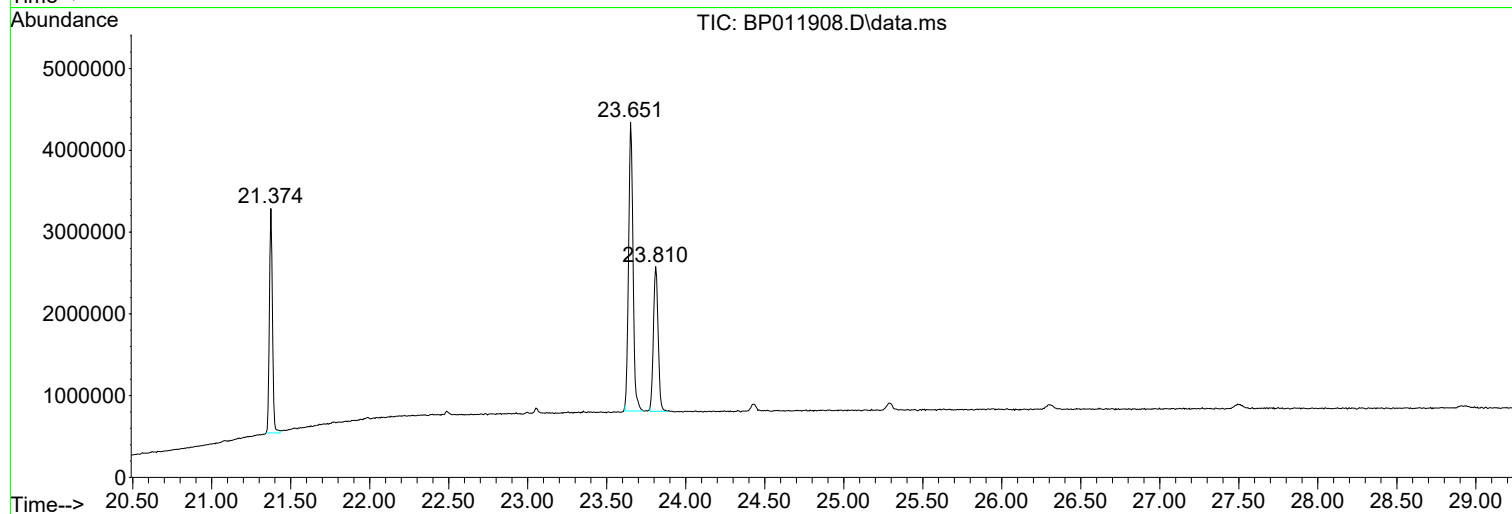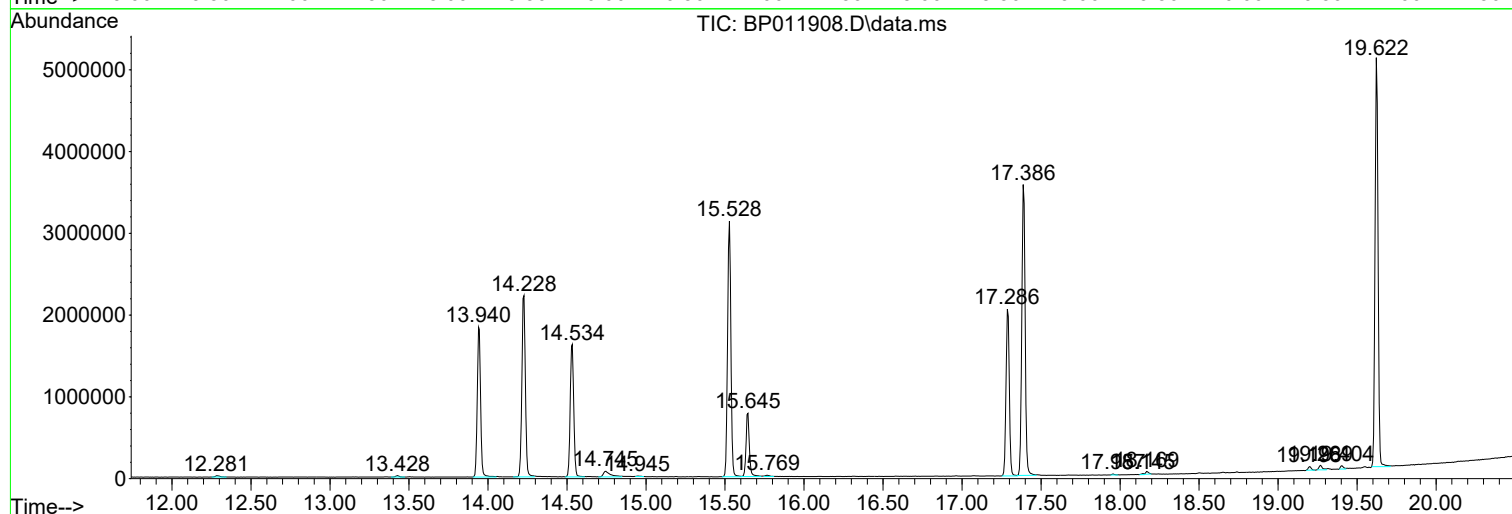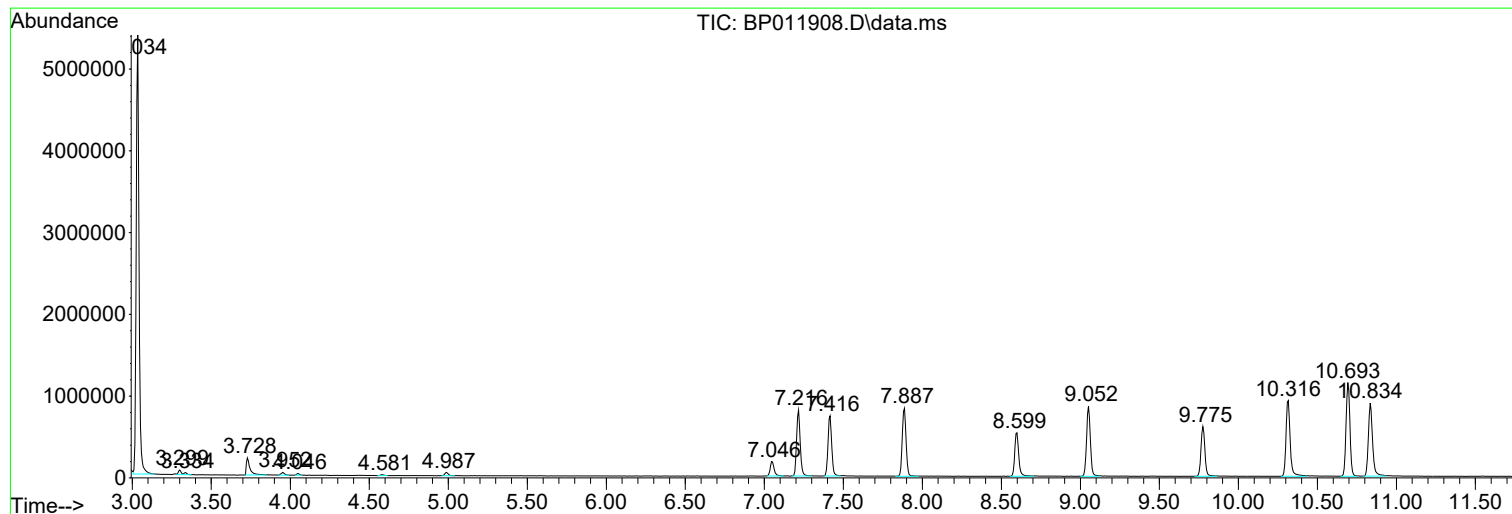

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011908.D
Acq On : 04 Oct 2022 12:43
Operator : CG/JU
Sample : N4873-09
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXZ55










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.034	97.46 ng/ul	6672100	1,4-Dichlorobenzene-d4	7.887

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	86
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	43
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9

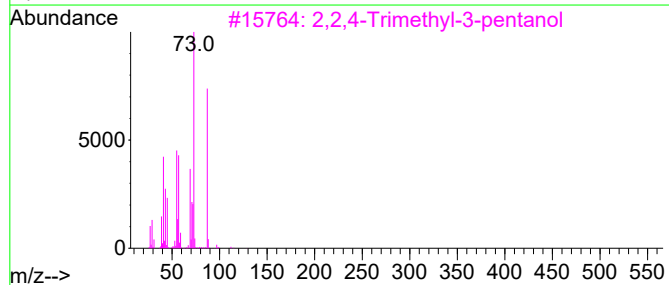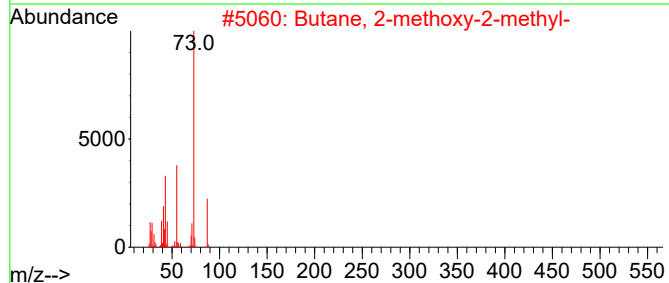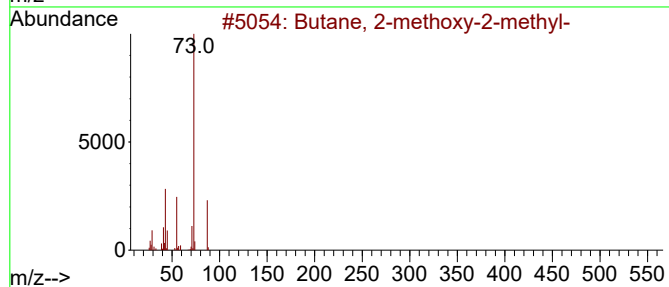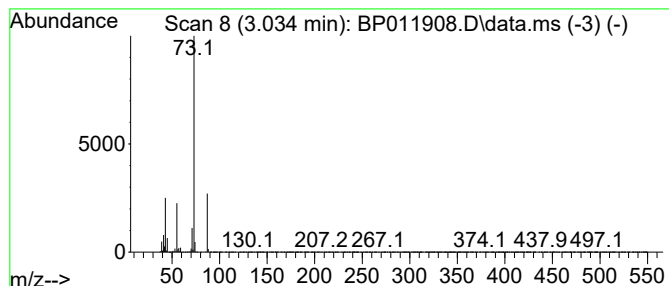

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011908.D
Acq On : 04 Oct 2022 12:43
Operator : CG/JU
Sample : N4873-09
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXZ55

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.034	97.5	ng/ul	6672100	1	7.887	1369210	20.0