

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
 Data File : BP011909.D
 Acq On : 04 Oct 2022 13:17
 Operator : CG/JU
 Sample : N4873-10
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXZ56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011909.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	3	8	31	rVB	3615731	4472362	68.11%	7.770%
2	3.299	50	53	63	rVB	45923	59256	0.90%	0.103%
3	3.746	128	129	138	rBV	25562	44439	0.68%	0.077%
4	3.952	160	164	172	rVB	21465	32939	0.50%	0.057%
5	4.046	177	180	188	rVB	32030	45891	0.70%	0.080%
6	5.517	425	430	438	rVB3	9503	18338	0.28%	0.032%
7	7.052	684	691	703	rBV	142470	255681	3.89%	0.444%
8	7.216	712	719	732	rBV	684975	1118303	17.03%	1.943%
9	7.416	744	753	764	rBV	627163	1042235	15.87%	1.811%
10	7.887	825	833	844	rBV	775766	1281048	19.51%	2.226%
11	8.599	946	954	968	rBV	460067	824879	12.56%	1.433%
12	9.052	1023	1031	1043	rBV	743061	1249757	19.03%	2.171%
13	9.216	1054	1059	1065	rVB5	10746	17250	0.26%	0.030%
14	9.775	1147	1154	1170	rBV	541736	924771	14.08%	1.607%
15	10.316	1236	1246	1268	rBV	800349	1538125	23.42%	2.672%
16	10.693	1302	1310	1327	rBV	1115742	1924437	29.31%	3.344%
17	10.840	1327	1335	1350	rBV	189307	392751	5.98%	0.682%
18	12.287	1574	1581	1588	rBV2	15267	36045	0.55%	0.063%
19	13.428	1768	1775	1781	rBV8	7189	13699	0.21%	0.024%
20	13.510	1787	1789	1799	rVB8	4246	6652	0.10%	0.012%
21	13.940	1855	1862	1878	rBV	1725373	2501503	38.10%	4.346%
22	14.228	1901	1911	1933	rBV	2047793	3113281	47.41%	5.409%
23	14.534	1955	1963	1972	rBV	1704536	2563349	39.04%	4.454%
24	14.745	1991	1999	2018	rBV	57425	194563	2.96%	0.338%
25	14.957	2030	2035	2042	rVB9	7333	15986	0.24%	0.028%
26	15.528	2124	2132	2145	rBV	2968513	4281869	65.21%	7.439%
27	15.645	2145	2152	2167	rVV	771936	1130032	17.21%	1.963%
28	15.769	2169	2173	2179	rVB2	13837	24783	0.38%	0.043%
29	15.892	2191	2194	2200	rVB2	7277	11014	0.17%	0.019%
30	17.081	2392	2396	2401	rVB4	5281	9742	0.15%	0.017%
31	17.286	2425	2431	2442	rBV	2045062	3016748	45.94%	5.241%
32	17.386	2442	2448	2462	rBV	3607522	5226613	79.60%	9.081%
33	17.957	2542	2545	2548	rVB4	9953	10349	0.16%	0.018%
34	18.169	2577	2581	2589	rBV3	62956	95770	1.46%	0.166%
35	19.198	2753	2756	2762	rBV2	41322	57587	0.88%	0.100%
36	19.269	2764	2768	2771	rBV	57236	81713	1.24%	0.142%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011909.D
Acq On : 04 Oct 2022 13:17
Operator : CG/JU
Sample : N4873-10
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXZ56

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Title : SVOA CALIBRATION

37	19.404	2788	2791	2796	rBV4	63872	89457	1.36%	0.155%
38	19.622	2822	2828	2839	rBV	4605149	6349742	96.70%	11.032%
39	21.374	3121	3126	3136	rBV	2746945	3466655	52.79%	6.023%
40	23.651	3506	3513	3528	rVB2	3115585	6566340	100.00%	11.408%
41	23.810	3534	3540	3552	rVB2	1708915	3451605	52.57%	5.997%




Sum of corrected areas: 57557559

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011909.D
Acq On : 04 Oct 2022 13:17
Operator : CG/JU
Sample : N4873-10
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXZ56

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

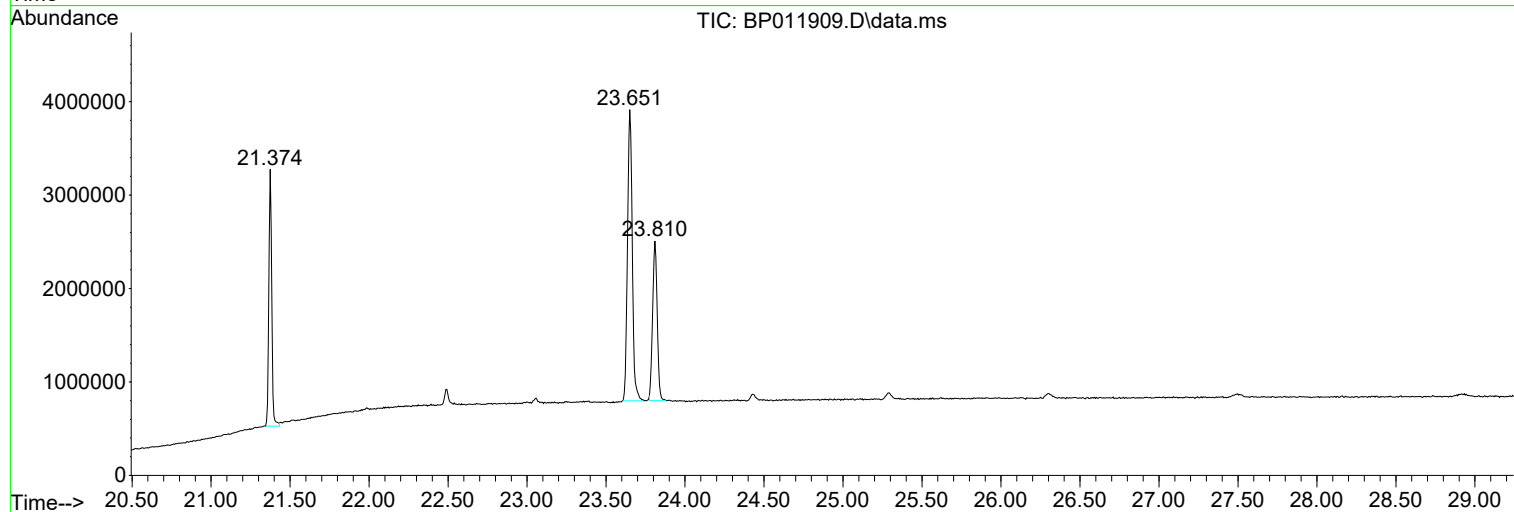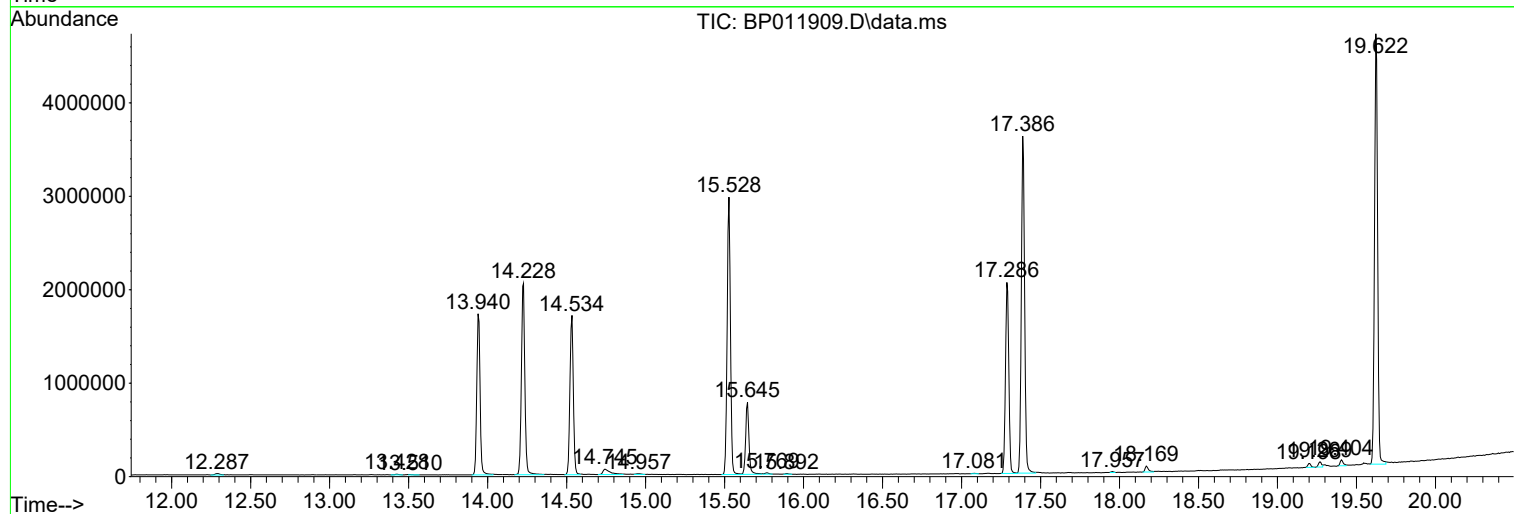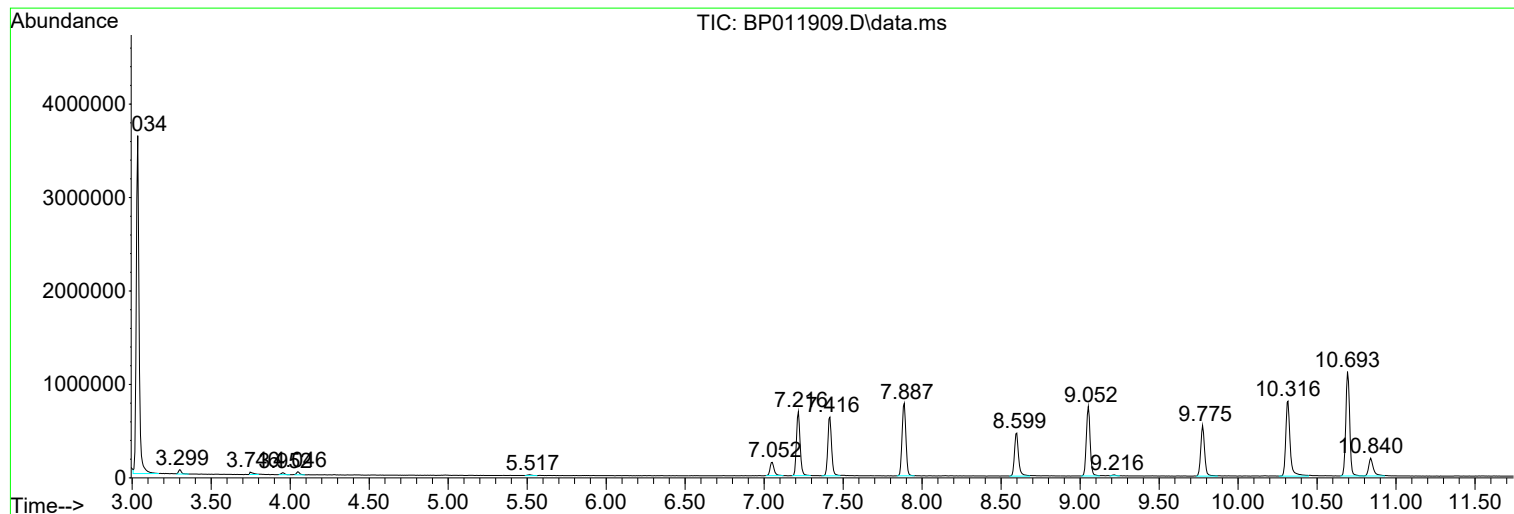

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011909.D
Acq On : 04 Oct 2022 13:17
Operator : CG/JU
Sample : N4873-10
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXZ56










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.034	69.82 ng/ul	4472360	1,4-Dichlorobenzene-d4	7.887

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	72
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	43
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9

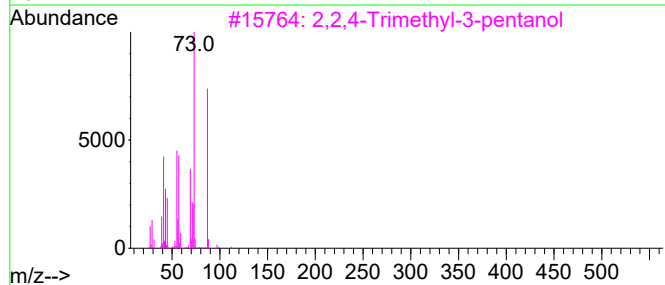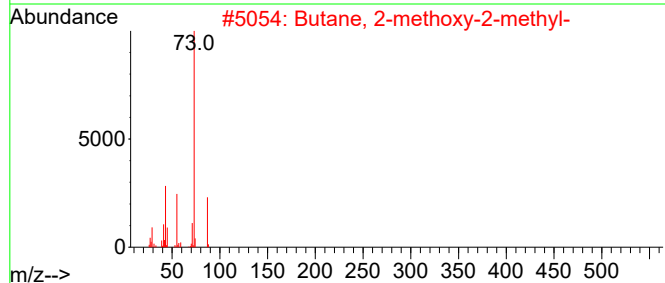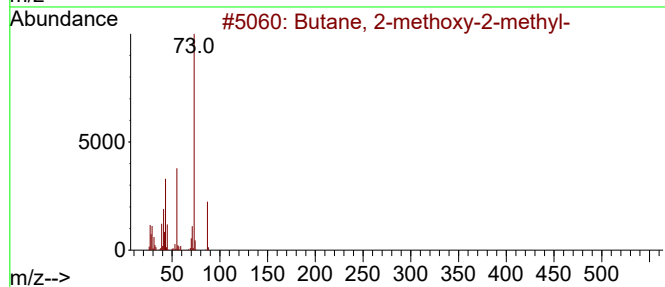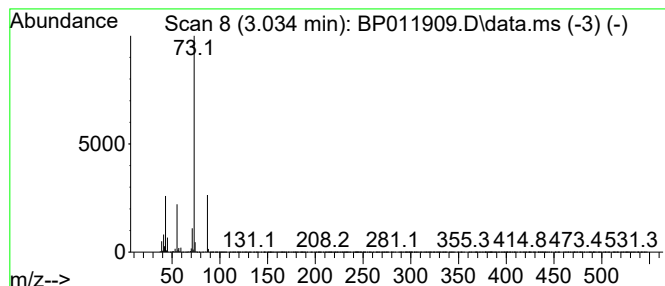

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP100322\
Data File : BP011909.D
Acq On : 04 Oct 2022 13:17
Operator : CG/JU
Sample : N4873-10
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXZ56

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP093022.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.034	69.8	ng/ul	4472360	1	7.887	1281050	20.0